


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051123\
Data File : VU054149.D
Acq On : 11 May 2023 08:58
Operator : JC/MD
Sample : BFB190
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB190

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis
Last Update : Sat May 06 01:14:00 2023

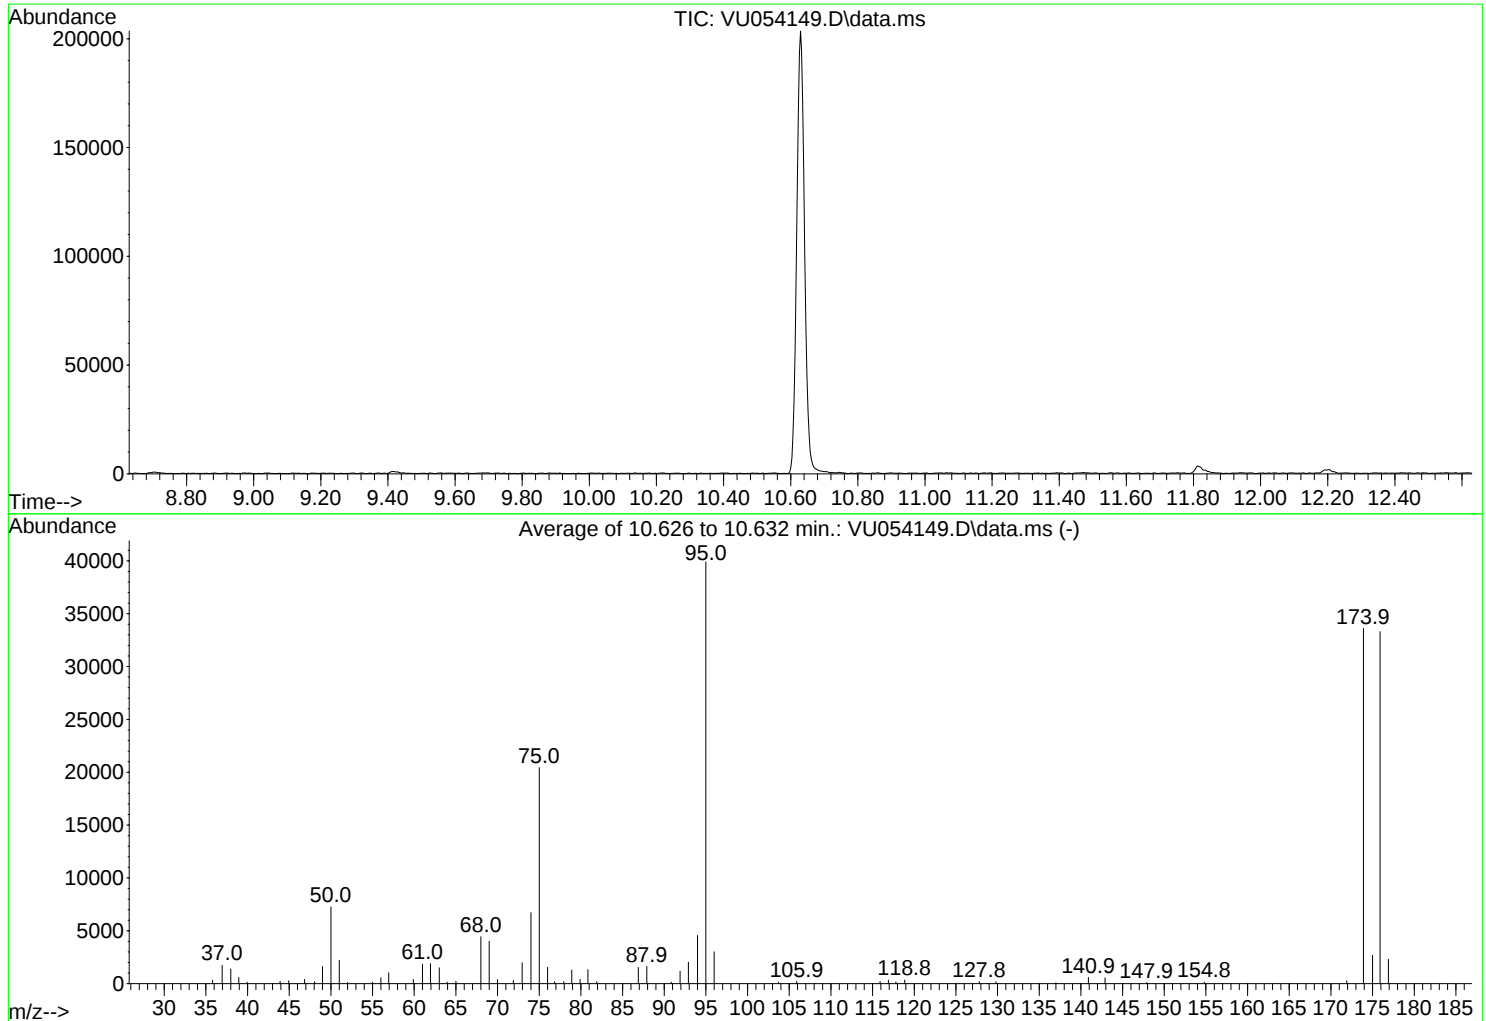

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	7256	PASS
75	95	30	80	51.2	20443	PASS
95	95	100	100	100.0	39907	PASS
96	95	5	9	7.6	3018	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.2	33600	PASS
175	174	5	9	8.0	2682	PASS
176	174	95	101	99.1	33309	PASS
177	176	5	9	6.9	2298	PASS

m/z	Abundance
43.90	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
35.80	340.0
37.00	1645.0
38.00	1275.0
39.00	637.0
40.00	147.0
43.90	404.0
45.00	288.0
46.90	427.0
48.10	155.0
49.00	1472.0
50.00	7538.0
51.00	2325.0
52.00	109.0
55.00	144.0
56.00	481.0
57.00	959.0
59.90	377.0
61.00	1914.0
61.90	1811.0
63.00	1429.0
63.90	175.0
65.00	216.0
68.00	4223.0
69.00	4100.0
70.00	299.0
71.90	302.0
72.90	2134.0
74.00	6542.0
75.00	20056.0
76.00	1587.0
76.90	172.0
78.00	137.0
78.90	1447.0
79.90	398.0
80.80	1399.0
81.80	186.0
86.90	1376.0
87.90	1453.0
90.80	120.0
91.90	1145.0
92.90	2055.0
94.00	4450.0
95.00	40200.0
96.00	3135.0
103.70	106.0
105.90	173.0
115.90	191.0
116.90	323.0
117.80	151.0
118.90	305.0
127.70	192.0
129.90	163.0
140.90	547.0
142.90	517.0
147.90	188.0
154.80	118.0
171.90	201.0
173.90	32328.0
175.00	2744.0
175.90	31664.0
176.90	2244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
35.80	332.0
37.00	1812.0
38.00	1382.0
39.00	585.0
40.00	140.0
43.90	445.0
44.90	261.0
46.90	392.0
48.00	170.0
49.00	1707.0
50.00	7514.0
51.00	2307.0
52.00	129.0
55.00	159.0
56.00	578.0
56.90	1065.0
59.90	417.0
61.00	1889.0
62.00	1960.0
63.00	1513.0
63.90	149.0
65.00	229.0
68.00	4684.0
69.00	4172.0
70.00	402.0
71.90	317.0
73.00	2045.0
74.00	6927.0
75.00	20992.0
76.00	1600.0
76.80	180.0
78.00	210.0
78.90	1315.0
79.90	433.0
80.90	1346.0
81.90	171.0
86.90	1579.0
87.90	1696.0
90.90	142.0
91.90	1214.0
92.90	2092.0
94.00	4723.0
95.00	41072.0
96.00	3141.0
103.70	148.0
105.90	208.0
115.90	206.0
116.90	369.0
117.80	183.0
118.80	368.0
127.80	189.0
129.80	176.0
137.00	117.0
140.90	598.0
142.90	555.0
147.90	140.0
154.80	170.0
171.90	288.0
173.90	34688.0
175.00	2768.0
175.90	34392.0
176.90	2364.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
35.80	276.0
36.90	1758.0
38.00	1513.0
38.90	509.0
39.90	102.0
44.00	438.0
44.90	249.0
46.80	357.0
48.00	208.0
49.00	1691.0
50.00	6715.0
51.00	2010.0
52.00	121.0
55.00	127.0
56.00	625.0
56.90	1059.0
59.90	391.0
61.00	1749.0
62.00	1901.0
63.00	1560.0
64.00	135.0
65.00	227.0
68.00	4407.0
69.00	3755.0
70.00	444.0
71.90	273.0
73.00	1782.0
74.00	6700.0
75.00	20280.0
76.00	1453.0
76.80	192.0
77.90	209.0
78.90	1118.0
79.90	413.0
80.80	1222.0
82.00	180.0
86.90	1633.0
87.90	1706.0
90.90	150.0
91.90	1172.0
92.90	1964.0
94.00	4511.0
95.00	38448.0
96.00	2779.0
103.70	176.0
105.90	237.0
115.90	198.0
116.90	322.0
117.80	176.0
118.80	394.0
127.90	179.0
128.70	115.0
129.70	199.0
137.00	132.0
140.90	592.0
142.90	567.0
154.80	184.0
171.90	379.0
173.90	33784.0
175.00	2535.0
175.90	33872.0
176.90	2286.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190