

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051219\
 Data File : VU031943.D
 Acq On : 12 May 2019 15:11
 Operator : JC/SP
 Sample : K2791-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9D37

Quant Time: May 13 07:29:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon May 13 07:00:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	466389	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	478218	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	164601	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	126813	3.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.80%
7) Chloroethane-d5	1.68	69	125546	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.27	63	183031	2.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.40%#
20) 2-Butanone-d5	4.18	46	525834	42.37	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.74%
24) Chloroform-d	4.64	84	283824	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.00%
26) 1,2-Dichloroethane-d4	5.31	65	160387	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
32) Benzene-d6	5.33	84	528782	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.40%
36) 1,2-Dichloropropane-d6	6.32	67	188678	4.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.00%
41) Toluene-d8	7.56	98	391484	3.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.80%
43) trans-1,3-Dichloropropene-	7.85	79	55624	3.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.60%
46) 2-Hexanone-d5	8.31	63	341699	42.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.66%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	164386	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	142482	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
47) Tetrachloroethene	8.22	164	18689	0.684 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051219\
Data File : VU031943.D
Acq On : 12 May 2019 15:11
Operator : JC/SP
Sample : K2791-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D37

Quant Time: May 13 07:29:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon May 13 07:00:03 2019
Response via : Initial Calibration

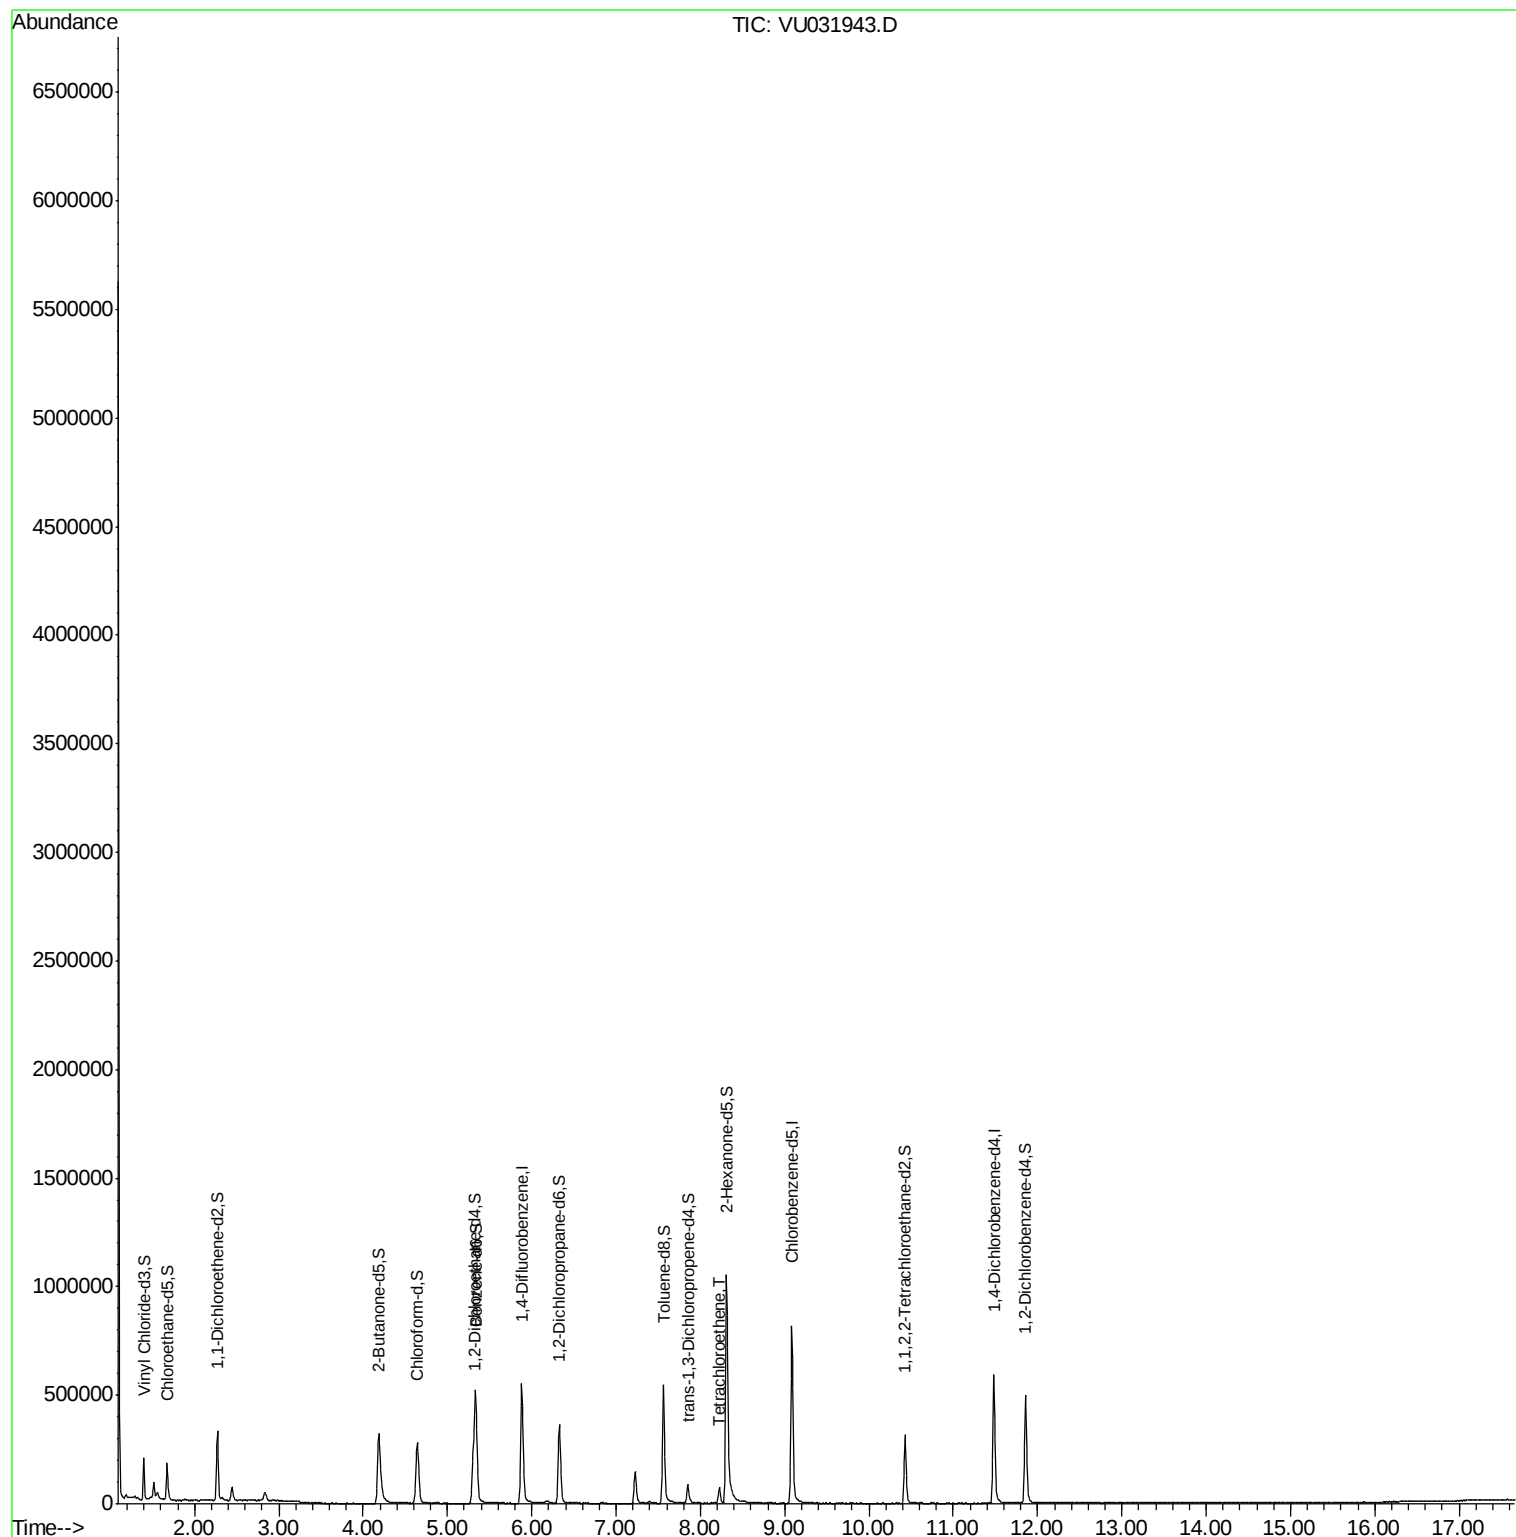

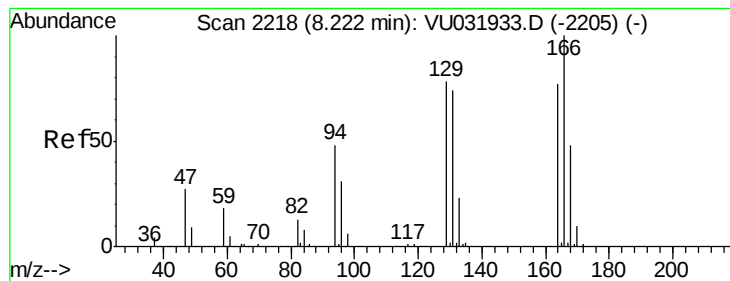

#47

Tetrachloroethene

Concen: 0.684 ug/L


RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU031943.D

Acq: 12 May 2019 15:11

Instrument :
MSVOA_U
ClientSampleId :
F9D37

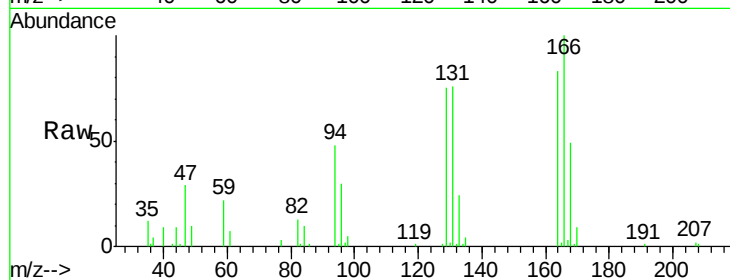

Tot Ion:164 Resp: 18689

Ion Ratio Lower Upper

164 100

129 90.7 70.3 130.5

131 91.4 65.4 121.4

166 120.9 86.0 159.8

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

