


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051219\
 Data File : VU031932.D
 Acq On : 12 May 2019 09:32
 Operator : JC/SP
 Sample : BFB06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon May 13 07:00:03 2019

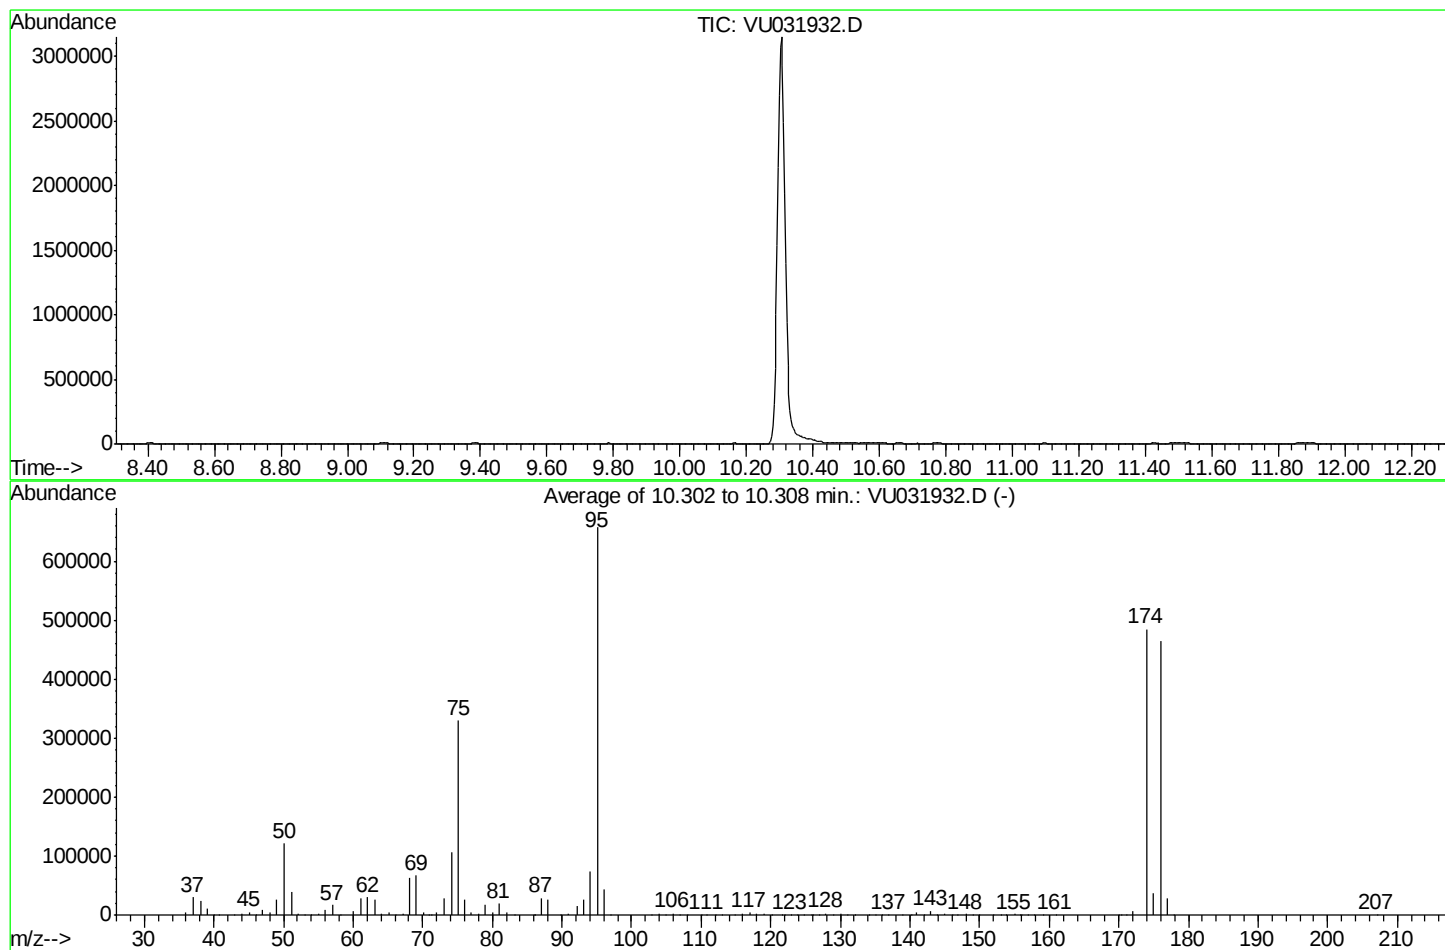

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	121098	PASS
75	95	30	80	50.1	329130	PASS
95	95	100	100	100.0	657472	PASS
96	95	5	9	6.6	43480	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.6	484181	PASS
175	174	5	9	7.7	37461	PASS
176	174	95	101	96.0	464938	PASS
177	176	5	9	6.3	29112	PASS

Scan 2850 (10.254 min): VU031932.D
BFB06

m/z	Abundance
39.90	1094.0
41.90	104.0
44.00	1216.0
78.10	111.0
207.30	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	4991.0
37.00	29864.0
38.10	25736.0
39.10	11703.0
40.00	1630.0
40.70	251.0
42.90	351.0
44.00	4390.0
45.00	5560.0
46.00	810.0
47.00	8409.0
48.00	4075.0
49.00	26608.0
50.10	124488.0
51.10	40128.0
52.00	1931.0
53.00	759.0
53.90	178.0
55.00	1731.0
56.00	9441.0
57.00	16848.0
58.10	777.0
60.00	6544.0
61.00	29120.0
62.10	30576.0
63.10	25952.0
64.10	3697.0
65.10	5745.0
66.00	719.0
67.10	2273.0
68.10	64656.0
69.10	66544.0
70.10	4699.0
71.20	190.0
72.10	3527.0
73.10	27984.0
74.10	108144.0
75.10	332544.0
76.10	27880.0
77.00	3535.0
78.00	3236.0
79.00	19032.0
80.00	4766.0
80.90	19168.0
82.00	3801.0
83.10	615.0
86.00	765.0
87.00	28640.0
88.00	27632.0
90.90	2089.0
92.10	15755.0
93.00	26904.0
94.10	75720.0
95.10	663232.0
96.10	45096.0
97.00	1139.0
102.90	451.0
103.90	2362.0
105.00	859.0
105.90	2395.0
106.90	726.0
108.10	299.0
110.00	332.0
110.80	453.0
112.00	463.0
112.90	443.0
114.90	634.0
116.00	2128.0
117.00	3957.0
118.00	2075.0
119.00	2956.0
120.10	189.0
121.70	145.0
122.90	185.0
123.90	407.0
124.70	171.0
125.80	144.0
126.90	334.0
128.00	2230.0
129.00	957.0
130.00	2011.0
130.90	865.0
132.00	219.0
134.10	121.0
135.00	820.0
136.00	386.0
136.90	844.0
139.00	228.0
141.00	5249.0
142.10	912.0
143.00	7746.0
144.10	533.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

145.00	2239.0
146.10	1190.0
146.80	419.0
148.00	1279.0
149.10	244.0
150.00	546.0
151.90	182.0
153.00	614.0
153.80	297.0
155.00	1374.0
156.00	254.0
157.00	1038.0
157.90	215.0
159.00	692.0
160.90	568.0
170.00	195.0
171.00	996.0
172.00	6308.0
174.00	474560.0
175.00	36072.0
176.00	459776.0
177.00	29656.0
177.90	750.0
207.00	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	5081.0
37.00	30936.0
38.10	25320.0
39.10	11183.0
39.90	1773.0
40.80	283.0
41.80	107.0
43.00	422.0
44.00	4214.0
45.10	5360.0
46.00	919.0
47.00	8280.0
48.00	4351.0
49.00	26400.0
50.10	125552.0
51.10	40240.0
52.10	1839.0
53.00	672.0
53.90	212.0
55.10	1543.0
56.00	9418.0
57.00	17664.0
58.10	863.0
60.00	6599.0
61.10	29328.0
62.10	31192.0
63.10	26288.0
64.10	3412.0
65.10	5490.0
66.10	737.0
67.10	2187.0
68.10	65712.0
69.10	69056.0
70.10	4785.0
70.90	122.0
71.20	149.0
72.00	3777.0
73.10	28968.0
74.10	109112.0
75.10	340352.0
76.10	26976.0
77.00	3532.0
78.00	3109.0
79.00	18424.0
80.00	4895.0
81.00	19104.0
82.00	4106.0
83.10	806.0
87.00	28752.0
88.00	27384.0
89.80	108.0
90.90	2076.0
92.10	16362.0
93.10	26392.0
94.10	76520.0
95.10	680064.0
96.10	44848.0
97.00	1212.0
102.90	451.0
104.00	2386.0
105.00	888.0
105.90	2559.0
106.90	585.0
108.10	236.0
109.90	395.0
110.80	506.0
112.00	429.0
112.90	487.0
114.80	730.0
116.00	2134.0
117.00	3729.0
118.00	1983.0
119.00	3147.0
120.10	152.0
121.70	157.0
122.90	215.0
123.90	531.0
124.80	151.0
126.10	157.0
127.00	307.0
128.00	2504.0
129.00	1012.0
130.00	1948.0
130.90	896.0
132.10	266.0
134.10	134.0
135.00	803.0
136.00	427.0
136.90	845.0
138.90	194.0
140.10	389.0
141.00	5244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

142.10	1047.0
143.00	7783.0
143.90	467.0
145.00	2209.0
146.10	994.0
146.80	437.0
148.00	1194.0
149.00	202.0
150.00	680.0
151.90	255.0
153.00	575.0
153.80	342.0
155.00	1300.0
156.10	168.0
157.00	1109.0
157.90	235.0
159.10	666.0
160.90	517.0
171.10	814.0
172.00	6292.0
174.00	501056.0
175.00	38896.0
176.00	479616.0
177.00	30000.0
177.90	825.0
207.00	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	4898.0
37.00	29240.0
38.10	23048.0
39.10	9894.0
39.90	1744.0
40.80	219.0
41.80	108.0
43.00	460.0
44.00	4004.0
45.10	4826.0
46.00	804.0
47.00	7511.0
48.00	3908.0
49.10	23800.0
50.10	113256.0
51.10	36216.0
52.10	1678.0
53.10	595.0
53.90	237.0
55.10	1178.0
56.00	8735.0
57.00	16760.0
58.10	829.0
60.00	6083.0
61.10	27032.0
62.10	28720.0
63.10	23752.0
64.10	2848.0
65.10	4437.0
66.10	669.0
67.10	1818.0
68.10	59800.0
69.10	64104.0
70.10	4503.0
70.90	125.0
72.00	3545.0
73.10	26808.0
74.10	98984.0
75.10	314496.0
76.10	24040.0
77.00	3386.0
78.00	2620.0
79.00	17000.0
80.00	4687.0
81.00	17928.0
82.00	4098.0
83.10	739.0
86.20	893.0
87.00	27392.0
88.00	24200.0
89.80	111.0
90.90	2020.0
92.10	15746.0
93.10	24360.0
94.10	70152.0
95.10	629120.0
96.10	40496.0
97.00	1168.0
102.90	338.0
104.00	2190.0
104.90	885.0
105.90	2422.0
106.90	495.0
108.00	233.0
109.90	436.0
110.90	576.0
112.00	351.0
112.90	405.0
114.80	779.0
115.90	1838.0
117.00	3242.0
118.00	1772.0
119.00	2934.0
121.90	149.0
122.90	139.0
123.90	490.0
124.90	168.0
126.00	155.0
127.00	200.0
127.90	2290.0
129.00	827.0
130.00	1666.0
130.90	840.0
132.10	203.0
134.10	157.0
135.00	735.0
136.00	285.0
136.90	755.0
138.90	127.0
140.10	427.0
141.00	4915.0
142.10	872.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

143.00	6961.0
143.90	387.0
145.00	2038.0
146.00	793.0
146.90	407.0
148.00	1096.0
148.90	194.0
150.00	543.0
151.90	253.0
153.00	435.0
153.80	355.0
155.00	1064.0
155.80	116.0
157.00	954.0
157.80	214.0
159.20	555.0
160.90	453.0
170.30	325.0
171.20	708.0
172.00	5900.0
174.00	476928.0
175.00	37416.0
176.00	455424.0
177.00	27680.0
178.00	788.0
207.10	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06