


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051221\
 Data File : VU043668.D
 Acq On : 12 May 2021 10:38
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
 Title : SW846 8260
 Last Update : Thu May 13 08:11:56 2021

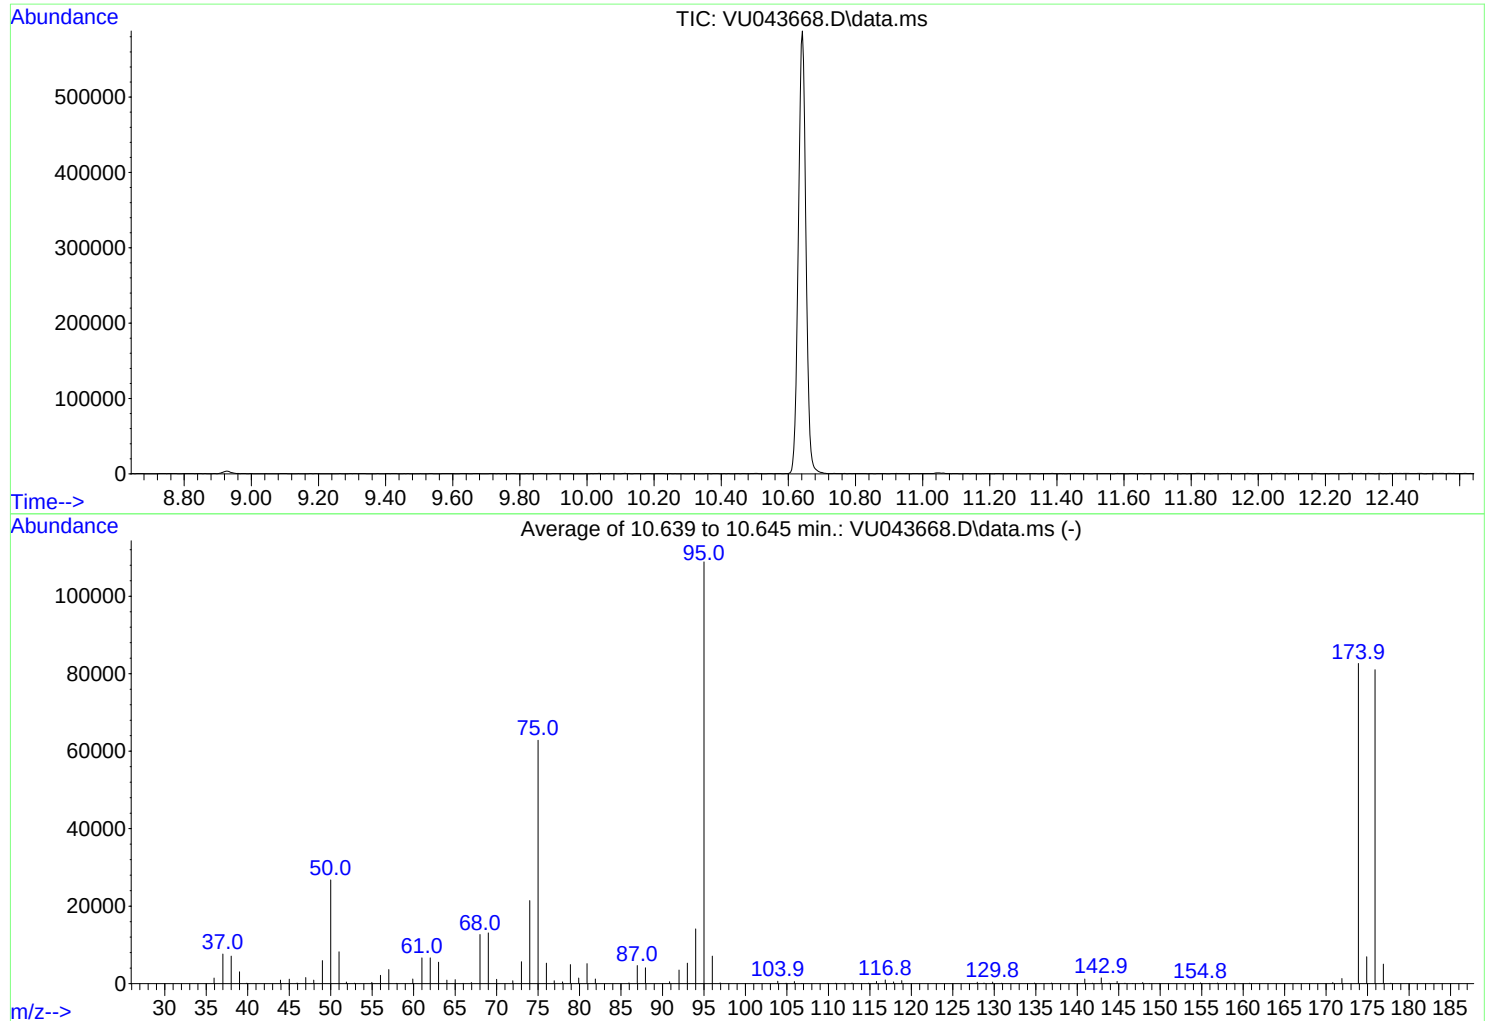

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	26752	PASS
75	95	30	60	57.7	62803	PASS
95	95	100	100	100.0	108875	PASS
96	95	5	9	6.5	7122	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.9	82627	PASS
175	174	5	9	8.4	6920	PASS
176	174	95	101	98.1	81040	PASS
177	176	5	9	6.2	5027	PASS