




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048533.D
Acq On : 12 May 2022 11:56
Operator : SY/MD
Sample : N2801-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLE0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/13/2022
Supervised By :Mahesh Dadoda 05/13/2022

Quant Time: May 13 03:57:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

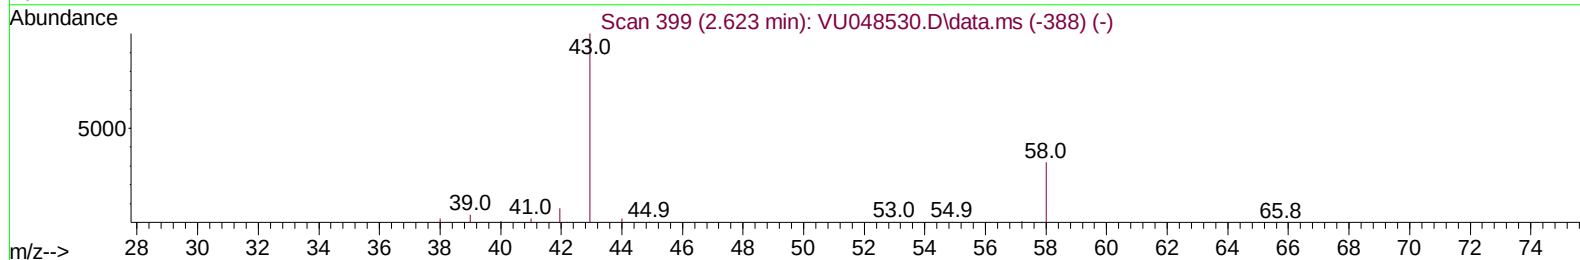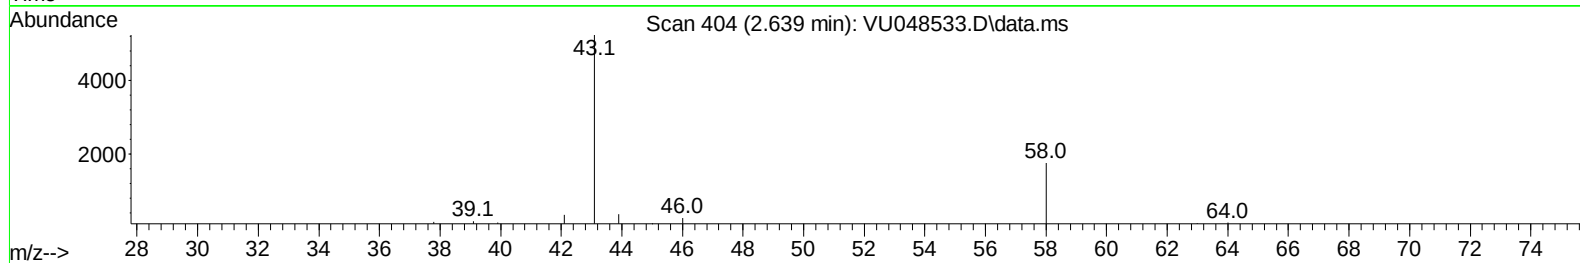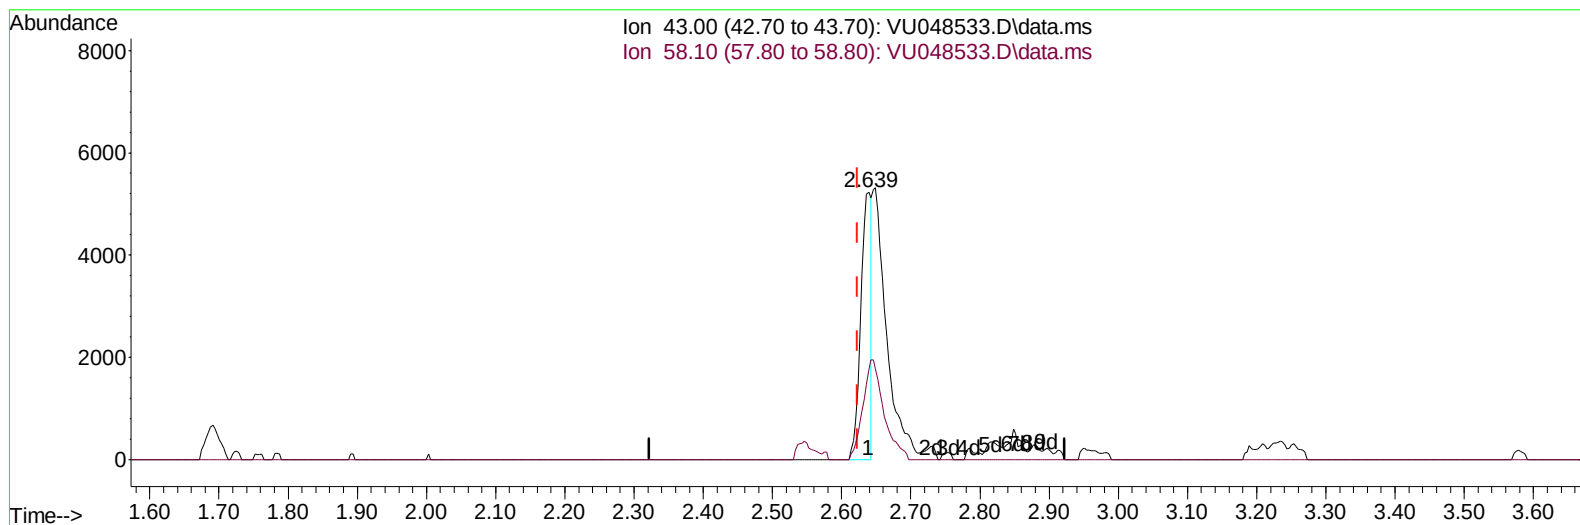

TIC: VU048533.D\data.ms

(13) Acetone (T)

2.639min (+ 0.017) 3.48 ug/L

response 5593

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.10	72.73#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048533.D
Acq On : 12 May 2022 11:56
Operator : SY/MD
Sample : N2801-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLE0

Manual IntegrationsAPPROVED

Quant Time: May 13 03:57:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/13/2022
Supervised By :Mahesh Dadoda 05/13/2022

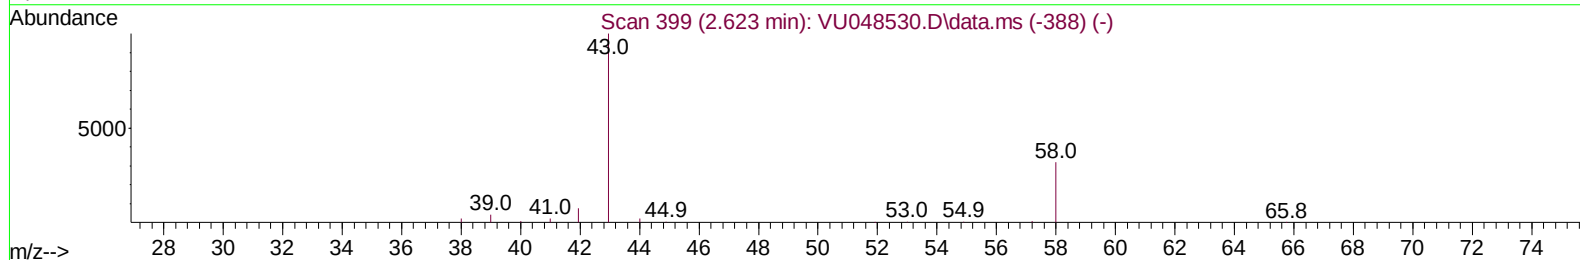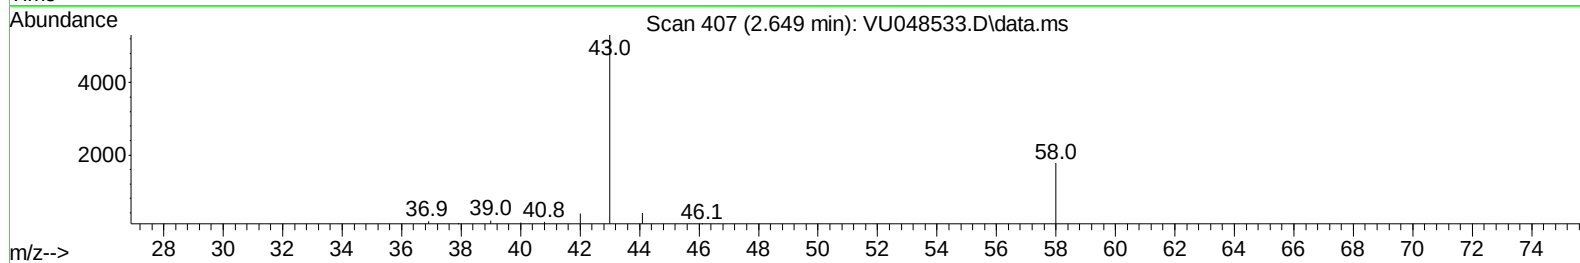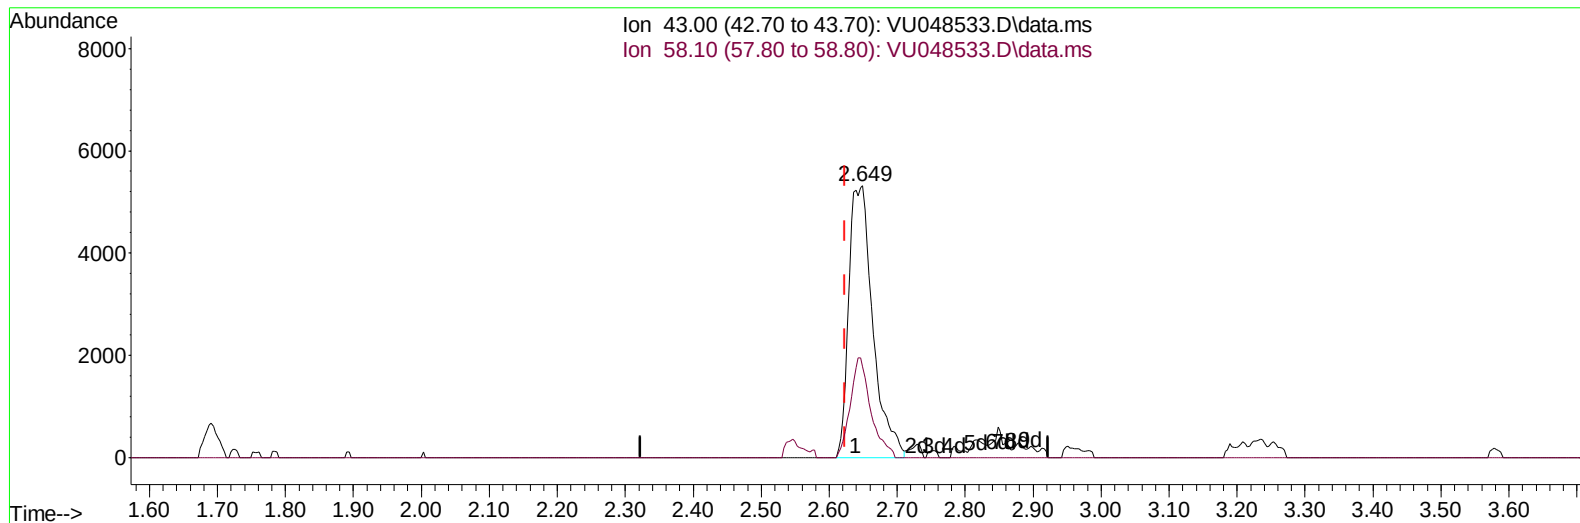

TIC: VU048533.D\data.ms

(13) Acetone (T)

2.649min (+ 0.026) 8.11 ug/L m

response 13059

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.10	31.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048533.D
 Acq On : 12 May 2022 11:56
 Operator : SY/MD
 Sample : N2801-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLE0

Manual IntegrationsAPPROVED

Quant Time: May 13 03:57:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 03:54:05 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/13/2022
 Supervised By :Mahesh Dadoda 05/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	291030	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	292610	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	154486	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	74050	29.544	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	59.080%#	
7) Chloroethane-d5	1.913	69	56260	34.394	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	68.780%#	
11) 1,1-Dichloroethene-d2	2.569	63	124850	27.989	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	55.980%#	
21) 2-Butanone-d5	4.630	46	148162	69.411	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	69.410%	
24) Chloroform-d	5.067	84	184546	42.391	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	84.780%	
26) 1,2-Dichloroethane-d4	5.704	65	132889	46.959	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.920%	
32) Benzene-d6	5.729	84	337832	37.994	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	75.980%	
36) 1,2-Dichloropropane-d6	6.691	67	105301	36.316	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	72.640%	
41) Toluene-d8	7.900	98	309947	39.413	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	78.820%#	
43) trans-1,3-Dichloroprop...	8.179	79	58335	43.710	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.420%	
47) 2-Hexanone-d5	8.636	63	107529	76.619	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	76.620%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	157977	35.768	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	71.540%	
66) 1,2-Dichlorobenzene-d4	12.192	152	132976	43.470	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	86.940%	
Target Compounds						
13) Acetone	2.649	43	13059m	8.115	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048533.D
Acq On : 12 May 2022 11:56
Operator : SY/MD
Sample : N2801-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLE0

Manual IntegrationsAPPROVED

Quant Time: May 13 03:57:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/13/2022
Supervised By :Mahesh Dadoda 05/13/2022

