

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048542.D
 Acq On : 12 May 2022 15:26
 Operator : SY/MD
 Sample : N2790-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP6

Quant Time: May 13 03:59:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 03:54:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	276161	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	282212	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	144406	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	78487	33.000	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	66.000%
7) Chloroethane-d5	1.912	69	62655	40.365	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.740%
11) 1,1-Dichloroethene-d2	2.568	63	130123	30.742	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.480%
21) 2-Butanone-d5	4.620	46	162522	80.238	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.240%
24) Chloroform-d	5.067	84	197923	47.911	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.820%
26) 1,2-Dichloroethane-d4	5.703	65	141797	52.804	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.600%
32) Benzene-d6	5.729	84	365356	42.603	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.200%
36) 1,2-Dichloropropane-d6	6.690	67	113336	40.527	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	81.060%
41) Toluene-d8	7.899	98	330537	43.580	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.160%
43) trans-1,3-Dichloroprop...	8.179	79	62181	48.309	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.620%
47) 2-Hexanone-d5	8.632	63	115813	85.562	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.560%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	176170	41.356	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.720%
66) 1,2-Dichlorobenzene-d4	12.195	152	139641	48.835	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.660%
Target Compounds						
13) Acetone	2.629	43	5046	3.304	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048542.D
Acq On : 12 May 2022 15:26
Operator : SY/MD
Sample : N2790-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP6

Quant Time: May 13 03:59:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

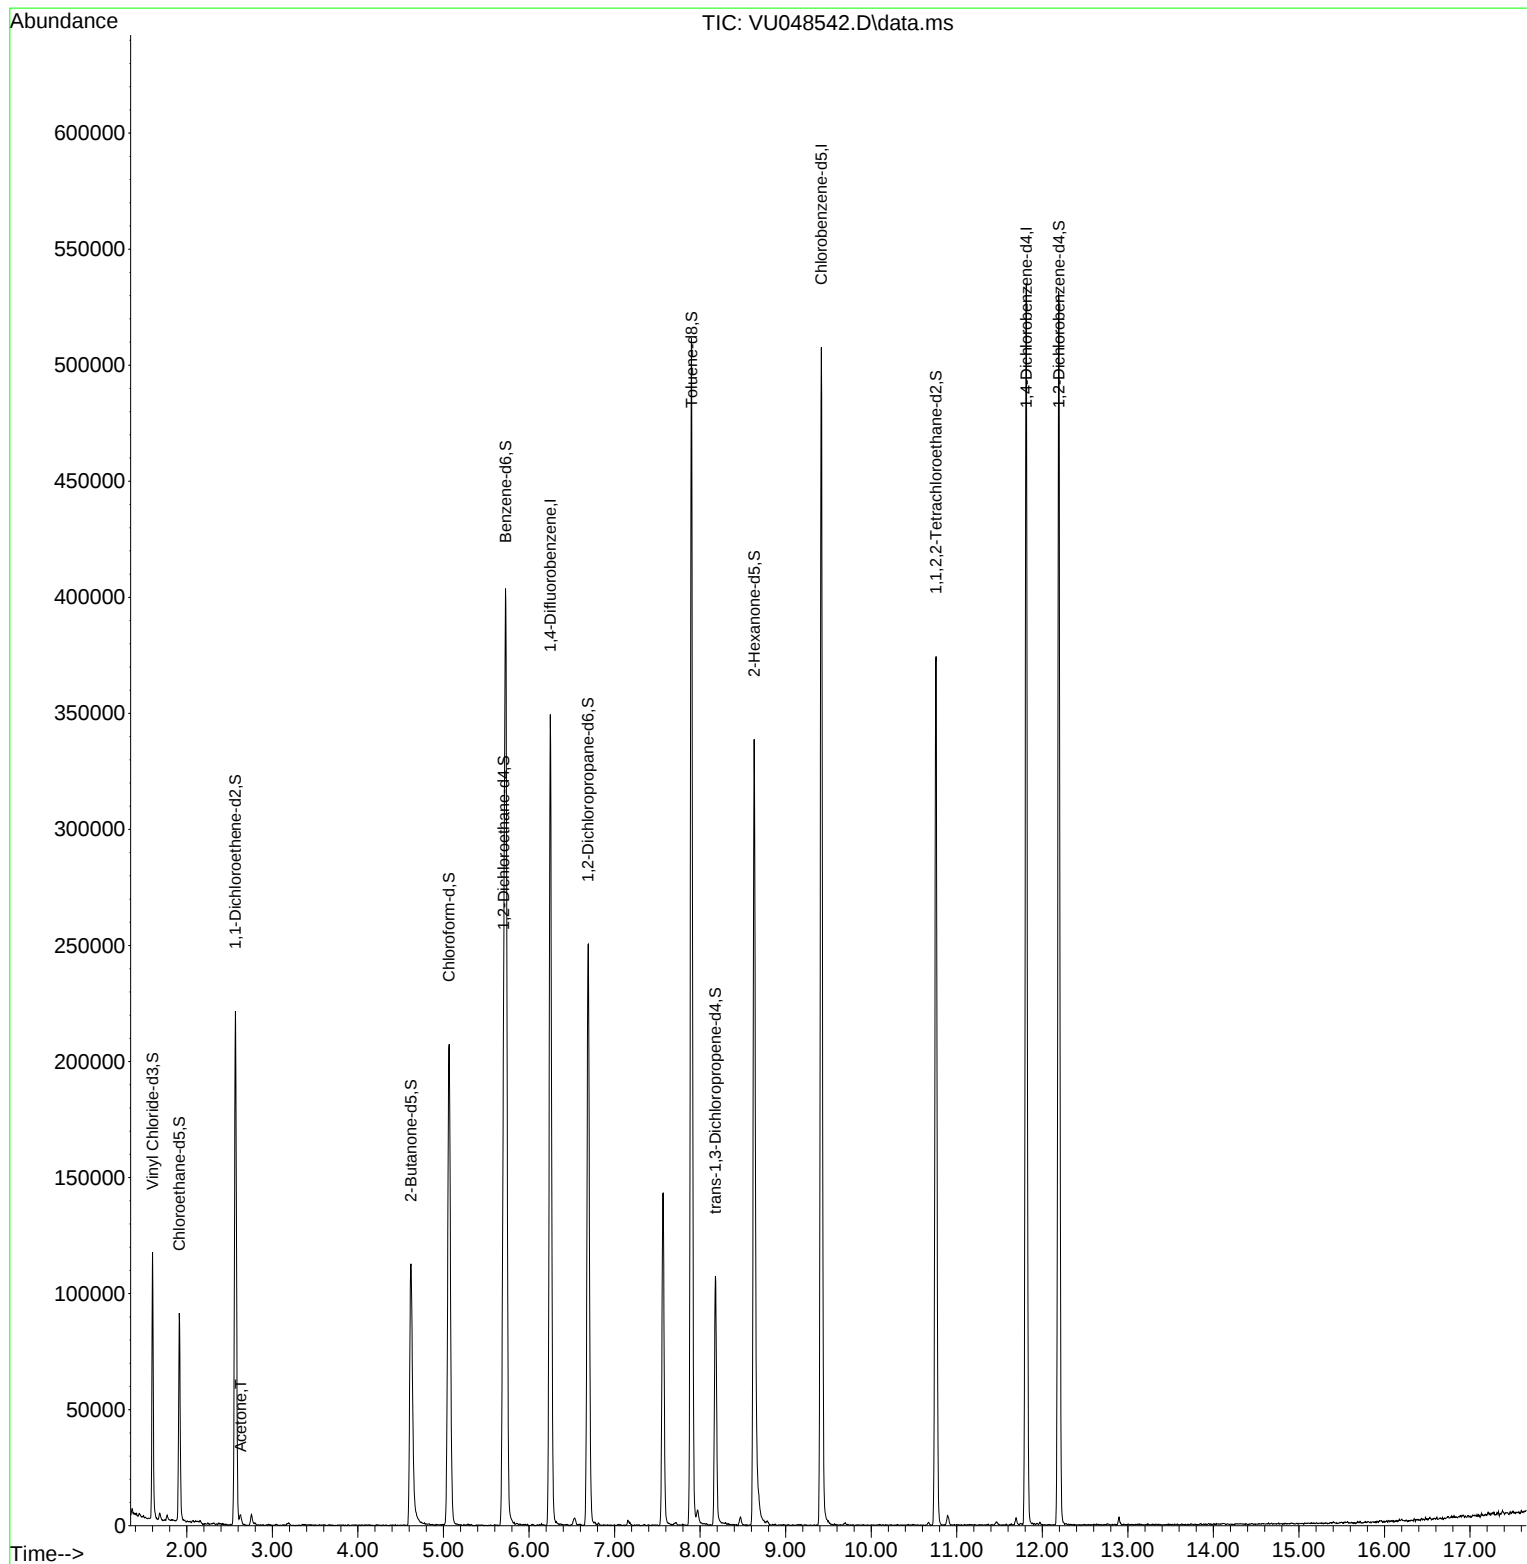

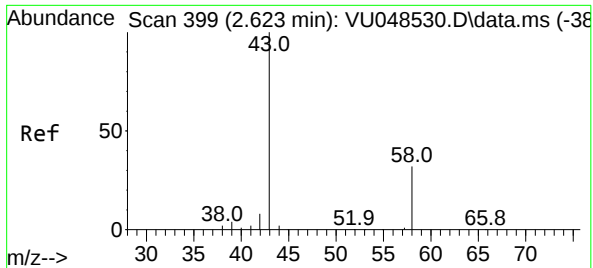

#13
 Acetone
 Concen: 3.304 ug/L
 RT: 2.629 min Scan# 401
 Delta R.T. 0.007 min
 Lab File: VU048542.D
 Acq: 12 May 2022 15:26

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP6

Tgt Ion: 43 Resp: 5046
 Ion Ratio Lower Upper
 43 100
 58 27.1 0.0 66.2

