

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048544.D
 Acq On : 12 May 2022 16:15
 Operator : SY/MD
 Sample : N2790-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP7

Quant Time: May 13 03:59:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 03:54:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	265697	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	268188	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	142785	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	76201	33.301	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	66.600%		
7) Chloroethane-d5	1.912	69	61903	41.451	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.900%		
11) 1,1-Dichloroethene-d2	2.568	63	131096	32.191	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	64.380%		
21) 2-Butanone-d5	4.620	46	160536	82.379	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.380%		
24) Chloroform-d	5.067	84	197868	49.784	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.560%		
26) 1,2-Dichloroethane-d4	5.703	65	144047	55.755	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	111.500%		
32) Benzene-d6	5.729	84	365850	44.891	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.780%		
36) 1,2-Dichloropropane-d6	6.690	67	112775	42.435	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.880%		
41) Toluene-d8	7.899	98	332431	46.122	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.240%		
43) trans-1,3-Dichloroprop...	8.179	79	60767	49.679	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	99.360%		
47) 2-Hexanone-d5	8.632	63	117490	91.340	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.340%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	177027	43.731	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.460%		
66) 1,2-Dichlorobenzene-d4	12.195	152	145441	51.440	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.880%		
Target Compounds					Qvalue	
13) Acetone	2.629	43	4835	3.291	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048544.D
Acq On : 12 May 2022 16:15
Operator : SY/MD
Sample : N2790-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP7

Quant Time: May 13 03:59:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

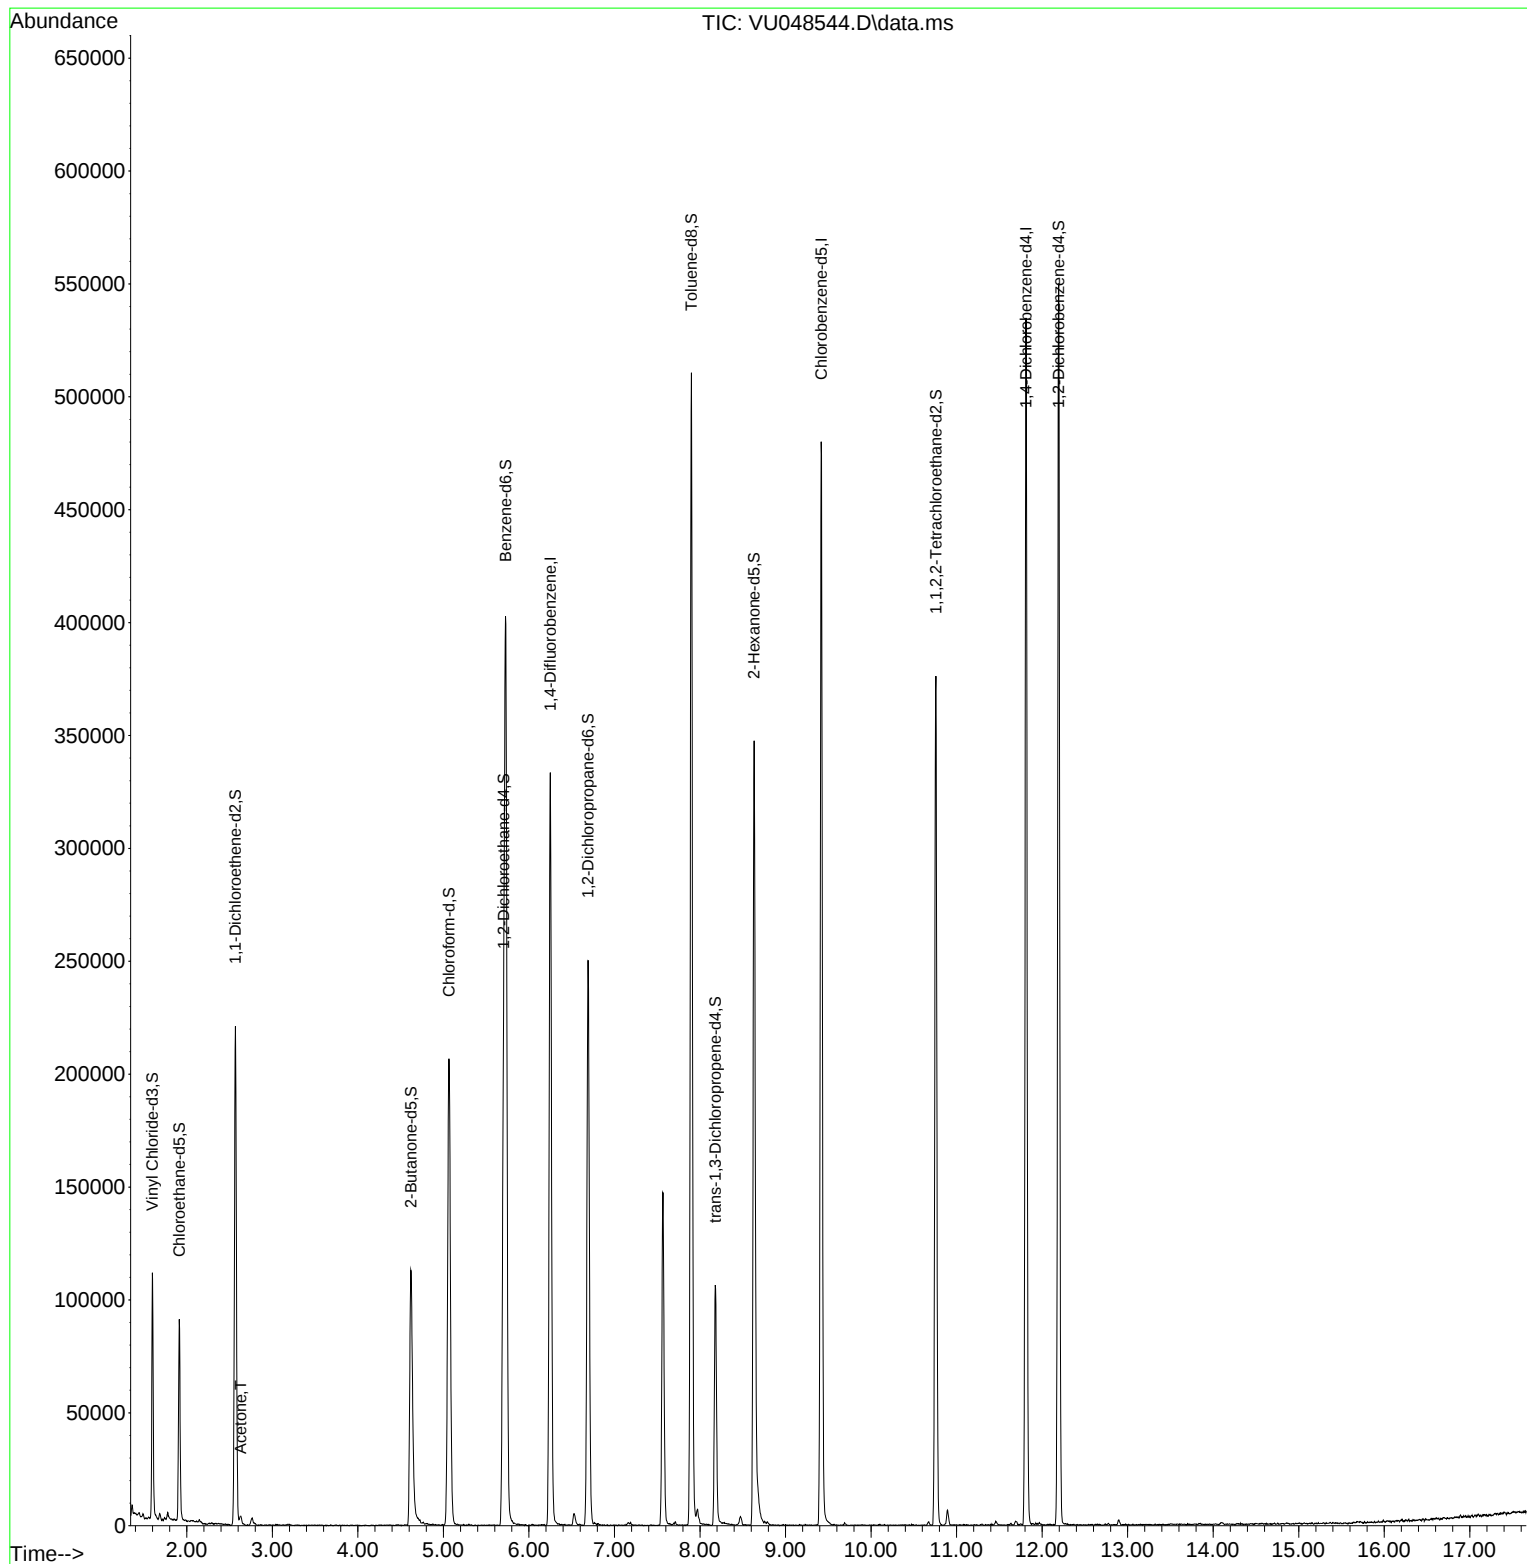

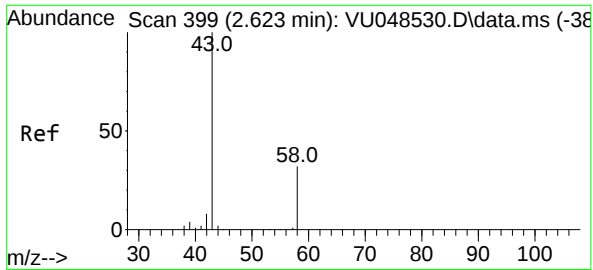

#13
 Acetone
 Concen: 3.291 ug/L
 RT: 2.629 min Scan# 401
 Delta R.T. 0.006 min
 Lab File: VU048544.D
 Acq: 12 May 2022 16:15

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP7

Tgt Ion: 43 Resp: 4835
 Ion Ratio Lower Upper
 43 100
 58 26.1 0.0 66.2

