

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048546.D
 Acq On : 12 May 2022 17:02
 Operator : SY/MD
 Sample : N2767-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ2

Quant Time: May 13 04:00:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 03:54:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	269910	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	272641	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	142532	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	77118	33.176	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	66.360%
7) Chloroethane-d5	1.912	69	60681	39.999	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.000%
11) 1,1-Dichloroethene-d2	2.568	63	127890	30.914	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.820%
21) 2-Butanone-d5	4.620	46	161738	81.701	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.700%
24) Chloroform-d	5.063	84	196788	48.740	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.480%
26) 1,2-Dichloroethane-d4	5.703	65	143085	54.518	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.040%
32) Benzene-d6	5.729	84	357161	43.109	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.220%
36) 1,2-Dichloropropane-d6	6.694	67	110611	40.941	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	81.880%
41) Toluene-d8	7.899	98	328145	44.783	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.560%
43) trans-1,3-Dichloroprop...	8.179	79	61011	49.064	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.120%
47) 2-Hexanone-d5	8.632	63	115121	88.036	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.040%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	176438	42.873	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.740%
66) 1,2-Dichlorobenzene-d4	12.195	152	140255	49.694	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.380%
Target Compounds						
13) Acetone	2.626	43	6057	4.058	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048546.D
Acq On : 12 May 2022 17:02
Operator : SY/MD
Sample : N2767-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ2

Quant Time: May 13 04:00:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

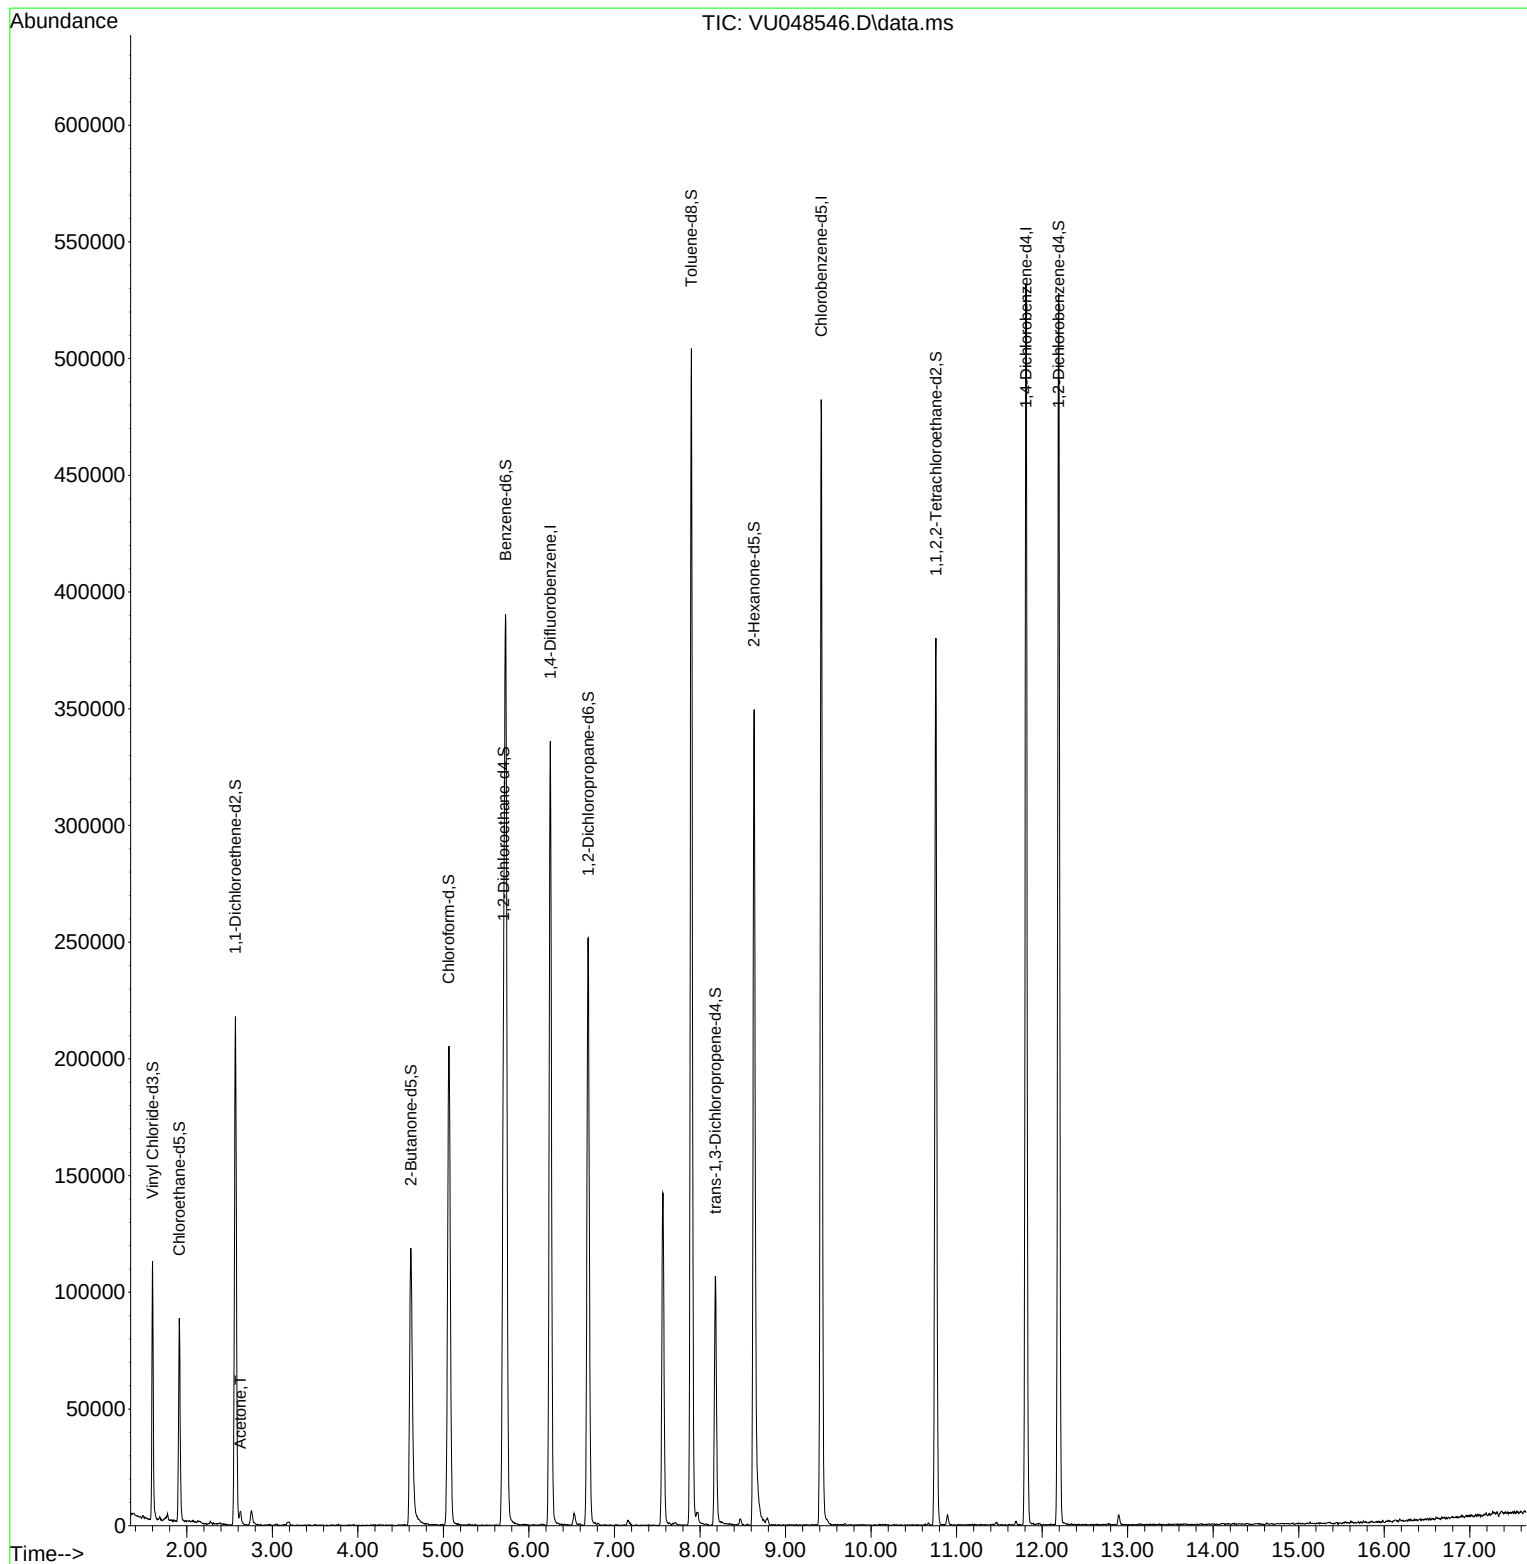

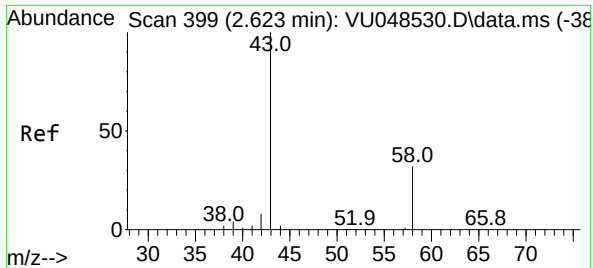

#13
 Acetone
 Concen: 4.058 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU048546.D
 Acq: 12 May 2022 17:02

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ2

Tgt Ion: 43 Resp: 6057
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 66.2

