

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048549.D
 Acq On : 12 May 2022 18:11
 Operator : SY/MD
 Sample : N2767-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP2

Quant Time: May 13 04:00:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 03:54:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	266674	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	269429	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	141342	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	74430	32.408	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.820%		
7) Chloroethane-d5	1.912	69	58380	38.949	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.900%		
11) 1,1-Dichloroethene-d2	2.568	63	124505	30.461	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.920%		
21) 2-Butanone-d5	4.620	46	159618	81.608	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	81.610%		
24) Chloroform-d	5.067	84	189872	47.598	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.200%		
26) 1,2-Dichloroethane-d4	5.703	65	141231	54.464	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.920%		
32) Benzene-d6	5.729	84	354748	43.329	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.660%		
36) 1,2-Dichloropropane-d6	6.690	67	110622	41.433	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.860%		
41) Toluene-d8	7.899	98	320373	44.244	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.480%		
43) trans-1,3-Dichloroprop...	8.179	79	60776	49.457	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.920%		
47) 2-Hexanone-d5	8.632	63	115173	89.126	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.130%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	171878	42.263	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.520%		
66) 1,2-Dichlorobenzene-d4	12.195	152	138217	49.385	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.760%		
Target Compounds					Qvalue	
13) Acetone	2.626	43	10213	6.926	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048549.D
Acq On : 12 May 2022 18:11
Operator : SY/MD
Sample : N2767-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP2

Quant Time: May 13 04:00:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

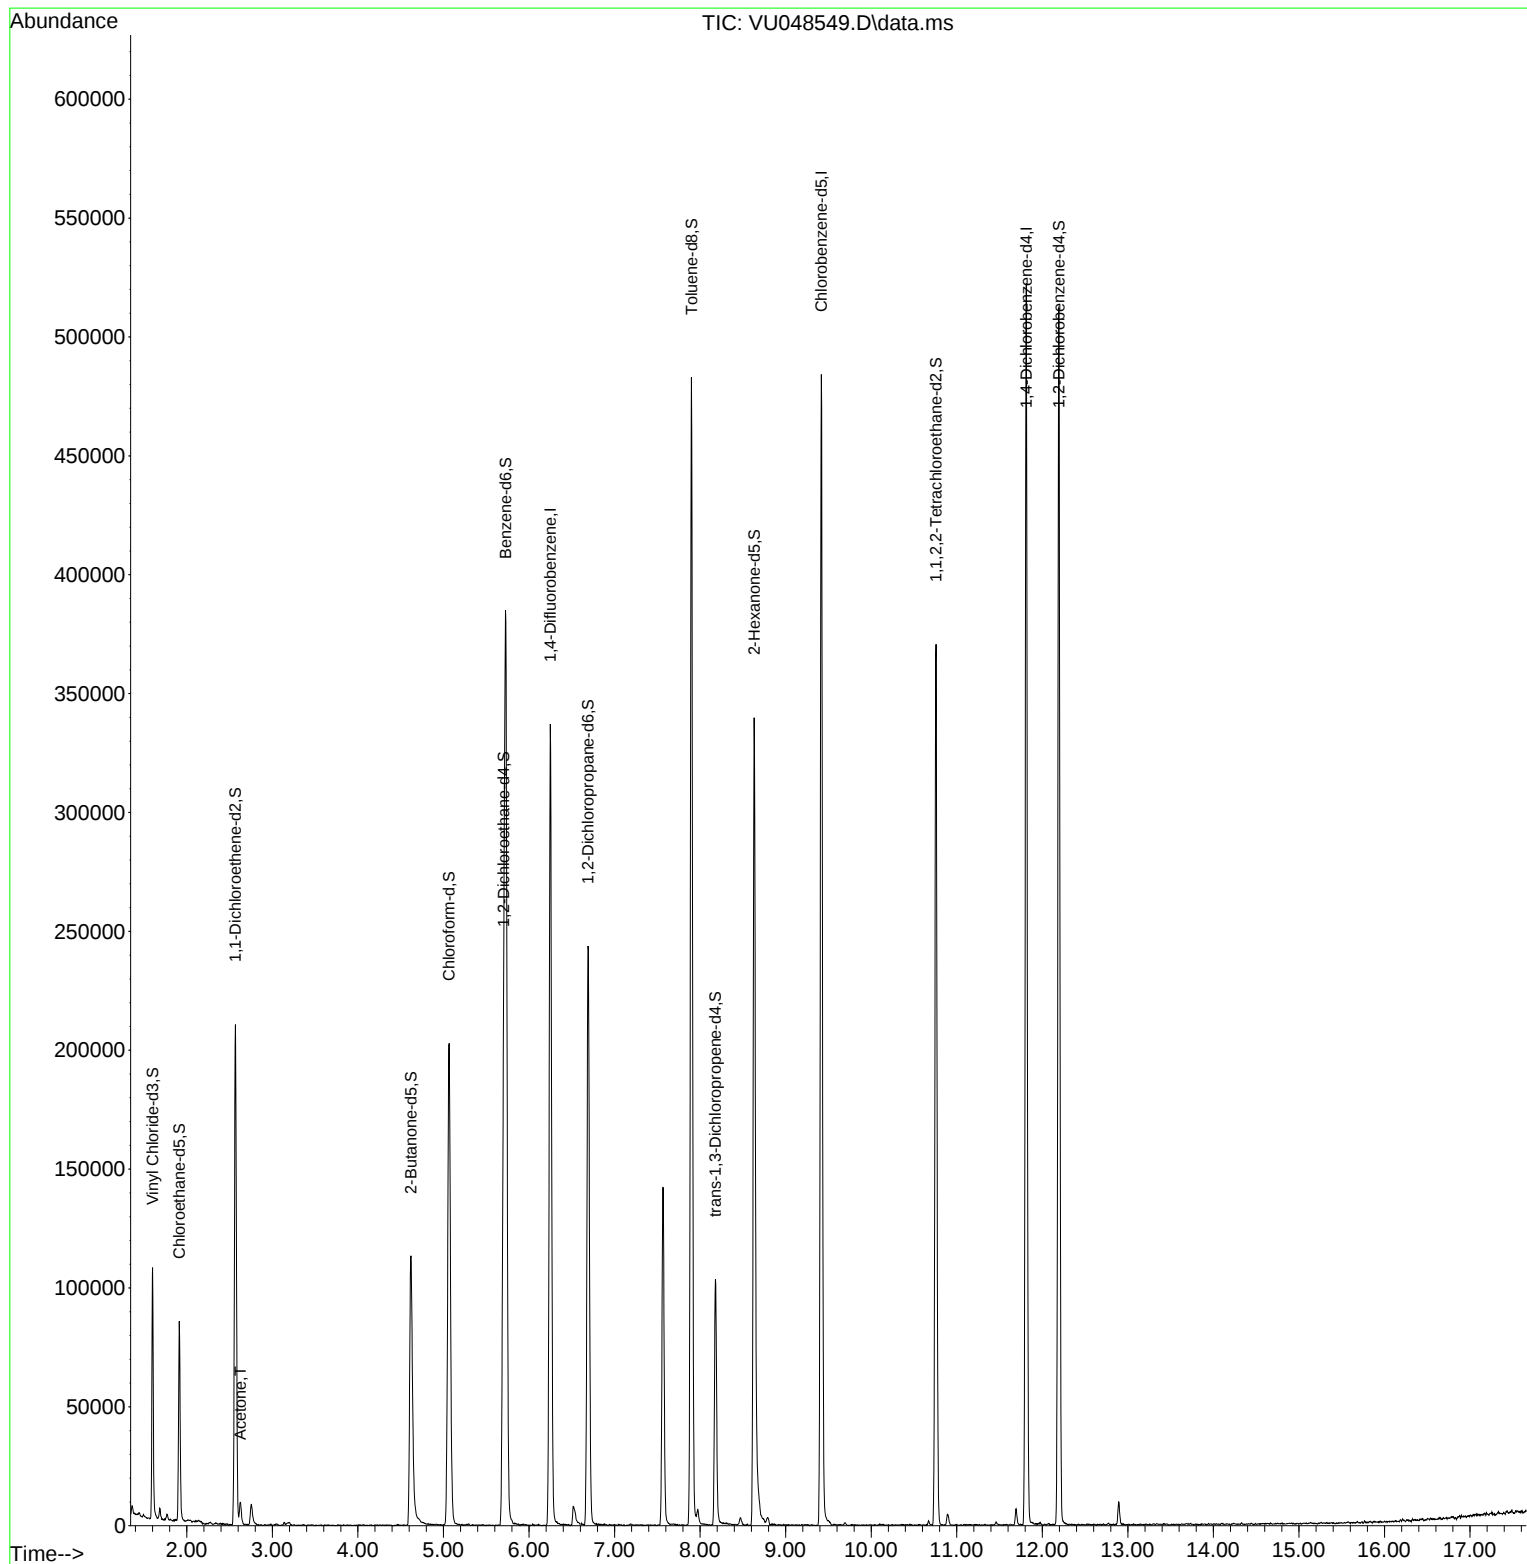

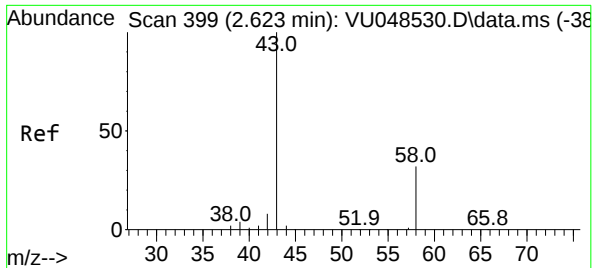

#13
 Acetone
 Concen: 6.926 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU048549.D
 Acq: 12 May 2022 18:11

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP2

Tgt Ion: 43 Resp: 10213
 Ion Ratio Lower Upper
 43 100
 58 29.0 0.0 66.2

