

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048550.D
 Acq On : 12 May 2022 18:34
 Operator : SY/MD
 Sample : N2767-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP3

Quant Time: May 13 04:00:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 03:54:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	263106	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	264444	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	137720	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	70543	31.132	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	62.260%		
7) Chloroethane-d5	1.912	69	59306	40.104	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.200%		
11) 1,1-Dichloroethene-d2	2.568	63	121342	30.089	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.180%		
21) 2-Butanone-d5	4.623	46	160195	83.014	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.010%		
24) Chloroform-d	5.067	84	191212	48.584	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.160%		
26) 1,2-Dichloroethane-d4	5.703	65	139369	54.475	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.960%		
32) Benzene-d6	5.729	84	346892	43.168	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.340%		
36) 1,2-Dichloropropane-d6	6.690	67	109838	41.915	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.840%		
41) Toluene-d8	7.899	98	316431	44.523	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.040%		
43) trans-1,3-Dichloroprop...	8.179	79	58491	48.495	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.000%		
47) 2-Hexanone-d5	8.636	63	119161	93.950	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.950%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	170126	42.621	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.240%		
66) 1,2-Dichlorobenzene-d4	12.192	152	137335	50.360	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.720%		
Target Compounds					Qvalue	
13) Acetone	2.633	43	6473	4.449	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048550.D
Acq On : 12 May 2022 18:34
Operator : SY/MD
Sample : N2767-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP3

Quant Time: May 13 04:00:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 03:54:05 2022
Response via : Initial Calibration

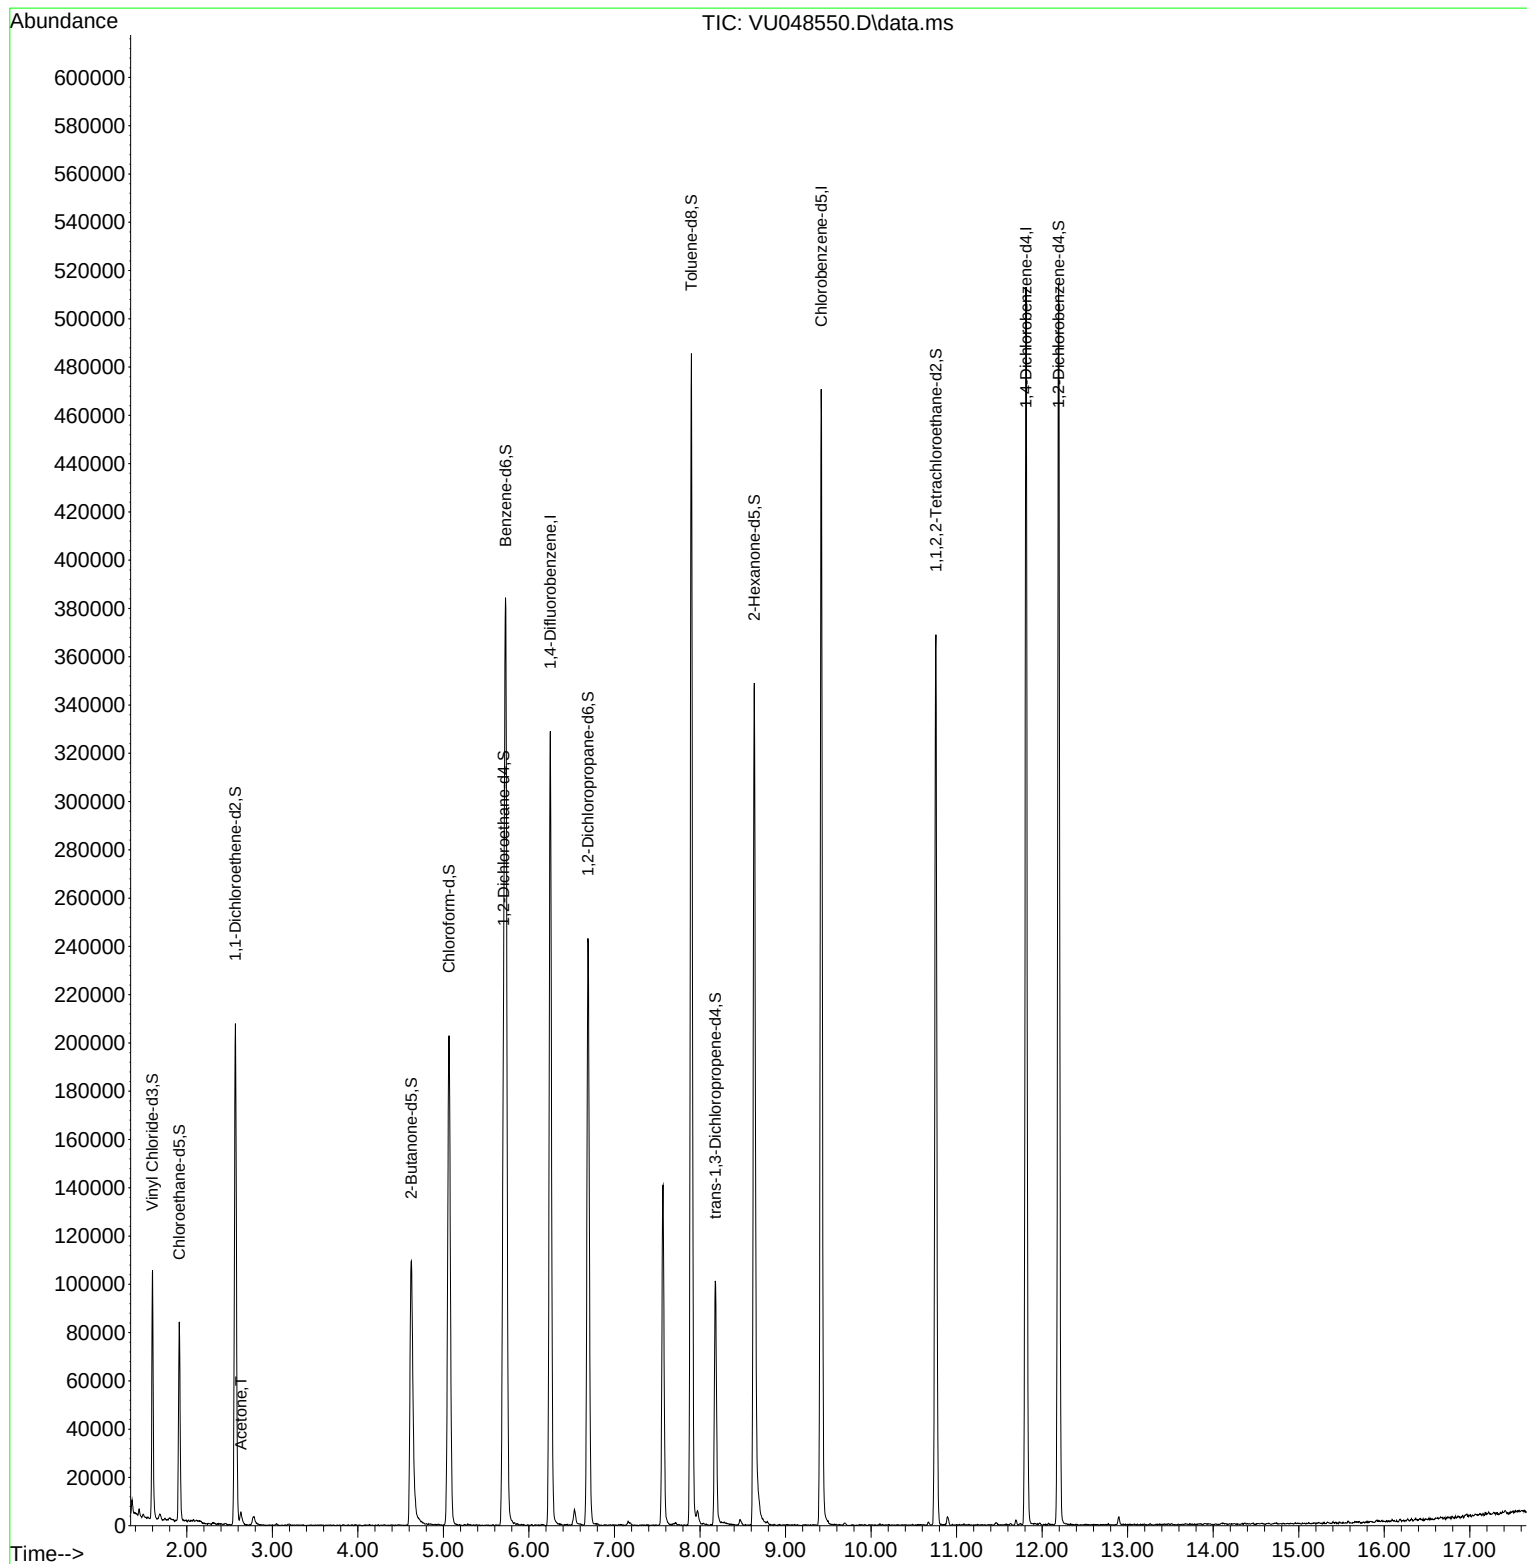

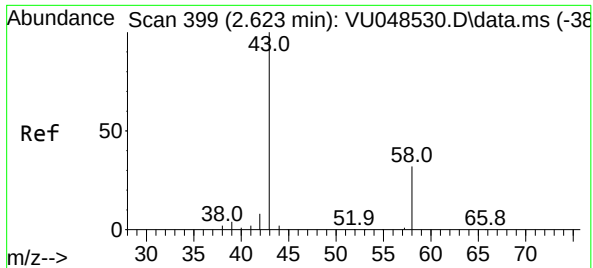

#13
 Acetone
 Concen: 4.449 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. 0.010 min
 Lab File: VU048550.D
 Acq: 12 May 2022 18:34

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP3

Tgt Ion: 43 Resp: 6473
 Ion Ratio Lower Upper
 43 100
 58 33.4 0.0 66.2

