

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048533.D
 Acq On : 12 May 2022 11:56
 Operator : SY/MD
 Sample : N2801-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	71	80	95	rVB	108220	134226	13.20%	1.582%
2	1.913	171	178	192	rVB	83625	106684	10.49%	1.257%
3	2.196	265	266	271	rVB	560	354	0.03%	0.004%
4	2.286	292	294	297	rBV	375	267	0.03%	0.003%
5	2.569	370	382	397	rBV	208614	343882	33.82%	4.053%
6	2.755	435	440	443	rBV3	385	399	0.04%	0.005%
7	2.987	510	512	513	rBV3	355	152	0.01%	0.002%
8	3.048	528	531	536	rVB2	526	347	0.03%	0.004%
9	3.077	536	540	543	rBV2	184	179	0.02%	0.002%
10	3.122	550	554	560	rVB2	269	243	0.02%	0.003%
11	3.504	670	673	677	rBV	222	237	0.02%	0.003%
12	3.553	684	688	691	rBV2	228	222	0.02%	0.003%
13	3.585	691	698	701	rBV3	362	451	0.04%	0.005%
14	3.778	755	758	760	rBV2	277	246	0.02%	0.003%
15	3.919	797	802	804	rBV	253	263	0.03%	0.003%
16	3.977	817	820	823	rBV	203	188	0.02%	0.002%
17	4.077	848	851	853	rBV2	255	174	0.02%	0.002%
18	4.163	874	878	880	rBV	175	157	0.02%	0.002%
19	4.205	887	891	895	rVV2	187	197	0.02%	0.002%
20	4.308	920	923	930	rVB	205	153	0.02%	0.002%
21	4.369	937	942	947	rBB	302	278	0.03%	0.003%
22	4.398	948	951	953	rBV	294	210	0.02%	0.002%
23	4.450	953	967	983	rBV5	4420	11303	1.11%	0.133%
24	4.517	983	988	990	rBV4	909	786	0.08%	0.009%
25	4.578	1003	1007	1009	rBV2	376	212	0.02%	0.002%
26	4.630	1009	1023	1049	rBV	97069	262054	25.78%	3.089%
27	4.900	1105	1107	1112	rVV2	369	314	0.03%	0.004%
28	5.067	1142	1159	1177	rBV	193028	422428	41.55%	4.979%
29	5.208	1198	1203	1205	rBV2	486	427	0.04%	0.005%
30	5.292	1225	1229	1234	rVB3	367	349	0.03%	0.004%
31	5.385	1251	1258	1264	rBV3	717	938	0.09%	0.011%
32	5.427	1267	1271	1276	rVB2	388	437	0.04%	0.005%
33	5.462	1276	1282	1285	rBB	186	221	0.02%	0.003%
34	5.620	1328	1331	1334	rVB	336	223	0.02%	0.003%
35	5.655	1340	1342	1343	rBV	316	164	0.02%	0.002%
36	5.726	1343	1364	1386	rBV2	371170	1016687	100.00%	11.983%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048533.D
 Acq On : 12 May 2022 11:56
 Operator : SY/MD
 Sample : N2801-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.909	1419	1421	1427	rVB	505	345	0.03%	0.004%
38	5.938	1427	1430	1431	rBV	215	138	0.01%	0.002%
39	5.983	1440	1444	1447	rBB	257	206	0.02%	0.002%
40	6.009	1447	1452	1453	rBV	230	187	0.02%	0.002%
41	6.048	1460	1464	1471	rVB3	525	630	0.06%	0.007%
42	6.080	1471	1474	1475	rBV2	284	153	0.02%	0.002%
43	6.112	1480	1484	1486	rBV	378	233	0.02%	0.003%
44	6.176	1500	1504	1505	rBV	292	189	0.02%	0.002%
45	6.250	1512	1527	1545	rBV	361264	693327	68.19%	8.171%
46	6.395	1568	1572	1575	rBV4	730	688	0.07%	0.008%
47	6.530	1605	1614	1626	rVV3	4968	8696	0.86%	0.102%
48	6.694	1650	1665	1685	rBV	233136	456862	44.94%	5.385%
49	6.880	1721	1723	1724	rBV	345	147	0.01%	0.002%
50	6.945	1740	1743	1745	rBV	352	249	0.02%	0.003%
51	7.041	1770	1773	1775	rBV2	183	139	0.01%	0.002%
52	7.096	1787	1790	1792	rBV2	431	334	0.03%	0.004%
53	7.131	1792	1801	1807	rVV3	1910	3373	0.33%	0.040%
54	7.221	1827	1829	1832	rVB	400	167	0.02%	0.002%
55	7.289	1844	1850	1854	rBV	210	334	0.03%	0.004%
56	7.488	1910	1912	1917	rBV2	264	308	0.03%	0.004%
57	7.568	1924	1937	1955	rBV	133439	237411	23.35%	2.798%
58	7.687	1972	1974	1976	rBV2	448	215	0.02%	0.003%
59	7.729	1984	1987	1991	rVB2	417	348	0.03%	0.004%
60	7.900	2027	2040	2055	rBV	472229	815002	80.16%	9.606%
61	8.179	2115	2127	2145	rBV2	100347	172800	17.00%	2.037%
62	8.382	2186	2190	2194	rBV2	273	322	0.03%	0.004%
63	8.404	2195	2197	2203	rVV2	306	214	0.02%	0.003%
64	8.446	2207	2210	2211	rBV2	672	422	0.04%	0.005%
65	8.475	2211	2219	2228	rVB4	3926	7039	0.69%	0.083%
66	8.636	2257	2269	2301	rVV	313625	585355	57.57%	6.899%
67	8.867	2338	2341	2344	rBV2	391	257	0.03%	0.003%
68	9.086	2405	2409	2411	rBV2	368	253	0.02%	0.003%
69	9.154	2426	2430	2432	rBV	278	213	0.02%	0.003%
70	9.218	2448	2450	2454	rVV	233	156	0.02%	0.002%
71	9.417	2499	2512	2540	rBV	534512	881356	86.69%	10.388%
72	9.568	2554	2559	2560	rBV	383	338	0.03%	0.004%
73	9.610	2569	2572	2575	rBV	277	170	0.02%	0.002%
74	9.649	2580	2584	2592	rVB3	409	381	0.04%	0.004%
75	9.691	2592	2597	2605	rBV3	991	1250	0.12%	0.015%
76	9.752	2614	2616	2619	rBV	224	148	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048533.D
 Acq On : 12 May 2022 11:56
 Operator : SY/MD
 Sample : N2801-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.896	2658	2661	2663	rBV	177	148	0.01%	0.002%
78	10.099	2720	2724	2725	rBV	612	421	0.04%	0.005%
79	10.150	2737	2740	2743	rBV	214	164	0.02%	0.002%
80	10.195	2747	2754	2755	rBV	267	268	0.03%	0.003%
81	10.347	2797	2801	2807	rVB4	1335	1637	0.16%	0.019%
82	10.453	2830	2834	2837	rBV	202	195	0.02%	0.002%
83	10.671	2898	2902	2910	rVB4	1660	1937	0.19%	0.023%
84	10.755	2916	2928	2948	rVB	333731	545391	53.64%	6.428%
85	10.838	2952	2954	2959	rBV3	380	289	0.03%	0.003%
86	10.893	2961	2971	2979	rBV3	5614	8386	0.82%	0.099%
87	11.038	3014	3016	3020	rBV	254	162	0.02%	0.002%
88	11.134	3044	3046	3052	rVB3	366	321	0.03%	0.004%
89	11.163	3052	3055	3060	rBV	291	183	0.02%	0.002%
90	11.199	3062	3066	3071	rBV	434	393	0.04%	0.005%
91	11.324	3101	3105	3108	rBV2	474	351	0.03%	0.004%
92	11.465	3138	3149	3162	rBV8	1884	3478	0.34%	0.041%
93	11.742	3231	3235	3244	rBV4	874	1167	0.11%	0.014%
94	11.813	3244	3257	3274	rBV	588967	925285	91.01%	10.905%
95	12.192	3362	3375	3393	rVV	499917	813994	80.06%	9.594%
96	12.330	3415	3418	3421	rBV2	767	603	0.06%	0.007%
97	12.684	3525	3528	3531	rBV2	369	261	0.03%	0.003%
98	13.218	3691	3694	3702	rBV3	936	1101	0.11%	0.013%
99	13.851	3883	3891	3893	rBV4	1353	1764	0.17%	0.021%
100	14.150	3981	3984	3987	rBV3	531	422	0.04%	0.005%




Sum of corrected areas: 8484728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048533.D
Acq On : 12 May 2022 11:56
Operator : SY/MD
Sample : N2801-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

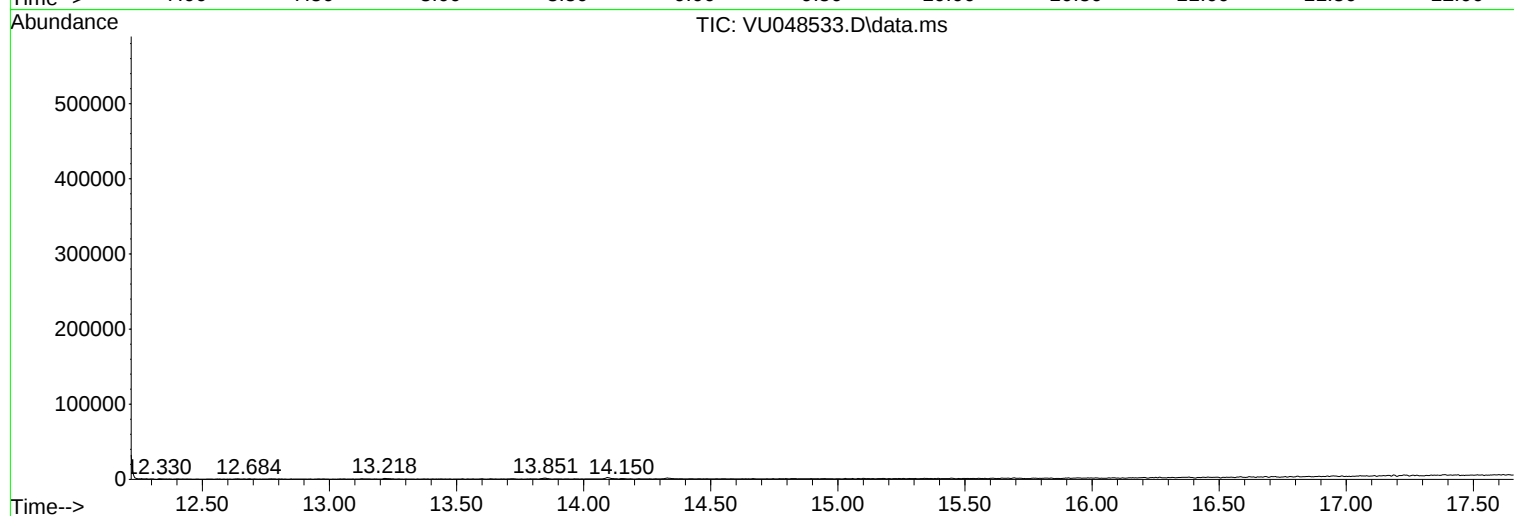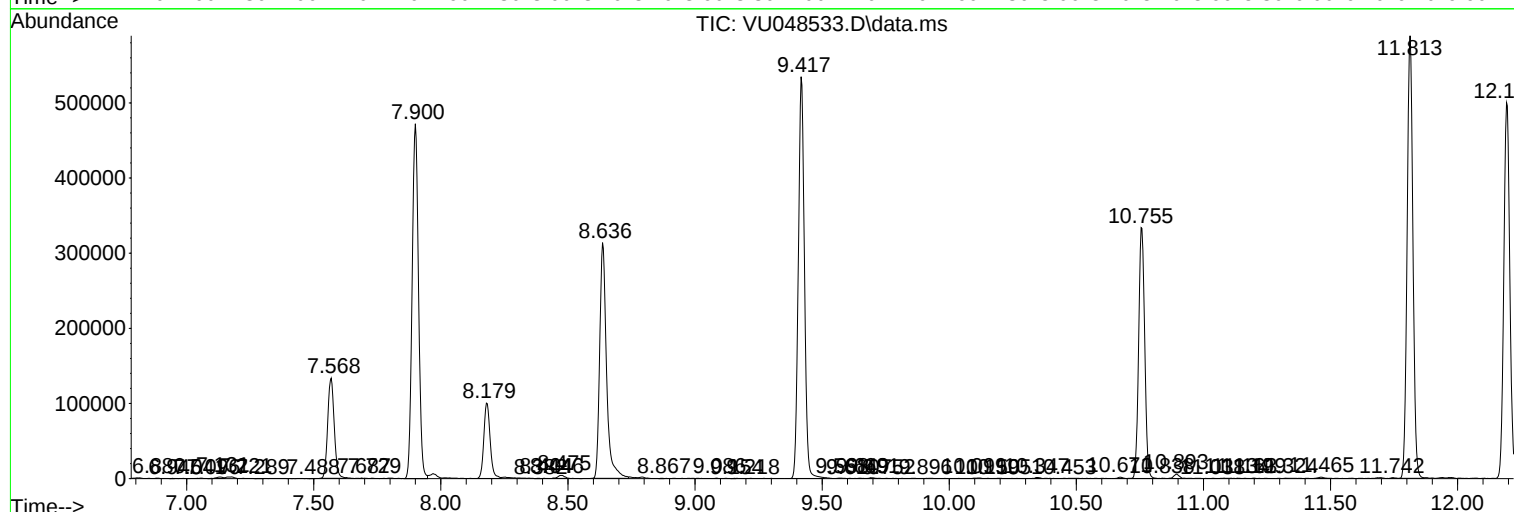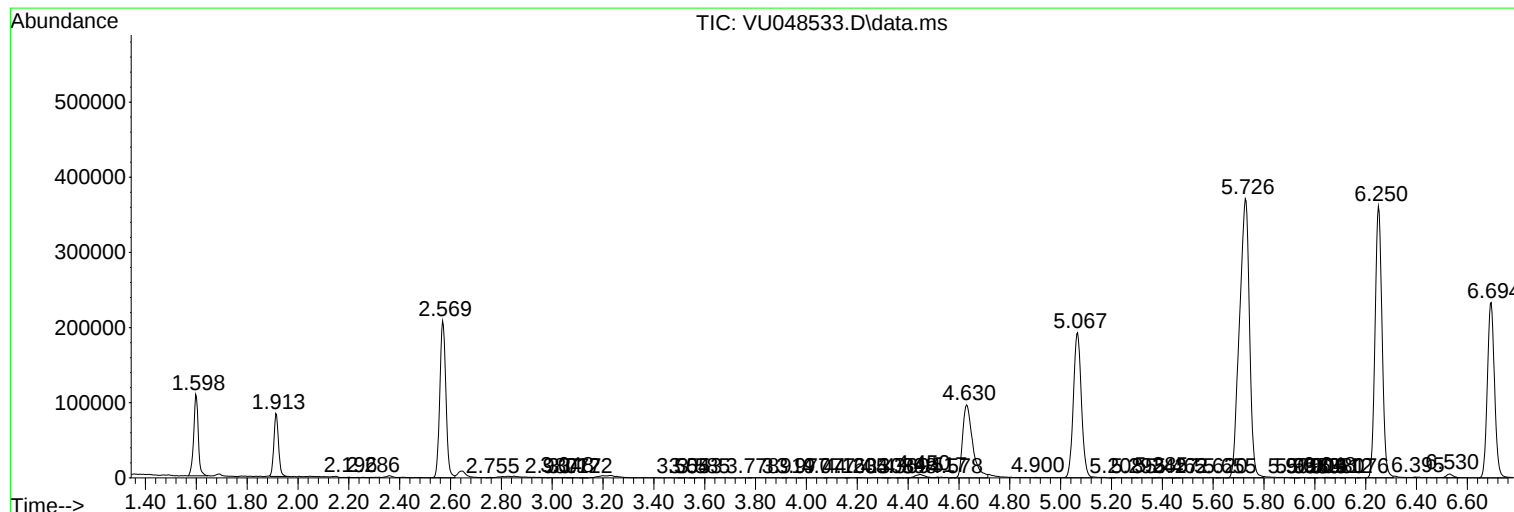

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048533.D
Acq On : 12 May 2022 11:56
Operator : SY/MD
Sample : N2801-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048533.D
Acq On : 12 May 2022 11:56
Operator : SY/MD
Sample : N2801-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------