

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048536.D
 Acq On : 12 May 2022 13:06
 Operator : SY/MD
 Sample : N2801-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	101	rVB	117436	132598	12.20%	1.528%
2	1.916	170	179	192	rVB	88055	114060	10.49%	1.315%
3	2.317	300	304	306	rBV2	492	335	0.03%	0.004%
4	2.372	318	321	326	rBV4	703	605	0.06%	0.007%
5	2.494	357	359	362	rBV	264	155	0.01%	0.002%
6	2.568	370	382	398	rBV	221011	358032	32.94%	4.127%
7	2.755	432	440	449	rBV3	1929	3275	0.30%	0.038%
8	2.861	470	473	478	rBV2	226	175	0.02%	0.002%
9	3.089	541	544	549	rBB	204	219	0.02%	0.003%
10	3.186	560	574	586	rBV3	2977	7094	0.65%	0.082%
11	3.260	594	597	599	rBV	346	244	0.02%	0.003%
12	3.327	615	618	623	rVB	470	202	0.02%	0.002%
13	3.369	629	631	634	rVB	337	177	0.02%	0.002%
14	3.395	635	639	640	rBV	199	172	0.02%	0.002%
15	3.642	714	716	719	rBB2	261	159	0.01%	0.002%
16	3.748	744	749	751	rBB2	301	284	0.03%	0.003%
17	3.938	806	808	812	rVB	269	175	0.02%	0.002%
18	3.960	813	815	820	rBB	381	330	0.03%	0.004%
19	3.989	820	824	825	rBV	276	181	0.02%	0.002%
20	3.999	825	827	832	rVV2	213	163	0.01%	0.002%
21	4.038	836	839	843	rBV	349	354	0.03%	0.004%
22	4.076	849	851	857	rVB2	278	255	0.02%	0.003%
23	4.108	857	861	866	rBB	369	328	0.03%	0.004%
24	4.279	911	914	920	rVB2	370	341	0.03%	0.004%
25	4.510	983	986	989	rVB2	277	177	0.02%	0.002%
26	4.555	997	1000	1004	rVB	322	262	0.02%	0.003%
27	4.620	1007	1020	1047	rBV	112469	265545	24.43%	3.061%
28	4.960	1122	1126	1129	rBV2	442	361	0.03%	0.004%
29	5.063	1142	1158	1182	rBV	205407	450027	41.41%	5.187%
30	5.198	1198	1200	1203	rVB3	507	283	0.03%	0.003%
31	5.224	1203	1208	1209	rBV	411	313	0.03%	0.004%
32	5.272	1220	1223	1225	rVB	367	170	0.02%	0.002%
33	5.301	1228	1232	1236	rVV4	433	446	0.04%	0.005%
34	5.356	1245	1249	1250	rBV	286	192	0.02%	0.002%
35	5.420	1267	1269	1275	rVB2	352	282	0.03%	0.003%
36	5.530	1298	1303	1305	rBV2	421	369	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048536.D
 Acq On : 12 May 2022 13:06
 Operator : SY/MD
 Sample : N2801-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.652	1335	1341	1343	rBV	309	370	0.03%	0.004%
38	5.726	1343	1364	1394	rBV2	394671	1086882	100.00%	12.528%
39	5.960	1433	1437	1439	rBV2	198	166	0.02%	0.002%
40	6.021	1453	1456	1459	rBV	217	168	0.02%	0.002%
41	6.041	1460	1462	1464	rVB2	319	158	0.01%	0.002%
42	6.092	1476	1478	1481	rBB2	263	147	0.01%	0.002%
43	6.111	1481	1484	1486	rBB	339	195	0.02%	0.002%
44	6.121	1486	1487	1489	rBV	269	154	0.01%	0.002%
45	6.250	1513	1527	1547	rBV	347188	649935	59.80%	7.491%
46	6.523	1605	1612	1624	rVB5	3239	5851	0.54%	0.067%
47	6.613	1637	1640	1642	rVB	339	202	0.02%	0.002%
48	6.690	1650	1664	1686	rBV	248109	480348	44.20%	5.537%
49	6.851	1712	1714	1718	rBV2	333	278	0.03%	0.003%
50	6.960	1745	1748	1751	rBV2	242	150	0.01%	0.002%
51	7.015	1762	1765	1768	rBV	162	157	0.01%	0.002%
52	7.041	1769	1773	1781	rVB2	254	355	0.03%	0.004%
53	7.089	1785	1788	1791	rBV	370	238	0.02%	0.003%
54	7.144	1803	1805	1808	rVB2	276	149	0.01%	0.002%
55	7.189	1814	1819	1825	rBV4	609	768	0.07%	0.009%
56	7.247	1834	1837	1841	rBV	236	230	0.02%	0.003%
57	7.269	1841	1844	1849	rVV	193	202	0.02%	0.002%
58	7.301	1851	1854	1858	rVB2	220	201	0.02%	0.002%
59	7.468	1903	1906	1909	rBV	306	240	0.02%	0.003%
60	7.565	1924	1936	1952	rBV	141749	251386	23.13%	2.898%
61	7.687	1970	1974	1975	rBV2	577	370	0.03%	0.004%
62	7.758	1992	1996	2000	rBV3	459	424	0.04%	0.005%
63	7.899	2026	2040	2056	rBV	499409	856461	78.80%	9.872%
64	8.179	2115	2127	2146	rBV	107514	183386	16.87%	2.114%
65	8.555	2233	2244	2256	rVB3	29798	50321	4.63%	0.580%
66	8.632	2256	2268	2293	rBV	323552	603045	55.48%	6.951%
67	8.816	2321	2325	2327	rBV	303	195	0.02%	0.002%
68	8.947	2362	2366	2369	rBV2	506	390	0.04%	0.004%
69	9.163	2430	2433	2434	rBV	315	199	0.02%	0.002%
70	9.343	2485	2489	2496	rVB	394	415	0.04%	0.005%
71	9.417	2496	2512	2535	rBV	498619	830437	76.41%	9.572%
72	9.568	2555	2559	2563	rBV3	378	378	0.03%	0.004%
73	9.642	2580	2582	2587	rBV	273	202	0.02%	0.002%
74	9.693	2592	2598	2599	rBV2	855	721	0.07%	0.008%
75	9.748	2613	2615	2619	rVB	236	144	0.01%	0.002%
76	9.877	2652	2655	2659	rBV	358	305	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048536.D
 Acq On : 12 May 2022 13:06
 Operator : SY/MD
 Sample : N2801-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXLB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.057	2706	2711	2717	rVB2	263	351	0.03%	0.004%
78	10.095	2721	2723	2728	rVV	266	192	0.02%	0.002%
79	10.140	2735	2737	2741	rVB	303	185	0.02%	0.002%
80	10.423	2821	2825	2830	rVB2	257	217	0.02%	0.003%
81	10.481	2839	2843	2847	rBV	372	384	0.04%	0.004%
82	10.668	2897	2901	2910	rVB5	2179	2629	0.24%	0.030%
83	10.706	2910	2913	2915	rBV2	280	188	0.02%	0.002%
84	10.754	2916	2928	2955	rVB	361031	593934	54.65%	6.846%
85	10.896	2962	2972	2983	rBV2	6599	11323	1.04%	0.131%
86	11.124	3041	3043	3047	rVB2	504	243	0.02%	0.003%
87	11.298	3090	3097	3104	rVB4	1315	1686	0.16%	0.019%
88	11.455	3142	3146	3147	rBV2	761	582	0.05%	0.007%
89	11.507	3159	3162	3164	rBV	199	154	0.01%	0.002%
90	11.812	3244	3257	3275	rBV	545010	857756	78.92%	9.887%
91	12.192	3362	3375	3395	rBV	525454	857986	78.94%	9.889%
92	12.372	3429	3431	3432	rBV	327	143	0.01%	0.002%
93	12.504	3470	3472	3476	rBV	359	240	0.02%	0.003%
94	13.031	3633	3636	3639	rBV3	479	379	0.03%	0.004%
95	13.227	3694	3697	3700	rBV2	719	502	0.05%	0.006%
96	13.352	3732	3736	3739	rBV2	351	318	0.03%	0.004%
97	13.796	3871	3874	3876	rBV	336	243	0.02%	0.003%
98	13.902	3905	3907	3912	rVB	608	328	0.03%	0.004%
99	13.925	3912	3914	3917	rBV2	439	290	0.03%	0.003%
100	14.185	3988	3995	3999	rBV3	583	957	0.09%	0.011%




Sum of corrected areas: 8675873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048536.D
Acq On : 12 May 2022 13:06
Operator : SY/MD
Sample : N2801-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

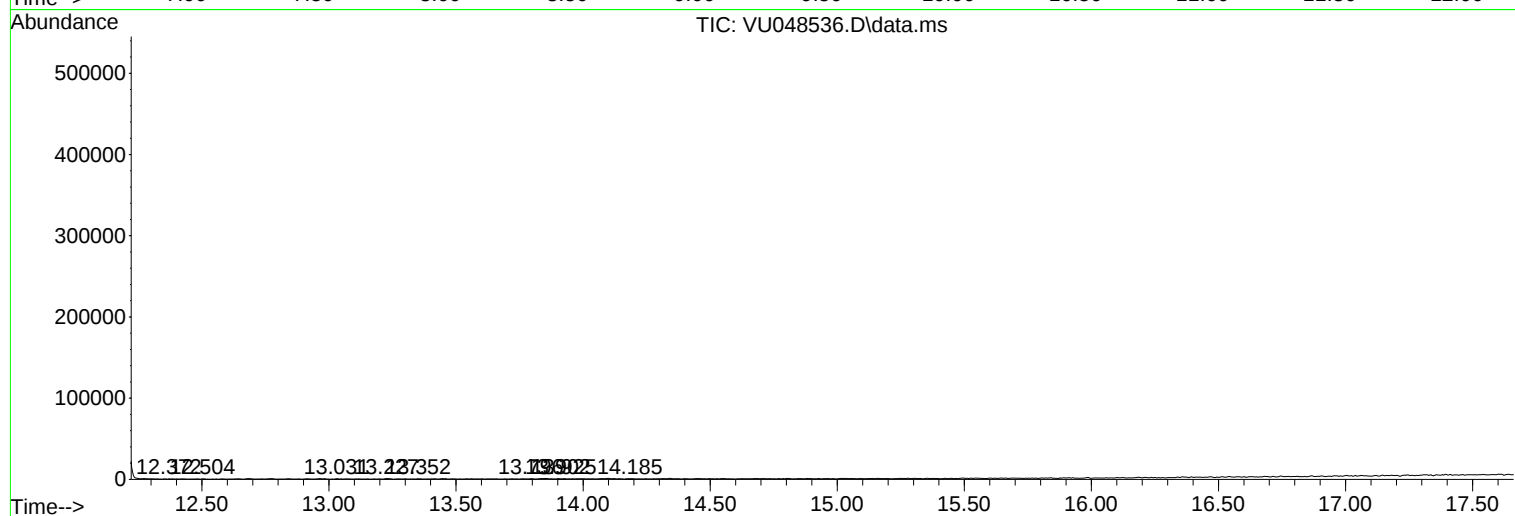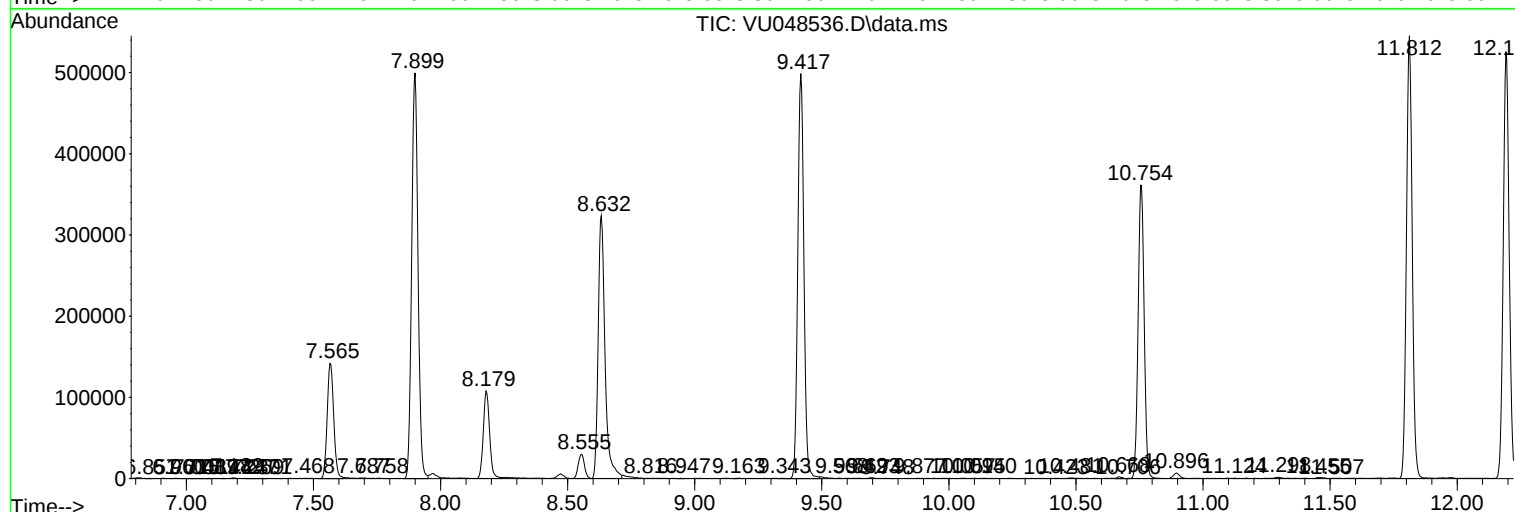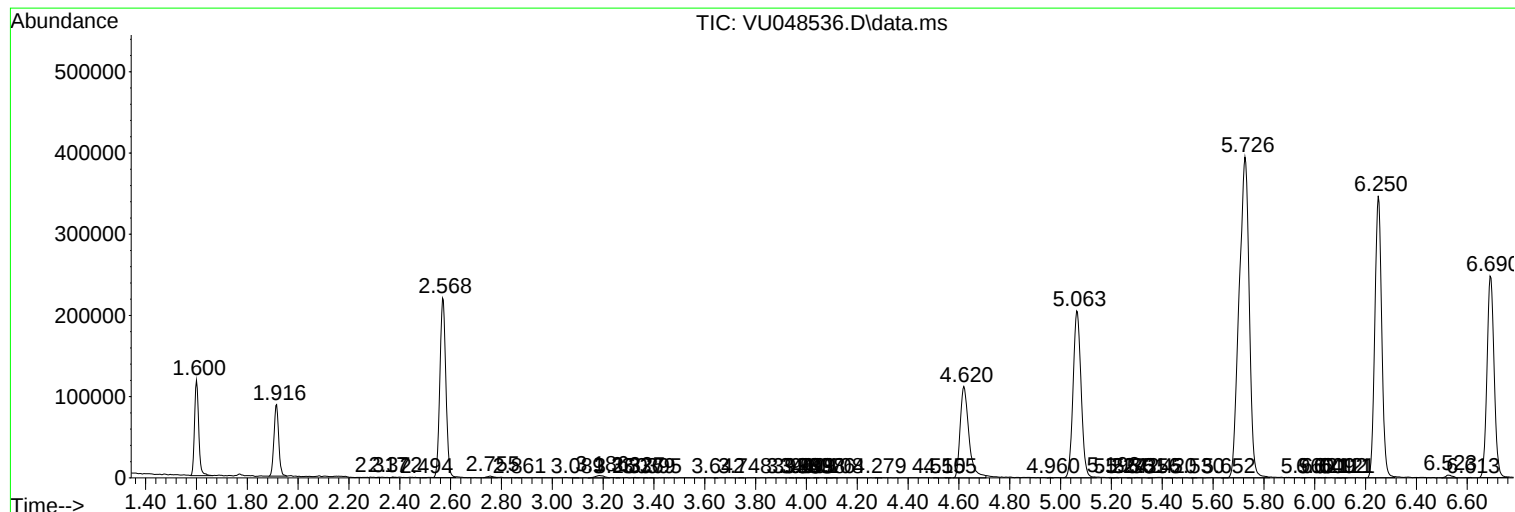

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048536.D
Acq On : 12 May 2022 13:06
Operator : SY/MD
Sample : N2801-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048536.D
Acq On : 12 May 2022 13:06
Operator : SY/MD
Sample : N2801-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXLB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------