

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048547.D
 Acq On : 12 May 2022 17:24
 Operator : SY/MD
 Sample : N2767-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M

Title : VOC Analysis

Signal : TIC: VU048547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rVB	112052	123013	11.39%	1.420%
2	1.912	170	178	191	rBV	84674	109928	10.18%	1.269%
3	2.453	345	346	349	rBV	250	154	0.01%	0.002%
4	2.568	370	382	396	rBV	212516	349828	32.40%	4.037%
5	2.697	419	422	429	rVB3	412	409	0.04%	0.005%
6	2.752	437	439	442	rBV	239	209	0.02%	0.002%
7	2.793	446	452	457	rBV2	503	709	0.07%	0.008%
8	3.176	563	571	587	rVB3	4906	9984	0.92%	0.115%
9	3.269	598	600	603	rBB	329	188	0.02%	0.002%
10	3.292	603	607	609	rBV	199	190	0.02%	0.002%
11	3.343	619	623	626	rBV	151	186	0.02%	0.002%
12	3.363	626	629	633	rBV	256	245	0.02%	0.003%
13	3.472	656	663	665	rBV2	268	300	0.03%	0.003%
14	3.584	696	698	701	rVV2	268	146	0.01%	0.002%
15	3.645	715	717	720	rVB	307	121	0.01%	0.001%
16	3.671	723	725	728	rVV2	292	128	0.01%	0.001%
17	3.771	754	756	762	rVB2	220	169	0.02%	0.002%
18	3.871	782	787	788	rBV2	205	140	0.01%	0.002%
19	3.944	808	810	814	rBV	227	187	0.02%	0.002%
20	3.990	822	824	827	rBB	263	157	0.01%	0.002%
21	4.047	839	842	843	rBV	242	127	0.01%	0.001%
22	4.208	890	892	894	rBV	367	249	0.02%	0.003%
23	4.289	913	917	926	rVB	373	500	0.05%	0.006%
24	4.469	969	973	976	rVB2	209	156	0.01%	0.002%
25	4.491	977	980	984	rBV2	252	173	0.02%	0.002%
26	4.565	999	1003	1005	rBV	207	133	0.01%	0.002%
27	4.620	1008	1020	1048	rBV	118311	284482	26.35%	3.283%
28	4.999	1131	1138	1141	rBB3	421	456	0.04%	0.005%
29	5.067	1141	1159	1181	rBV	206558	453266	41.98%	5.231%
30	5.263	1217	1220	1222	rVB2	312	149	0.01%	0.002%
31	5.288	1225	1228	1232	rBV2	468	338	0.03%	0.004%
32	5.340	1240	1244	1247	rBV	282	241	0.02%	0.003%
33	5.395	1258	1261	1266	rBV	301	297	0.03%	0.003%
34	5.430	1266	1272	1275	rBV2	557	593	0.05%	0.007%
35	5.520	1297	1300	1303	rBV	191	197	0.02%	0.002%
36	5.568	1309	1315	1316	rBV	383	321	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048547.D
 Acq On : 12 May 2022 17:24
 Operator : SY/MD
 Sample : N2767-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1388	rBV2	389865	1079620	100.00%	12.458%
38	5.977	1439	1442	1443	rBV	348	204	0.02%	0.002%
39	6.051	1462	1465	1469	rVV3	404	309	0.03%	0.004%
40	6.099	1478	1480	1483	rBV2	146	126	0.01%	0.001%
41	6.134	1488	1491	1492	rBV	232	133	0.01%	0.002%
42	6.173	1497	1503	1510	rBV3	589	741	0.07%	0.009%
43	6.250	1510	1527	1549	rBV	341708	641852	59.45%	7.407%
44	6.530	1605	1614	1625	rVB2	5670	9696	0.90%	0.112%
45	6.690	1650	1664	1685	rBV	247980	484687	44.89%	5.593%
46	6.838	1708	1710	1713	rVB2	422	170	0.02%	0.002%
47	6.903	1727	1730	1732	rBV2	401	154	0.01%	0.002%
48	6.928	1735	1738	1740	rBV	174	120	0.01%	0.001%
49	6.993	1756	1758	1761	rVB	208	114	0.01%	0.001%
50	7.018	1761	1766	1769	rBV2	281	267	0.02%	0.003%
51	7.047	1772	1775	1777	rBV	385	230	0.02%	0.003%
52	7.224	1828	1830	1831	rBV	259	113	0.01%	0.001%
53	7.272	1839	1845	1850	rBV2	335	549	0.05%	0.006%
54	7.327	1860	1862	1866	rVB2	334	224	0.02%	0.003%
55	7.343	1866	1867	1870	rBV	226	129	0.01%	0.001%
56	7.398	1881	1884	1888	rBV	243	236	0.02%	0.003%
57	7.443	1894	1898	1901	rBV	228	169	0.02%	0.002%
58	7.485	1909	1911	1914	rBV	273	134	0.01%	0.002%
59	7.565	1924	1936	1954	rBV	143269	250327	23.19%	2.889%
60	7.690	1969	1975	1980	rBV5	1760	2425	0.22%	0.028%
61	7.835	2018	2020	2022	rVB	285	112	0.01%	0.001%
62	7.899	2025	2040	2055	rBV	498208	856703	79.35%	9.886%
63	8.179	2115	2127	2144	rBV	104692	178718	16.55%	2.062%
64	8.452	2208	2212	2214	rBV2	532	435	0.04%	0.005%
65	8.468	2214	2217	2225	rVB4	978	1155	0.11%	0.013%
66	8.632	2255	2268	2294	rBV	353367	644254	59.67%	7.434%
67	8.803	2320	2321	2323	rBV	344	151	0.01%	0.002%
68	8.877	2341	2344	2347	rBV	376	344	0.03%	0.004%
69	8.996	2379	2381	2387	rBV2	202	178	0.02%	0.002%
70	9.118	2415	2419	2420	rBV2	150	113	0.01%	0.001%
71	9.153	2426	2430	2433	rBV2	278	293	0.03%	0.003%
72	9.275	2464	2468	2469	rBV	258	185	0.02%	0.002%
73	9.324	2481	2483	2485	rBV2	214	122	0.01%	0.001%
74	9.417	2499	2512	2551	rBV	495619	826529	76.56%	9.538%
75	9.632	2576	2579	2585	rVB2	294	292	0.03%	0.003%
76	9.960	2678	2681	2684	rBV	256	153	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048547.D
 Acq On : 12 May 2022 17:24
 Operator : SY/MD
 Sample : N2767-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.976	2684	2686	2689	rVB2	390	203	0.02%	0.002%
78	10.009	2693	2696	2700	rBV2	291	191	0.02%	0.002%
79	10.176	2745	2748	2750	rBV	207	110	0.01%	0.001%
80	10.317	2790	2792	2796	rVB	295	188	0.02%	0.002%
81	10.372	2806	2809	2815	rBV2	304	318	0.03%	0.004%
82	10.529	2855	2858	2859	rBV	213	121	0.01%	0.001%
83	10.668	2895	2901	2905	rBV3	1467	1537	0.14%	0.018%
84	10.758	2916	2929	2948	rVB	374699	602539	55.81%	6.953%
85	10.838	2951	2954	2956	rVB	269	142	0.01%	0.002%
86	10.854	2956	2959	2962	rVB	248	121	0.01%	0.001%
87	10.870	2962	2964	2965	rBV	460	223	0.02%	0.003%
88	10.886	2966	2969	2970	rBV2	1158	652	0.06%	0.008%
89	10.992	2997	3002	3004	rBV	345	309	0.03%	0.004%
90	11.063	3019	3024	3027	rBV	426	376	0.03%	0.004%
91	11.452	3142	3145	3146	rBV2	722	423	0.04%	0.005%
92	11.812	3243	3257	3281	rBV	538819	858088	79.48%	9.902%
93	11.973	3303	3307	3312	rVB2	1239	846	0.08%	0.010%
94	12.079	3338	3340	3343	rBV2	301	168	0.02%	0.002%
95	12.192	3361	3375	3394	rBV	525754	861241	79.77%	9.938%
96	12.906	3593	3597	3599	rBV	336	278	0.03%	0.003%
97	13.015	3623	3631	3646	rBV4	8682	16206	1.50%	0.187%
98	13.259	3704	3707	3711	rBV2	320	249	0.02%	0.003%
99	13.359	3734	3738	3741	rBV	450	454	0.04%	0.005%
100	13.539	3792	3794	3798	rVB2	589	305	0.03%	0.004%




Sum of corrected areas: 8665823

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048547.D
Acq On : 12 May 2022 17:24
Operator : SY/MD
Sample : N2767-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

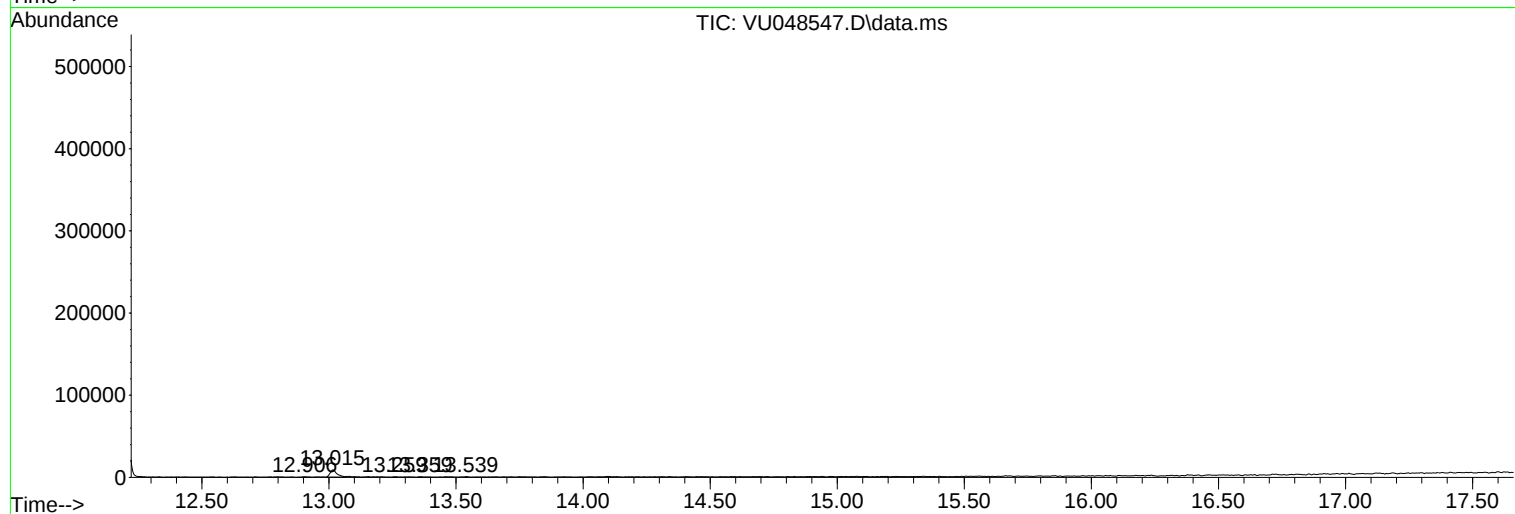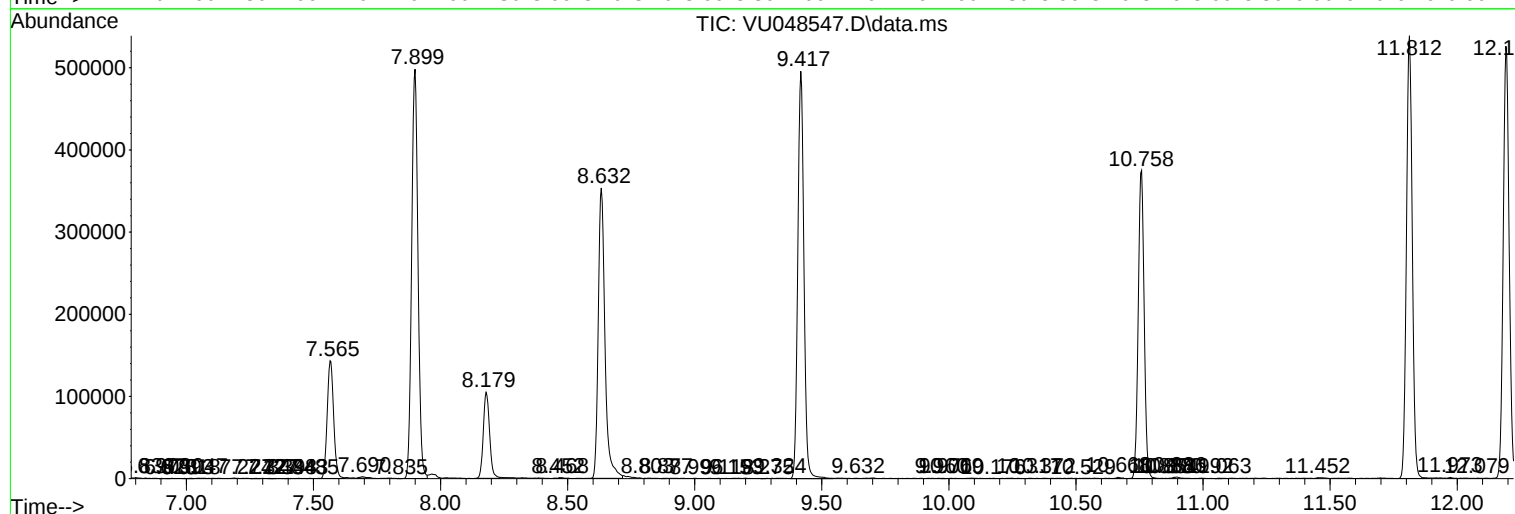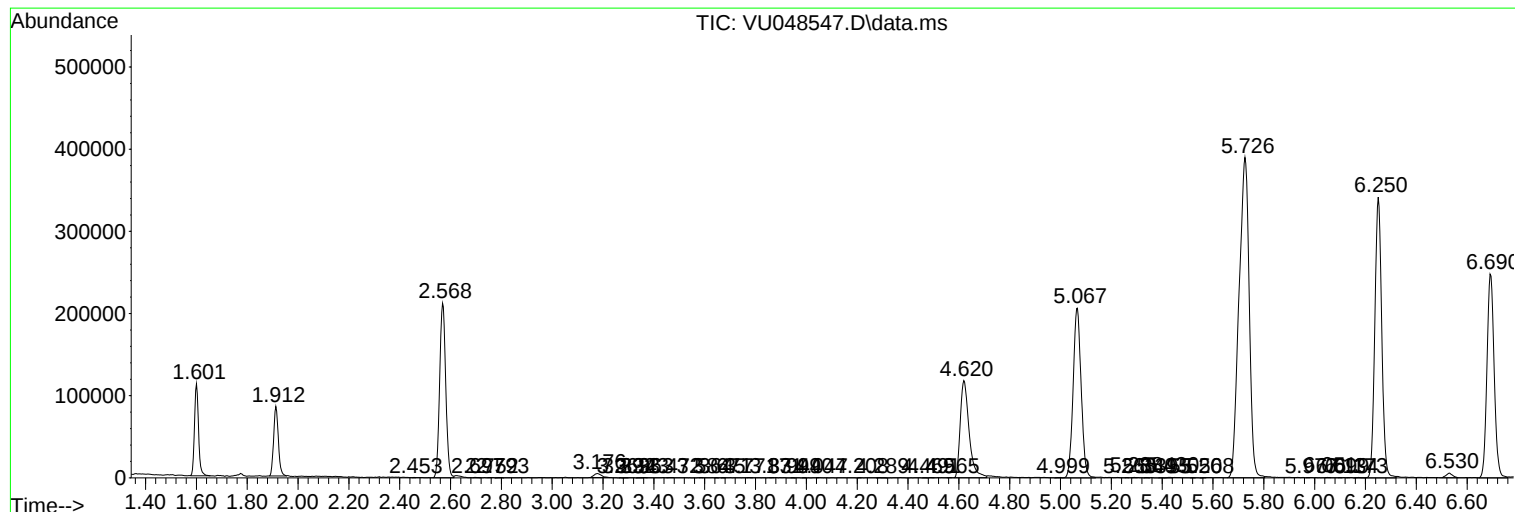

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048547.D
Acq On : 12 May 2022 17:24
Operator : SY/MD
Sample : N2767-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048547.D
Acq On : 12 May 2022 17:24
Operator : SY/MD
Sample : N2767-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------