

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048548.D
 Acq On : 12 May 2022 17:47
 Operator : SY/MD
 Sample : N2767-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rVB	106409	121650	11.33%	1.414%
2	1.684	102	107	116	rVB	14777	16733	1.56%	0.195%
3	1.912	170	178	193	rVB	82989	107877	10.05%	1.254%
4	2.568	369	382	394	rBV	208364	341152	31.77%	3.966%
5	2.755	431	440	450	rBV2	6969	13269	1.24%	0.154%
6	2.922	490	492	493	rBV2	371	185	0.02%	0.002%
7	3.176	566	571	574	rBV2	1047	1194	0.11%	0.014%
8	3.263	595	598	601	rBV	207	142	0.01%	0.002%
9	3.369	627	631	632	rBV	241	139	0.01%	0.002%
10	3.378	632	634	638	rVV	347	232	0.02%	0.003%
11	3.398	638	640	643	rVV	295	202	0.02%	0.002%
12	3.417	643	646	649	rVB2	315	188	0.02%	0.002%
13	3.488	665	668	671	rVB2	305	174	0.02%	0.002%
14	3.636	712	714	717	rVB2	343	216	0.02%	0.003%
15	3.658	718	721	724	rBV2	374	288	0.03%	0.003%
16	3.732	740	744	746	rBV	351	159	0.01%	0.002%
17	3.829	770	774	776	rBV2	396	346	0.03%	0.004%
18	3.989	821	824	828	rBV2	307	218	0.02%	0.003%
19	4.022	830	834	839	rVB2	269	253	0.02%	0.003%
20	4.118	861	864	868	rBB2	245	190	0.02%	0.002%
21	4.141	868	871	874	rBV2	374	327	0.03%	0.004%
22	4.211	891	893	894	rBV2	254	134	0.01%	0.002%
23	4.240	899	902	908	rVV2	328	281	0.03%	0.003%
24	4.269	908	911	915	rVV	208	143	0.01%	0.002%
25	4.353	934	937	940	rVB	226	140	0.01%	0.002%
26	4.404	950	953	956	rVV2	239	149	0.01%	0.002%
27	4.620	1004	1020	1038	rBV	113977	267874	24.95%	3.114%
28	5.063	1142	1158	1184	rBV	205238	468168	43.60%	5.442%
29	5.256	1215	1218	1220	rBV	262	205	0.02%	0.002%
30	5.340	1240	1244	1246	rVB	282	222	0.02%	0.003%
31	5.375	1252	1255	1256	rBV	253	161	0.01%	0.002%
32	5.423	1267	1270	1272	rBV2	226	152	0.01%	0.002%
33	5.449	1274	1278	1279	rBV	284	185	0.02%	0.002%
34	5.513	1295	1298	1302	rVV2	210	179	0.02%	0.002%
35	5.600	1321	1325	1327	rVB	400	264	0.02%	0.003%
36	5.726	1342	1364	1389	rBV2	388353	1073685	100.00%	12.481%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048548.D
 Acq On : 12 May 2022 17:47
 Operator : SY/MD
 Sample : N2767-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.922	1423	1425	1432	rVB3	377	346	0.03%	0.004%
38	6.050	1461	1465	1471	rVB2	467	506	0.05%	0.006%
39	6.076	1471	1473	1475	rBV	304	201	0.02%	0.002%
40	6.105	1480	1482	1487	rVB2	225	133	0.01%	0.002%
41	6.140	1487	1493	1497	rBV4	1021	1289	0.12%	0.015%
42	6.163	1497	1500	1506	rVB2	1142	972	0.09%	0.011%
43	6.192	1506	1509	1512	rVB	251	162	0.02%	0.002%
44	6.250	1512	1527	1549	rBV	333480	626880	58.39%	7.287%
45	6.459	1590	1592	1594	rBV	280	159	0.01%	0.002%
46	6.484	1598	1600	1603	rBV2	277	190	0.02%	0.002%
47	6.526	1603	1613	1622	rBV5	6113	12169	1.13%	0.141%
48	6.690	1648	1664	1685	rBV	246798	481854	44.88%	5.601%
49	6.883	1717	1724	1731	rBV4	2263	3376	0.31%	0.039%
50	6.970	1749	1751	1754	rBV	265	137	0.01%	0.002%
51	7.041	1769	1773	1778	rBV3	414	504	0.05%	0.006%
52	7.160	1803	1810	1813	rBV4	1368	1722	0.16%	0.020%
53	7.346	1864	1868	1872	rBV2	209	180	0.02%	0.002%
54	7.436	1892	1896	1898	rBV2	321	233	0.02%	0.003%
55	7.568	1923	1937	1954	rBV	137824	250227	23.31%	2.909%
56	7.697	1974	1977	1980	rBV4	965	883	0.08%	0.010%
57	7.790	2001	2006	2008	rBV	258	234	0.02%	0.003%
58	7.899	2026	2040	2056	rBV	491319	841242	78.35%	9.779%
59	8.102	2100	2103	2107	rVB2	447	278	0.03%	0.003%
60	8.179	2116	2127	2146	rBV	105286	178726	16.65%	2.078%
61	8.427	2201	2204	2206	rBV	209	153	0.01%	0.002%
62	8.443	2206	2209	2210	rVV2	652	388	0.04%	0.005%
63	8.475	2211	2219	2232	rVB3	5307	9039	0.84%	0.105%
64	8.545	2240	2241	2244	rVB2	406	192	0.02%	0.002%
65	8.632	2256	2268	2297	rBV	342504	631359	58.80%	7.339%
66	8.938	2361	2363	2365	rBV2	264	132	0.01%	0.002%
67	9.076	2403	2406	2407	rBV	306	205	0.02%	0.002%
68	9.250	2458	2460	2462	rBV	233	146	0.01%	0.002%
69	9.330	2482	2485	2490	rVB2	241	180	0.02%	0.002%
70	9.356	2490	2493	2496	rBV	310	248	0.02%	0.003%
71	9.417	2499	2512	2538	rBV	480625	802468	74.74%	9.328%
72	9.562	2553	2557	2558	rBV	445	295	0.03%	0.003%
73	9.639	2579	2581	2589	rVB2	251	241	0.02%	0.003%
74	9.684	2589	2595	2597	rBV4	1491	1399	0.13%	0.016%
75	9.787	2624	2627	2630	rBV2	201	139	0.01%	0.002%
76	10.037	2702	2705	2709	rVB2	290	207	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048548.D
 Acq On : 12 May 2022 17:47
 Operator : SY/MD
 Sample : N2767-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	10.127	2730	2733	2734	rBV	390	227	0.02%	0.003%
78	10.243	2762	2769	2776	rVB3	755	1059	0.10%	0.012%
79	10.343	2795	2800	2808	rVV5	1484	2336	0.22%	0.027%
80	10.372	2808	2809	2813	rVB	618	231	0.02%	0.003%
81	10.703	2909	2912	2915	rBV	266	273	0.03%	0.003%
82	10.758	2916	2929	2945	rVV	368078	597680	55.67%	6.948%
83	10.896	2960	2972	2985	rBV3	6086	10884	1.01%	0.127%
84	11.005	3003	3006	3009	rBV2	502	483	0.04%	0.006%
85	11.147	3048	3050	3051	rBV2	318	133	0.01%	0.002%
86	11.462	3141	3148	3158	rBV6	1781	2846	0.27%	0.033%
87	11.578	3181	3184	3190	rBV3	351	389	0.04%	0.005%
88	11.629	3195	3200	3208	rVV3	1041	1358	0.13%	0.016%
89	11.693	3212	3220	3232	rVB5	9869	15014	1.40%	0.175%
90	11.812	3244	3257	3277	rBV	525431	841646	78.39%	9.783%
91	12.031	3323	3325	3328	rVB	292	158	0.01%	0.002%
92	12.066	3334	3336	3346	rVB2	858	970	0.09%	0.011%
93	12.192	3362	3375	3394	rBV	516128	844594	78.66%	9.818%
94	12.317	3412	3414	3417	rBV2	304	214	0.02%	0.002%
95	12.590	3496	3499	3503	rBV3	410	365	0.03%	0.004%
96	12.658	3518	3520	3522	rBV	323	165	0.02%	0.002%
97	12.680	3523	3527	3530	rVV2	1120	1003	0.09%	0.012%
98	12.893	3585	3593	3607	rBV4	9009	13577	1.26%	0.158%
99	13.002	3622	3627	3628	rBV	516	394	0.04%	0.005%
100	13.442	3761	3764	3766	rBV2	349	244	0.02%	0.003%




Sum of corrected areas: 8602713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048548.D
Acq On : 12 May 2022 17:47
Operator : SY/MD
Sample : N2767-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

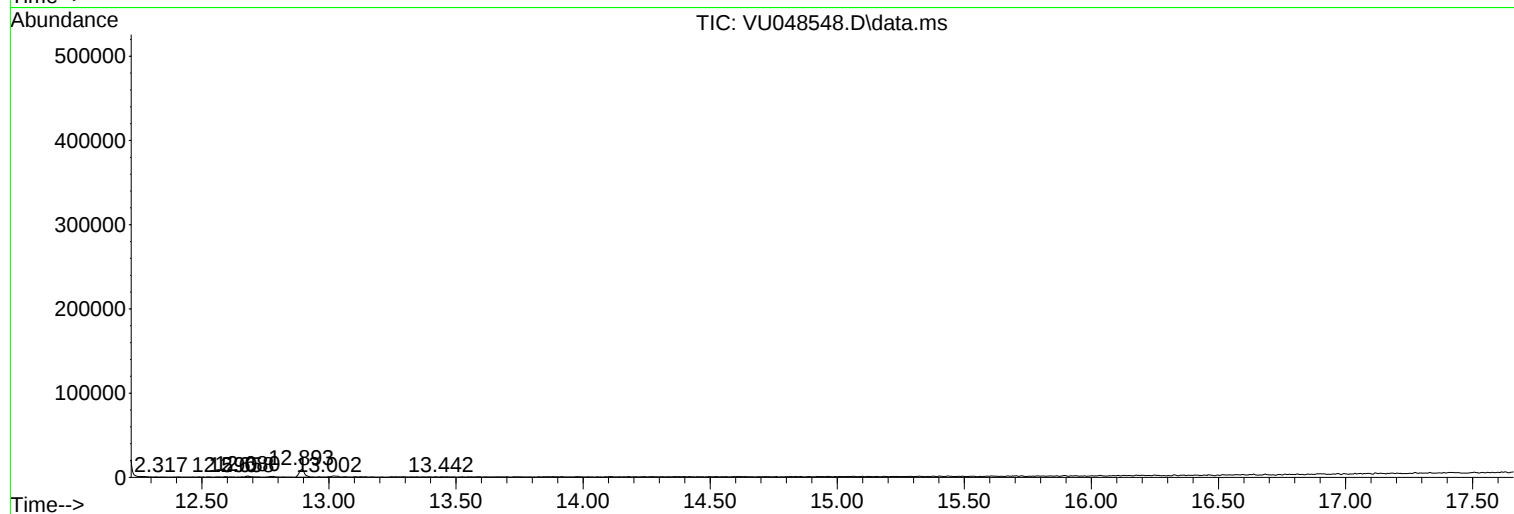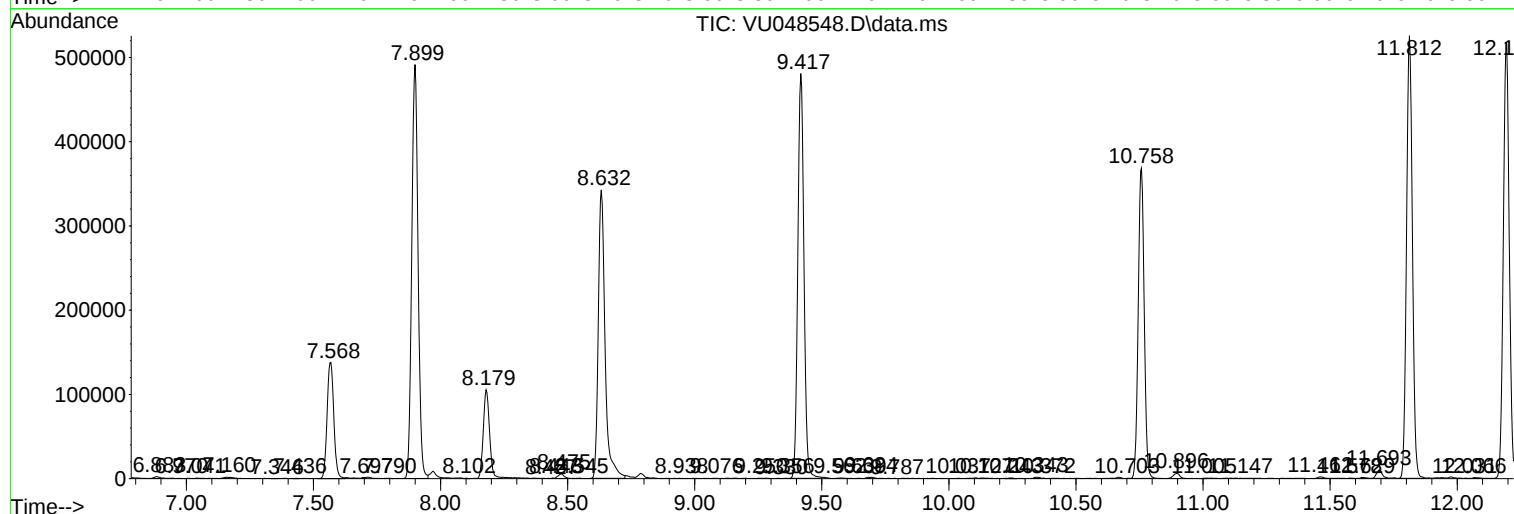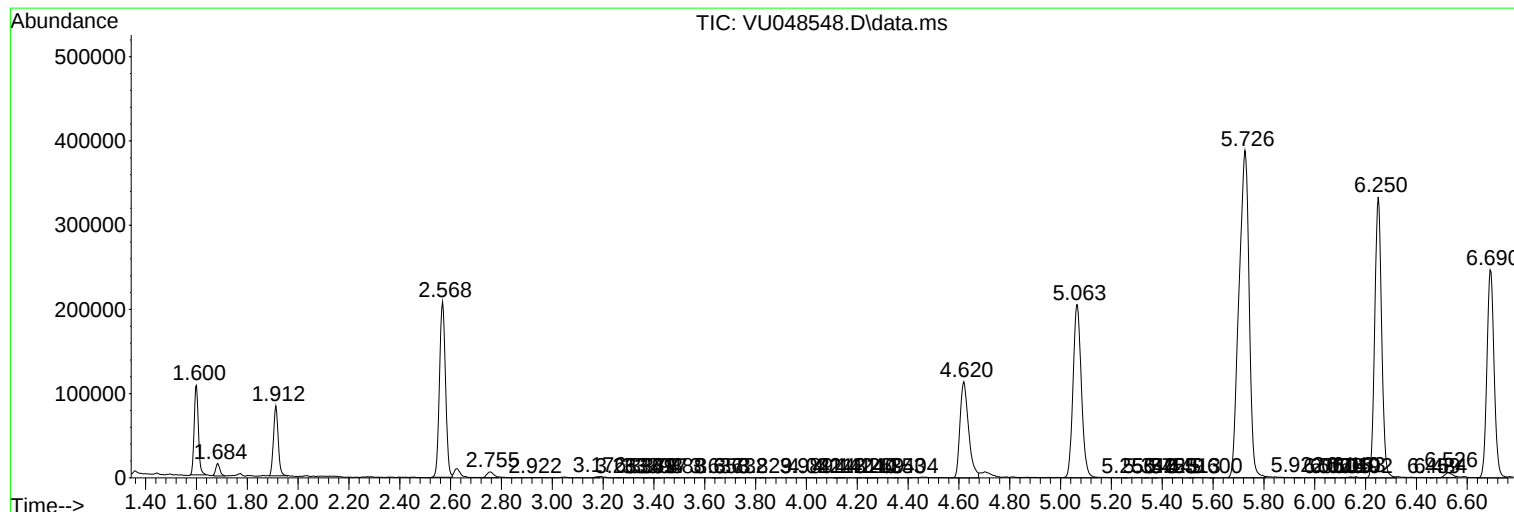

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048548.D
Acq On : 12 May 2022 17:47
Operator : SY/MD
Sample : N2767-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048548.D
Acq On : 12 May 2022 17:47
Operator : SY/MD
Sample : N2767-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc