

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048551.D
 Acq On : 12 May 2022 18:58
 Operator : SY/MD
 Sample : N2767-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rVB	103421	120769	11.65%	1.440%
2	1.912	170	178	192	rBV	82510	105139	10.15%	1.253%
3	2.253	281	284	285	rBV2	691	444	0.04%	0.005%
4	2.568	368	382	394	rBV	204368	333762	32.21%	3.979%
5	2.690	417	420	423	rBV	327	263	0.03%	0.003%
6	2.752	431	439	440	rBV2	2391	2139	0.21%	0.025%
7	3.192	563	576	583	rBV4	1359	2914	0.28%	0.035%
8	3.289	601	606	609	rVB	281	269	0.03%	0.003%
9	3.327	615	618	622	rVB3	340	265	0.03%	0.003%
10	3.362	626	629	631	rBV	290	196	0.02%	0.002%
11	3.420	643	647	655	rVB2	416	508	0.05%	0.006%
12	3.571	691	694	695	rBV	256	170	0.02%	0.002%
13	3.600	701	703	709	rVB2	584	482	0.05%	0.006%
14	3.629	709	712	714	rBV	293	212	0.02%	0.003%
15	3.668	721	724	731	rVB2	298	370	0.04%	0.004%
16	3.700	732	734	737	rBV2	350	251	0.02%	0.003%
17	3.739	742	746	749	rBV2	235	200	0.02%	0.002%
18	3.935	804	807	810	rBV2	333	313	0.03%	0.004%
19	3.970	816	818	821	rVB	286	161	0.02%	0.002%
20	4.012	824	831	833	rBV2	367	432	0.04%	0.005%
21	4.063	844	847	851	rBV	302	186	0.02%	0.002%
22	4.131	866	868	873	rBV2	279	286	0.03%	0.003%
23	4.285	913	916	918	rBV	275	195	0.02%	0.002%
24	4.353	935	937	939	rBV	278	196	0.02%	0.002%
25	4.456	962	969	972	rBV3	792	1126	0.11%	0.013%
26	4.620	1005	1020	1041	rBV	113036	266000	25.67%	3.171%
27	5.063	1141	1158	1182	rBV	201748	460704	44.46%	5.492%
28	5.227	1205	1209	1210	rBV	325	249	0.02%	0.003%
29	5.288	1224	1228	1232	rBV3	585	667	0.06%	0.008%
30	5.353	1243	1248	1249	rBV2	247	160	0.02%	0.002%
31	5.504	1291	1295	1298	rBV2	273	243	0.02%	0.003%
32	5.594	1319	1323	1329	rVB	397	418	0.04%	0.005%
33	5.626	1330	1333	1336	rBV	220	191	0.02%	0.002%
34	5.726	1343	1364	1393	rVV2	378286	1036307	100.00%	12.353%
35	5.886	1412	1414	1416	rBV	363	192	0.02%	0.002%
36	6.002	1448	1450	1451	rBV	365	181	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048551.D
 Acq On : 12 May 2022 18:58
 Operator : SY/MD
 Sample : N2767-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	6.079	1471	1474	1477	rBV	235	203	0.02%	0.002%
38	6.124	1486	1488	1490	rBV	349	178	0.02%	0.002%
39	6.150	1494	1496	1499	rVB2	786	487	0.05%	0.006%
40	6.250	1510	1527	1553	rBV	331726	631225	60.91%	7.525%
41	6.443	1584	1587	1589	rBV	208	165	0.02%	0.002%
42	6.526	1602	1613	1623	rBV8	3219	7043	0.68%	0.084%
43	6.694	1650	1665	1682	rBV	237363	467840	45.14%	5.577%
44	6.880	1718	1723	1724	rBV3	2235	1510	0.15%	0.018%
45	6.993	1753	1758	1763	rBV2	410	445	0.04%	0.005%
46	7.163	1801	1811	1814	rBV4	1574	2560	0.25%	0.031%
47	7.247	1834	1837	1840	rBV2	273	183	0.02%	0.002%
48	7.378	1875	1878	1881	rBV	457	327	0.03%	0.004%
49	7.485	1909	1911	1913	rVB2	266	145	0.01%	0.002%
50	7.510	1914	1919	1920	rBV	271	218	0.02%	0.003%
51	7.565	1924	1936	1955	rBV	136494	240708	23.23%	2.869%
52	7.706	1978	1980	1982	rBV2	566	291	0.03%	0.003%
53	7.899	2026	2040	2057	rBV	474511	814847	78.63%	9.713%
54	8.131	2110	2112	2116	rBV2	258	196	0.02%	0.002%
55	8.179	2116	2127	2146	rBV	102156	171194	16.52%	2.041%
56	8.407	2194	2198	2201	rBV3	317	318	0.03%	0.004%
57	8.427	2201	2204	2207	rVV	543	373	0.04%	0.004%
58	8.475	2211	2219	2230	rVB2	4204	6755	0.65%	0.081%
59	8.520	2231	2233	2236	rVB	470	179	0.02%	0.002%
60	8.552	2241	2243	2246	rVB	590	271	0.03%	0.003%
61	8.568	2246	2248	2251	rBV	323	145	0.01%	0.002%
62	8.632	2256	2268	2300	rBV	335341	623784	60.19%	7.436%
63	9.079	2404	2407	2410	rBV	252	163	0.02%	0.002%
64	9.156	2428	2431	2433	rBV	270	168	0.02%	0.002%
65	9.253	2456	2461	2462	rBV2	231	207	0.02%	0.002%
66	9.417	2499	2512	2544	rBV	470237	788362	76.07%	9.398%
67	9.645	2577	2583	2586	rVB3	448	451	0.04%	0.005%
68	9.693	2591	2598	2605	rVB3	2103	2701	0.26%	0.032%
69	9.745	2611	2614	2617	rVB2	304	218	0.02%	0.003%
70	10.137	2730	2736	2741	rBV3	648	749	0.07%	0.009%
71	10.189	2749	2752	2755	rBV	300	218	0.02%	0.003%
72	10.346	2795	2801	2808	rBV5	1959	2385	0.23%	0.028%
73	10.610	2880	2883	2886	rBV	214	204	0.02%	0.002%
74	10.658	2896	2898	2899	rBV	451	244	0.02%	0.003%
75	10.758	2916	2929	2946	rBV	366141	591375	57.07%	7.050%
76	10.893	2963	2971	2984	rVB2	5451	8141	0.79%	0.097%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048551.D
 Acq On : 12 May 2022 18:58
 Operator : SY/MD
 Sample : N2767-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	11.111	3034	3039	3043	rBV3	537	525	0.05%	0.006%
78	11.176	3057	3059	3064	rVB	369	247	0.02%	0.003%
79	11.330	3104	3107	3109	rBV2	263	185	0.02%	0.002%
80	11.459	3144	3147	3149	rBV	686	511	0.05%	0.006%
81	11.693	3212	3220	3230	rBV6	8182	13777	1.33%	0.164%
82	11.751	3235	3238	3243	rBV4	738	647	0.06%	0.008%
83	11.812	3244	3257	3279	rBV	515822	825090	79.62%	9.836%
84	11.938	3292	3296	3301	rVB3	987	769	0.07%	0.009%
85	12.073	3335	3338	3341	rBV3	637	534	0.05%	0.006%
86	12.115	3348	3351	3353	rBV	378	205	0.02%	0.002%
87	12.192	3363	3375	3393	rBV	509376	825917	79.70%	9.845%
88	12.397	3437	3439	3443	rBV2	357	258	0.02%	0.003%
89	12.471	3459	3462	3465	rBV2	478	267	0.03%	0.003%
90	12.680	3525	3527	3531	rVB3	711	457	0.04%	0.005%
91	12.722	3537	3540	3543	rBV2	314	239	0.02%	0.003%
92	12.832	3571	3574	3576	rBV	268	204	0.02%	0.002%
93	12.893	3586	3593	3604	rVB4	8665	12617	1.22%	0.150%
94	13.134	3664	3668	3669	rBV	344	261	0.03%	0.003%
95	13.369	3739	3741	3744	rBV	383	315	0.03%	0.004%
96	13.407	3750	3753	3758	rVB2	504	503	0.05%	0.006%
97	13.542	3791	3795	3798	rBV	501	352	0.03%	0.004%
98	13.758	3859	3862	3865	rBV2	542	299	0.03%	0.004%
99	14.240	4009	4012	4017	rBV3	586	501	0.05%	0.006%
100	14.336	4039	4042	4045	rBV2	601	433	0.04%	0.005%




Sum of corrected areas: 8388849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048551.D
Acq On : 12 May 2022 18:58
Operator : SY/MD
Sample : N2767-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

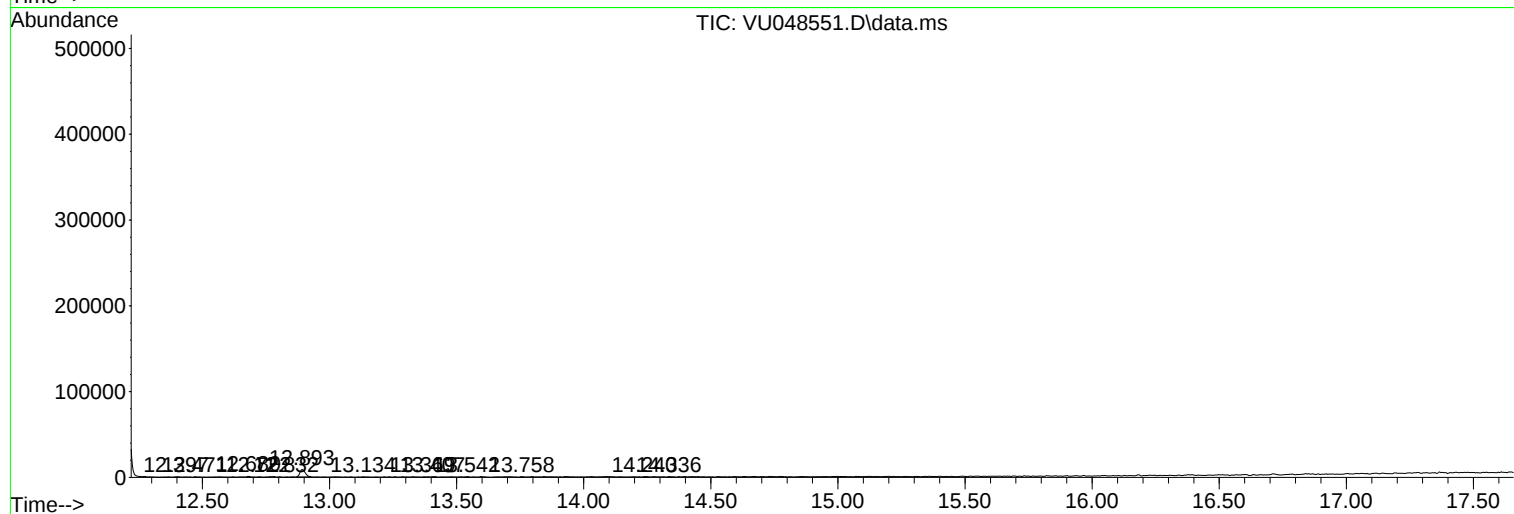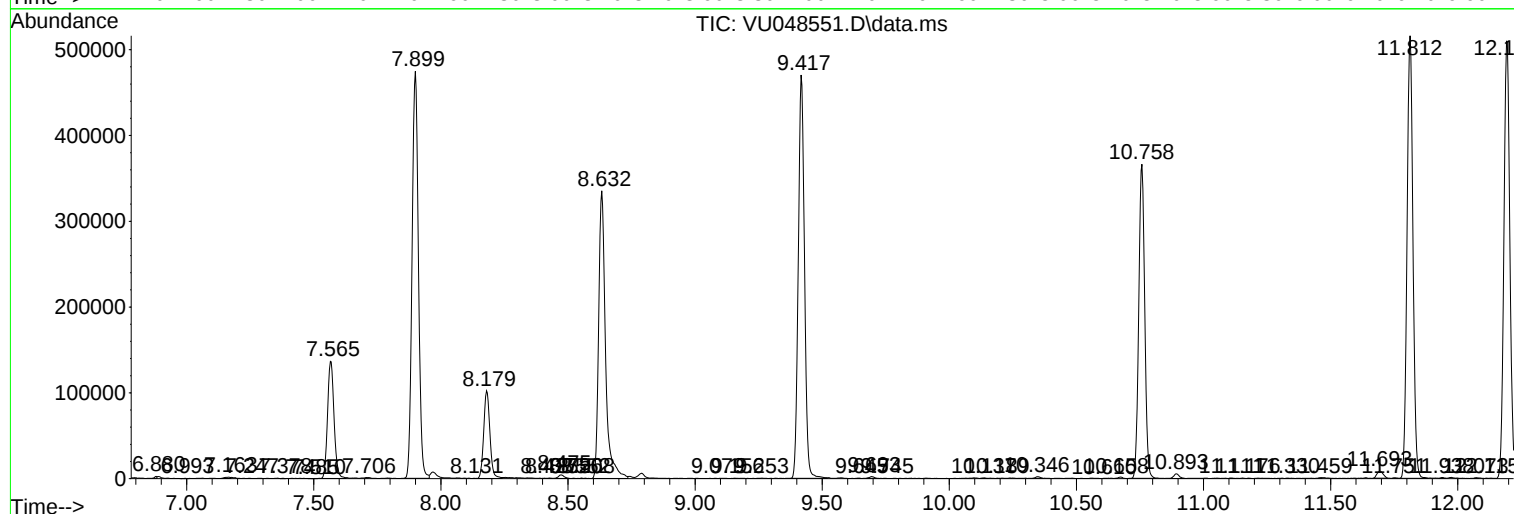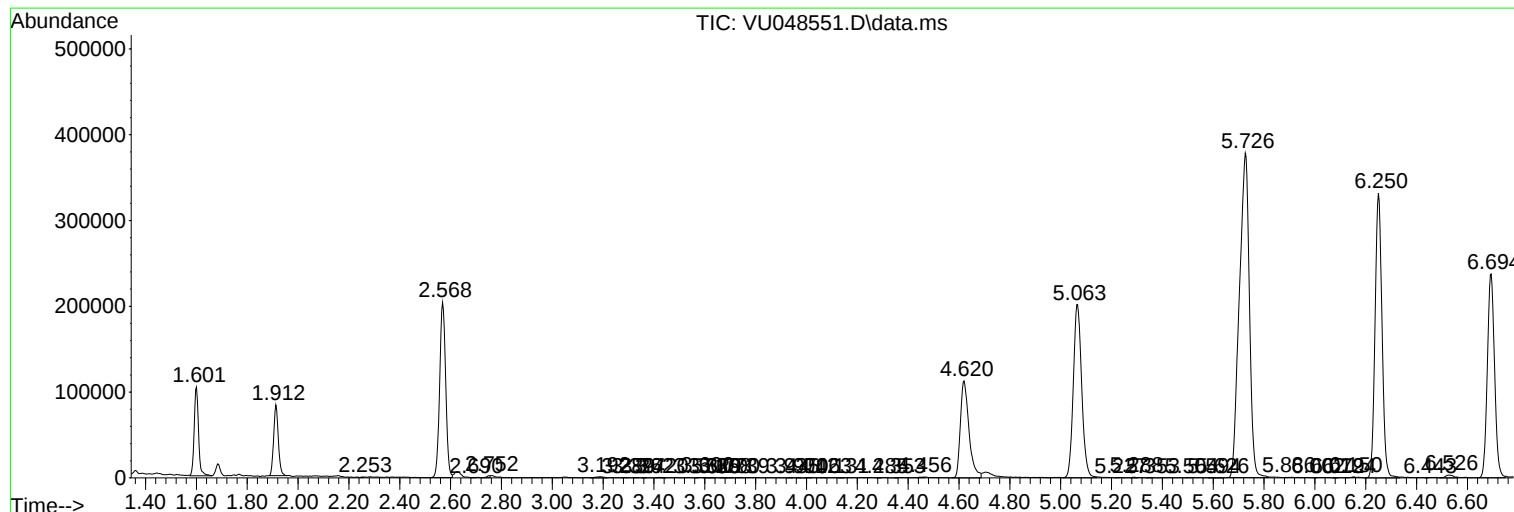

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048551.D
Acq On : 12 May 2022 18:58
Operator : SY/MD
Sample : N2767-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
Data File : VU048551.D
Acq On : 12 May 2022 18:58
Operator : SY/MD
Sample : N2767-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------