


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051222\
 Data File : VU048529.D
 Acq On : 12 May 2022 09:31
 Operator : SY/MD
 Sample : BFB085
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB085

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis
 Last Update : Fri May 13 03:54:05 2022

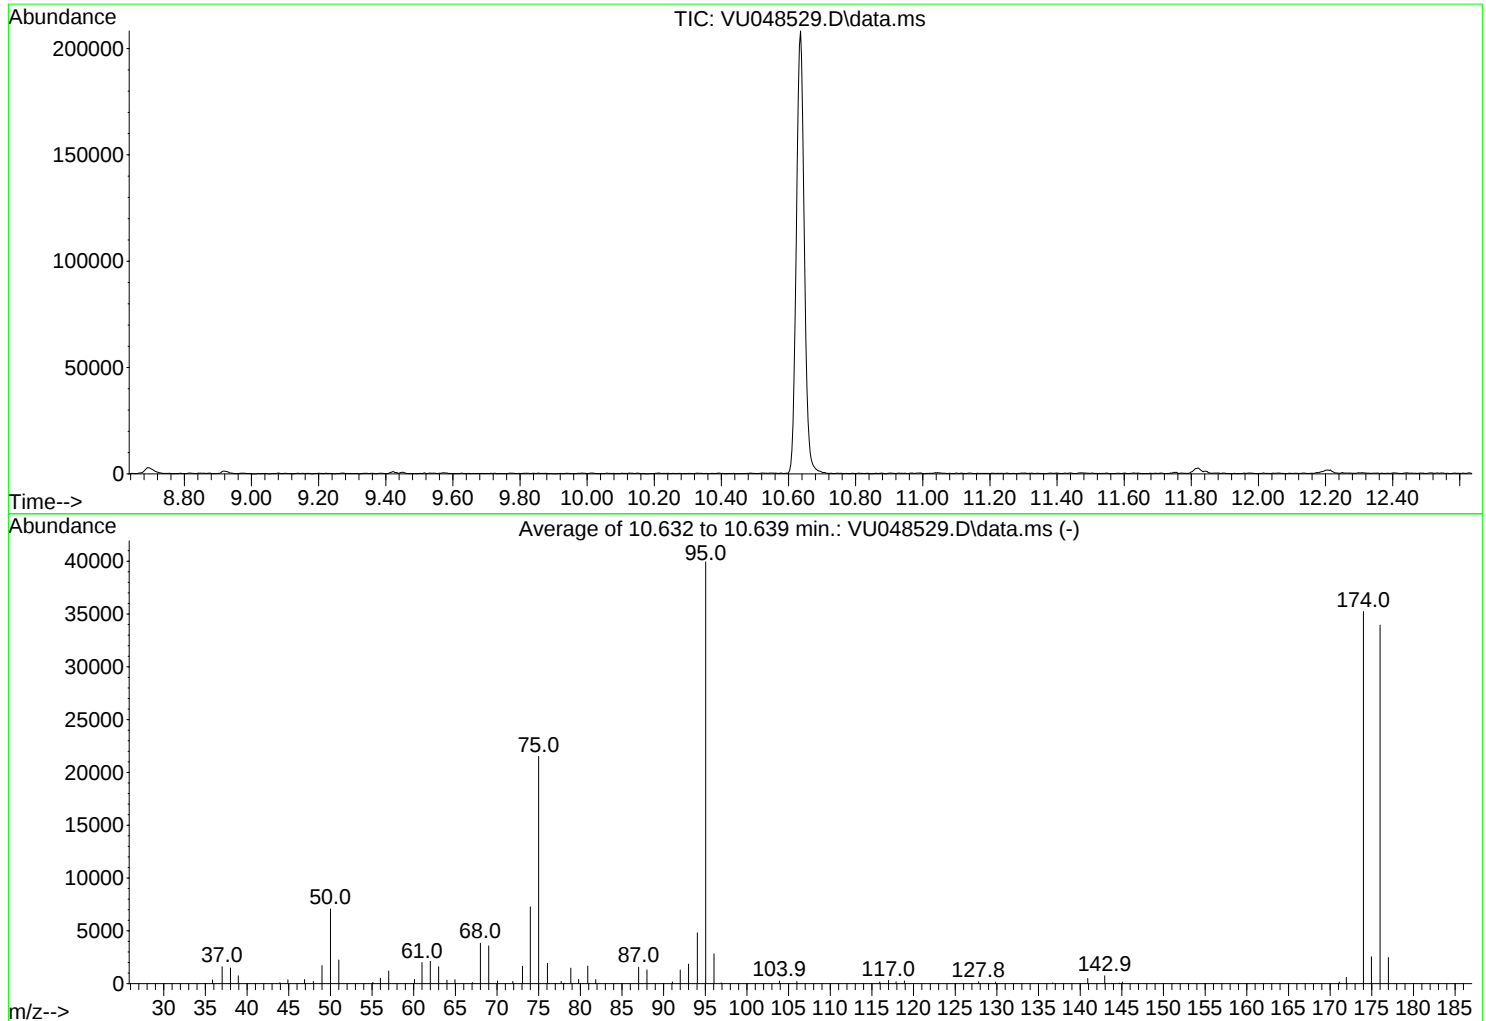

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7081	PASS
75	95	30	80	53.9	21515	PASS
95	95	100	100	100.0	39944	PASS
96	95	5	9	7.0	2816	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.2	35240	PASS
175	174	5	9	7.2	2552	PASS
176	174	95	101	96.3	33952	PASS
177	176	5	9	7.3	2470	PASS

m/z	Abundance
35.80	371.0
37.00	1659.0
38.00	1540.0
38.90	767.0
44.00	314.0
44.90	370.0
46.90	342.0
48.00	220.0
49.00	1512.0
50.00	7421.0
51.00	2289.0
56.00	535.0
57.00	1169.0
60.10	395.0
61.00	1967.0
62.00	1994.0
63.00	1602.0
64.00	332.0
64.90	358.0
68.00	3804.0
69.00	3626.0
70.00	240.0
71.90	250.0
73.10	1732.0
74.00	7324.0
75.00	21160.0
76.10	2007.0
77.70	183.0
78.10	135.0
78.80	1491.0
79.80	486.0
80.90	1670.0
81.90	376.0
87.00	1377.0
88.00	1345.0
91.10	203.0
92.00	1289.0
93.00	1945.0
94.00	4814.0
95.10	40472.0
96.00	2771.0
96.90	130.0
103.90	245.0
106.00	178.0
115.90	149.0
117.00	318.0
117.90	214.0
118.90	278.0
127.80	195.0
129.90	158.0
140.90	481.0
143.00	698.0
143.80	116.0
145.10	254.0
171.10	143.0
171.90	568.0
174.00	35104.0
175.00	2535.0
176.00	33424.0
177.00	2385.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

Scan 2878 (10.594 min): VU048529.D\data.ms
BFB085

m/z	Abundance
39.80	138.0
43.90	218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	332.0
37.00	1516.0
38.00	1366.0
39.00	712.0
40.00	140.0
44.00	295.0
44.90	345.0
46.90	431.0
47.90	212.0
49.00	1865.0
50.00	6475.0
51.00	2136.0
55.10	207.0
56.00	481.0
57.00	1162.0
60.10	378.0
61.00	1977.0
62.00	2138.0
63.00	1603.0
64.00	328.0
65.00	396.0
67.00	166.0
68.00	3771.0
69.00	3527.0
70.10	259.0
71.90	174.0
73.00	1548.0
74.00	6904.0
75.00	21144.0
76.00	1742.0
77.00	106.0
77.70	206.0
78.90	1414.0
79.80	316.0
80.90	1586.0
81.80	402.0
87.00	1648.0
88.00	1204.0
91.00	129.0
92.00	1244.0
93.00	1680.0
94.10	4760.0
95.00	38288.0
96.10	2816.0
103.90	206.0
106.00	209.0
116.00	164.0
117.00	282.0
117.90	154.0
118.90	228.0
127.80	151.0
129.80	150.0
136.70	118.0
140.90	502.0
142.90	763.0
144.70	202.0
171.10	163.0
172.00	583.0
174.00	34408.0
174.90	2443.0
176.00	33344.0
177.00	2451.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.80	367.0
37.00	1642.0
38.00	1529.0
39.00	752.0
44.00	299.0
44.90	377.0
46.90	428.0
48.00	214.0
49.00	1767.0
50.00	7347.0
51.00	2307.0
55.10	152.0
56.00	532.0
57.00	1259.0
60.10	422.0
61.00	2074.0
62.00	2244.0
63.00	1639.0
64.00	357.0
65.00	386.0
67.10	172.0
68.00	3946.0
69.00	3584.0
70.10	257.0
71.90	237.0
73.10	1693.0
74.00	7591.0
75.00	22240.0
76.10	2030.0
77.70	231.0
78.90	1525.0
79.80	418.0
80.90	1744.0
81.80	414.0
87.00	1643.0
88.00	1376.0
91.10	170.0
92.00	1319.0
93.00	1904.0
94.10	4899.0
95.10	41072.0
96.00	2862.0
96.90	120.0
103.90	268.0
106.00	222.0
116.00	180.0
117.00	290.0
117.90	200.0
118.90	280.0
127.80	189.0
129.80	147.0
136.70	103.0
140.90	512.0
143.00	770.0
145.00	209.0
171.10	160.0
172.00	604.0
174.00	36208.0
174.90	2679.0
176.00	35088.0
177.00	2574.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085