

Data File : VU031960.D
Acq On : 13 May 2019 10:25
Operator : JC/SP
Sample : K2744-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D11

Quant Time: May 14 02:41:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 14 02:38:02 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	475898	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	495403	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	189092	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	111272	3.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.60%
7) Chloroethane-d5	1.68	69	119173	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.00%
11) 1,1-Dichloroethene-d2	2.27	63	176733	2.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.60%#
20) 2-Butanone-d5	4.20	46	500445	39.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.04%
24) Chloroform-d	4.64	84	267229	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.40%
26) 1,2-Dichloroethane-d4	5.31	65	149916	3.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.20%
32) Benzene-d6	5.33	84	503197	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.40%
36) 1,2-Dichloropropane-d6	6.32	67	178675	3.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	76.80%
41) Toluene-d8	7.56	98	383991	3.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.80%
43) trans-1,3-Dichloropropene-	7.85	79	55448	3.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.80%
46) 2-Hexanone-d5	8.31	63	370005	44.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.54%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	164321	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	150961	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%

Target Compounds


						Qvalue
22) cis-1,2-Dichloroethene	4.22	96	85024	2.030	ug/L	79
35) Methylcyclohexane	6.33	83	40604	0.649	ug/L #	11
37) 1,2-Dichloropropane	6.32	63	18603	0.376	ug/L #	92
47) Tetrachloroethene	8.22	164	6986	0.247	ug/L	93
48) 2-Hexanone	8.37	43	25765	1.090	ug/L #	87
49) Dibromochloromethane	8.23	129	7479	0.220	ug/L #	10
59) 1,2,3-Trichloropropane	11.48	75	23521	0.804	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU031960.D
Acq On : 13 May 2019 10:25
Operator : JC/SP
Sample : K2744-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9D11

Quant Time: May 14 02:41:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 14 02:38:02 2019
Response via : Initial Calibration

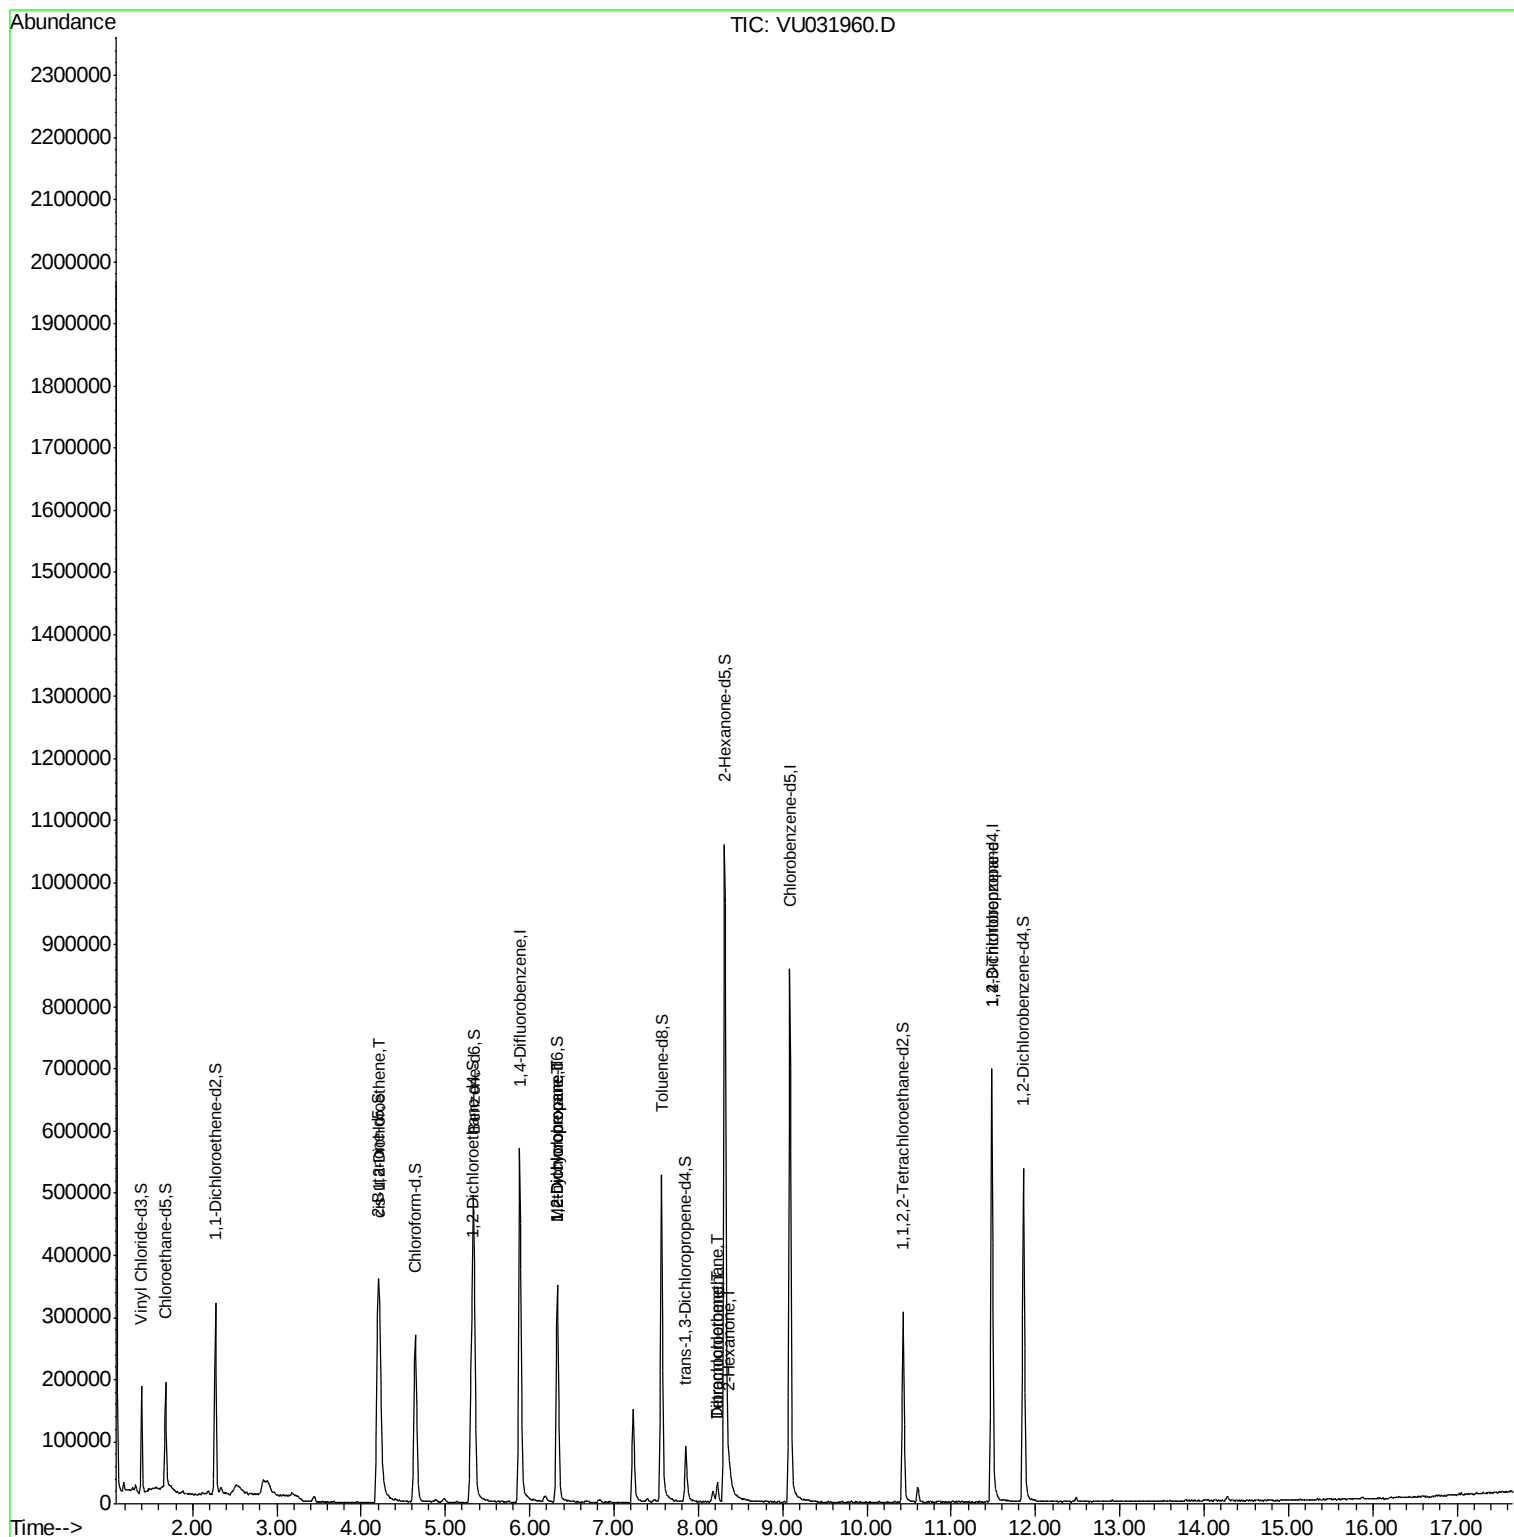




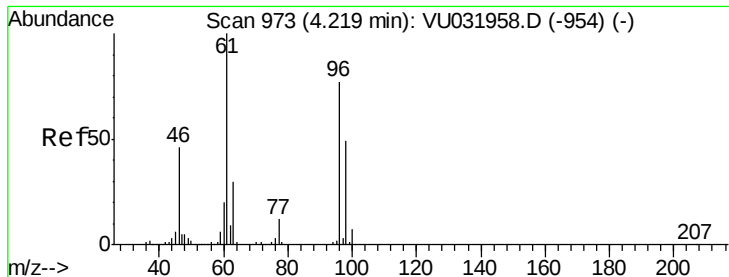


#22

cis-1,2-Dichloroethene
Concen: 2.030 ug/L
RT: 4.22 min Scan# 973
Delta R.T. 0.00 min
Lab File: VU031960.D
Acq: 13 May 2019 10:25

Instrument :
MSVOA_U
ClientSampleId :
F9D11




Tgt Ion: 96 Resp: 85024
Ion Ratio Lower Upper
96 100
61 133.7 113.3 210.5
68 0.0 0.0 0.0

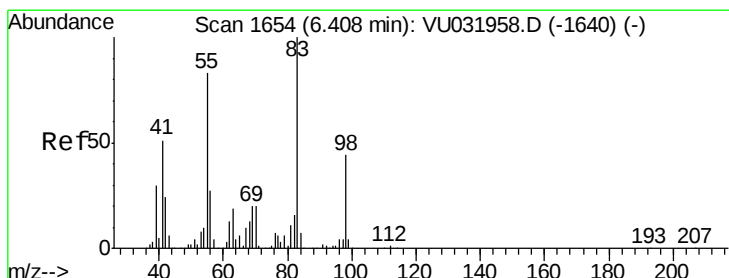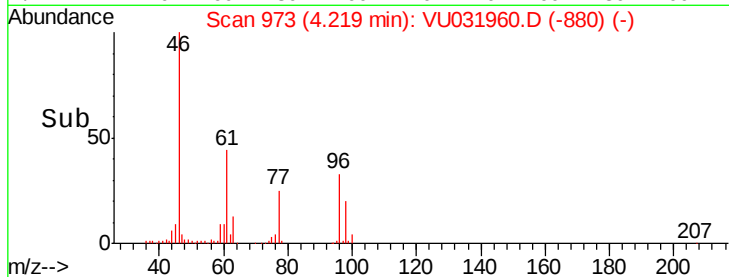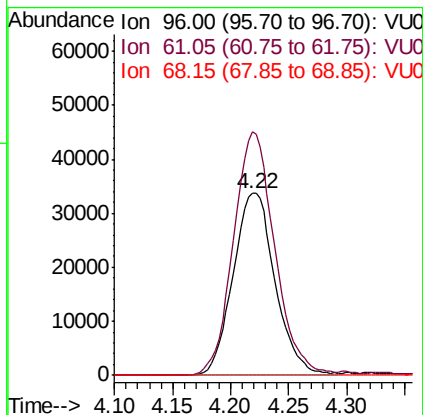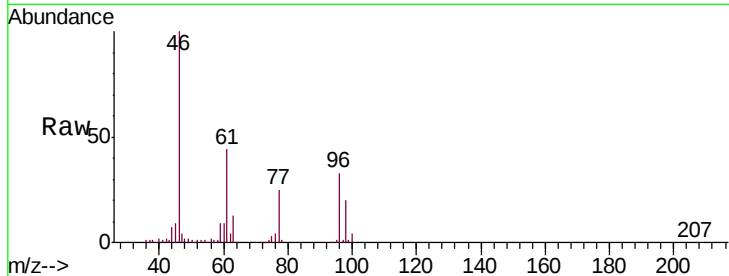


#35

Methylcyclohexane
Concen: 0.649 ug/L
RT: 6.33 min Scan# 1629
Delta R.T. -0.08 min
Lab File: VU031960.D
Acq: 13 May 2019 10:25

Tgt Ion: 83 Resp: 40604
Ion Ratio Lower Upper
83 100
55 0.5 79.2 118.8#
98 0.9 34.0 51.0#


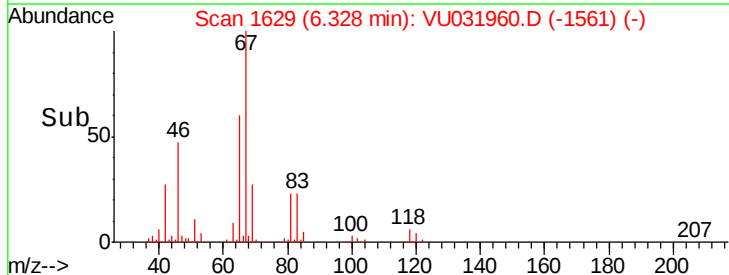
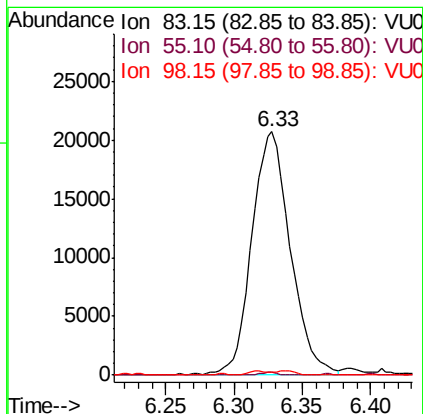
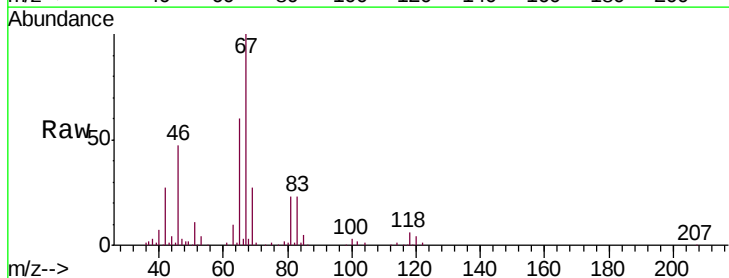


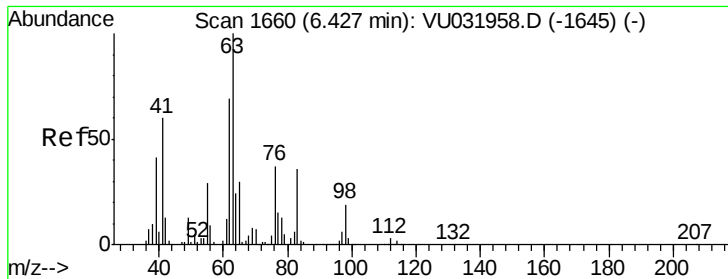

#37
 1,2-Dichloropropane
 Concen: 0.376 ug/L
 RT: 6.32 min Scan# 1628
 Delta R.T. -0.10 min
 Lab File: VU031960.D
 Acq: 13 May 2019 10:25




Instrument :
 MSVOA_U
 ClientSampleId :
 F9D11


Tgt Ion: 63 Resp: 18603
 Ion Ratio Lower Upper
 63 100
 112 0.6 2.5 3.7#

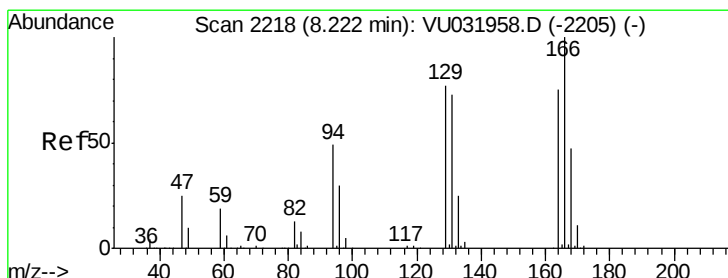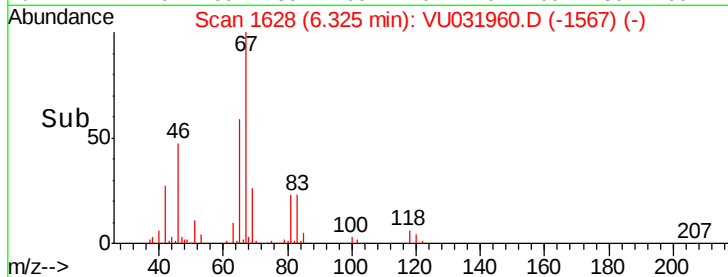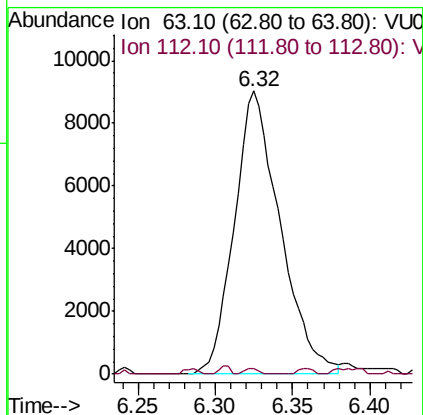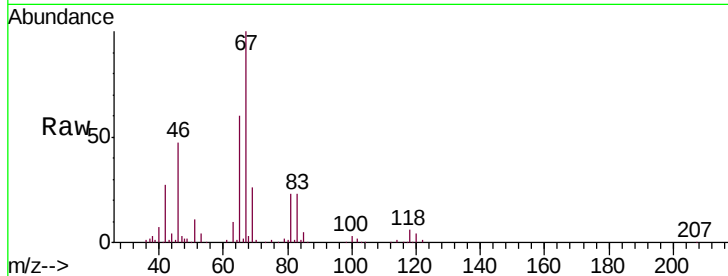

#47
 Tetrachloroethene
 Concen: 0.247 ug/L
 RT: 8.22 min Scan# 2219
 Delta R.T. 0.00 min
 Lab File: VU031960.D
 Acq: 13 May 2019 10:25

Tgt Ion: 164 Resp: 6986
 Ion Ratio Lower Upper
 164 100
 129 89.6 70.3 130.5
 131 101.6 65.4 121.4
 166 126.2 86.0 159.8


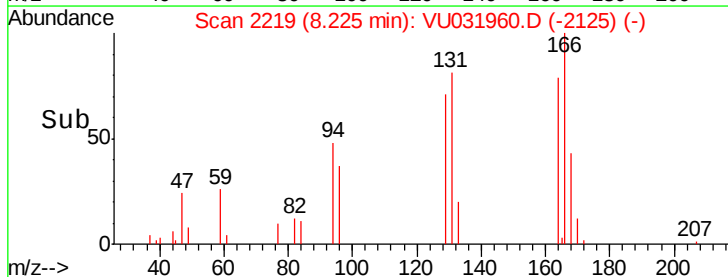
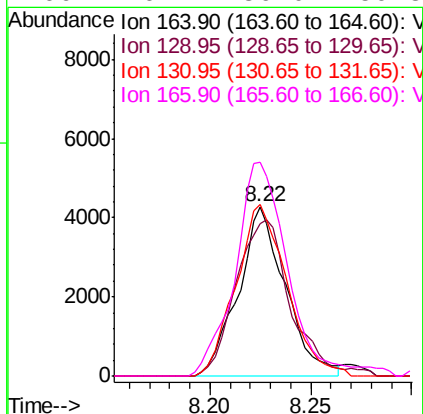
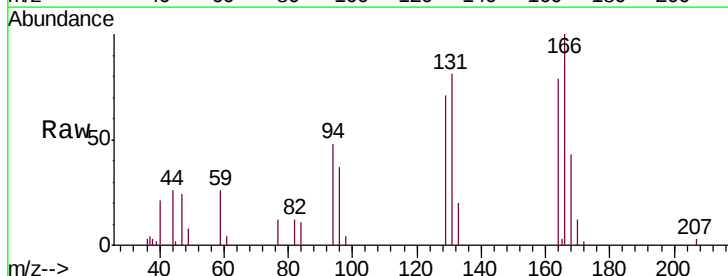


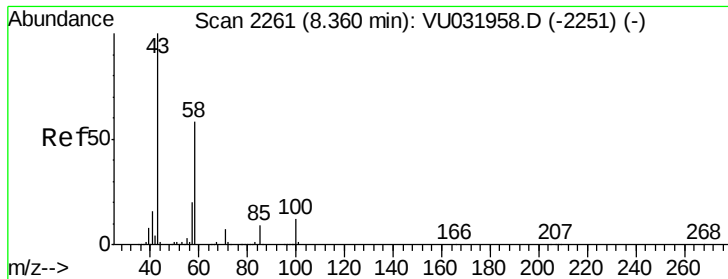

#48
2-Hexanone
Concen: 1.090 ug/L
RT: 8.37 min Scan# 2264
Delta R.T. 0.01 min
Lab File: VU031960.D
Acq: 13 May 2019 10:25




Instrument :
MSVOA_U
ClientSampleId :
F9D11


Tgt Ion: 43 Resp: 25765
Ion Ratio Lower Upper
43 100
58 38.4 40.2 60.2#
57 19.2 13.8 20.6
100 11.5 6.4 9.6#

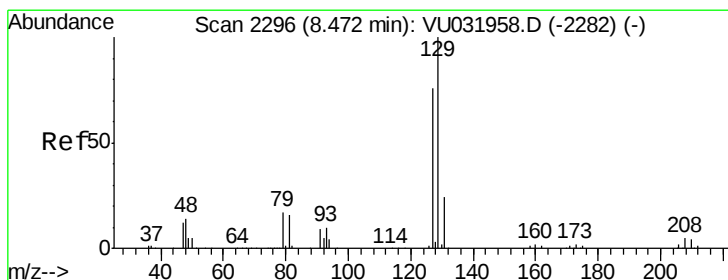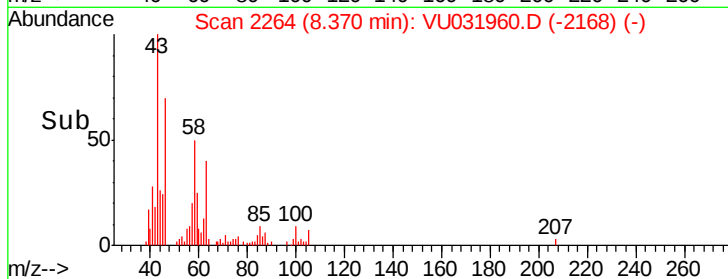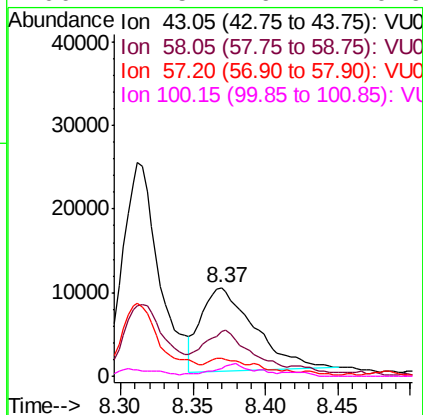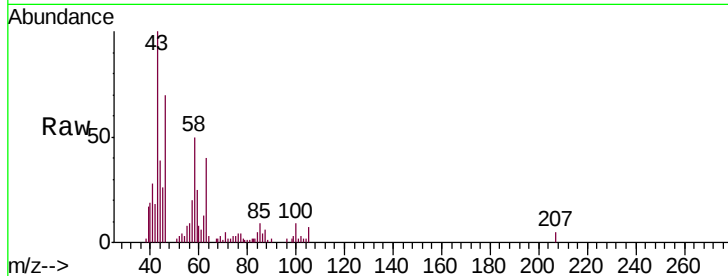

#49
Dibromochloromethane
Concen: 0.220 ug/L
RT: 8.23 min Scan# 2220
Delta R.T. -0.24 min
Lab File: VU031960.D
Acq: 13 May 2019 10:25

Tgt Ion: 129 Resp: 7479
Ion Ratio Lower Upper
129 100
127 0.0 54.7 101.7#

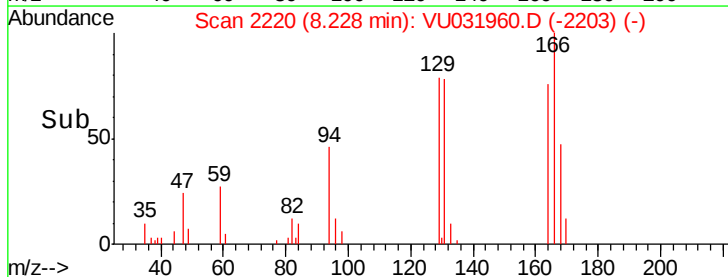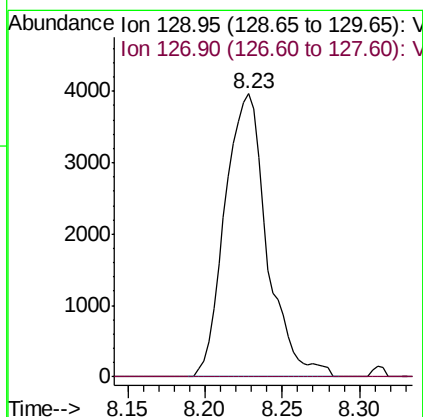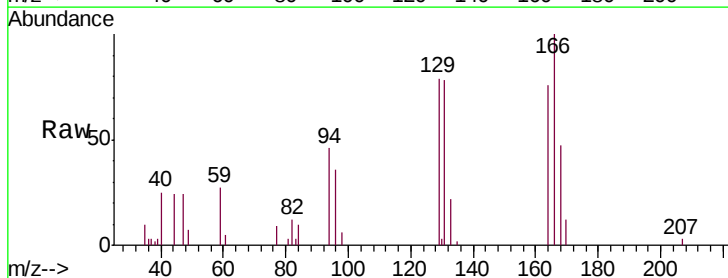

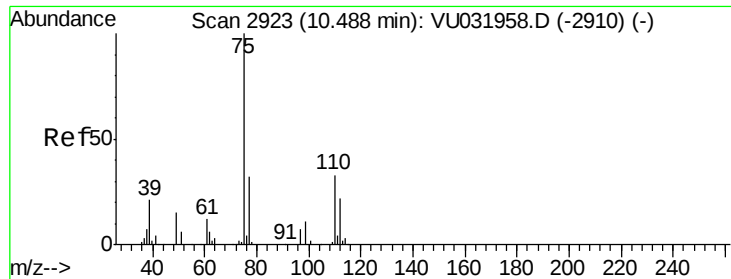

#59

1,2,3-Trichloropropane

Concen: 0.804 ug/L

RT: 11.48 min Scan# 3232

Delta R.T. 0.99 min

Lab File: VU031960.D

Acq: 13 May 2019 10:25

Instrument :

MSVOA_U

ClientSampleId :

F9D11

Tgt Ion: 75 Resp: 23521

Ion Ratio Lower Upper

75 100

77 37.9 26.3 39.5

