

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051319\
 Data File : VU031965.D
 Acq On : 13 May 2019 12:29
 Operator : JC/SP
 Sample : K2739-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB889

Quant Time: May 14 03:47:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 14 02:38:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	490513	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	510206	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	183906	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	104857	3.14	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.80%
7) Chloroethane-d5	1.68	69	109491	3.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.40%
11) 1,1-Dichloroethene-d2	2.27	63	163563	2.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	45.40%#
20) 2-Butanone-d5	4.18	46	470461	36.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.08%
24) Chloroform-d	4.64	84	247546	3.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.20%
26) 1,2-Dichloroethane-d4	5.31	65	142318	3.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.40%#
32) Benzene-d6	5.33	84	468919	3.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.80%
36) 1,2-Dichloropropane-d6	6.33	67	173445	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.40%
41) Toluene-d8	7.56	98	343954	3.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	61.60%#
43) trans-1,3-Dichloropropene-	7.85	79	52982	3.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.00%
46) 2-Hexanone-d5	8.31	63	321187	37.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.46%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	152021	4.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	135045	4.44	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	30493	3.421 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051319\
Data File : VU031965.D
Acq On : 13 May 2019 12:29
Operator : JC/SP
Sample : K2739-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB889

Quant Time: May 14 03:47:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 14 02:38:02 2019
Response via : Initial Calibration

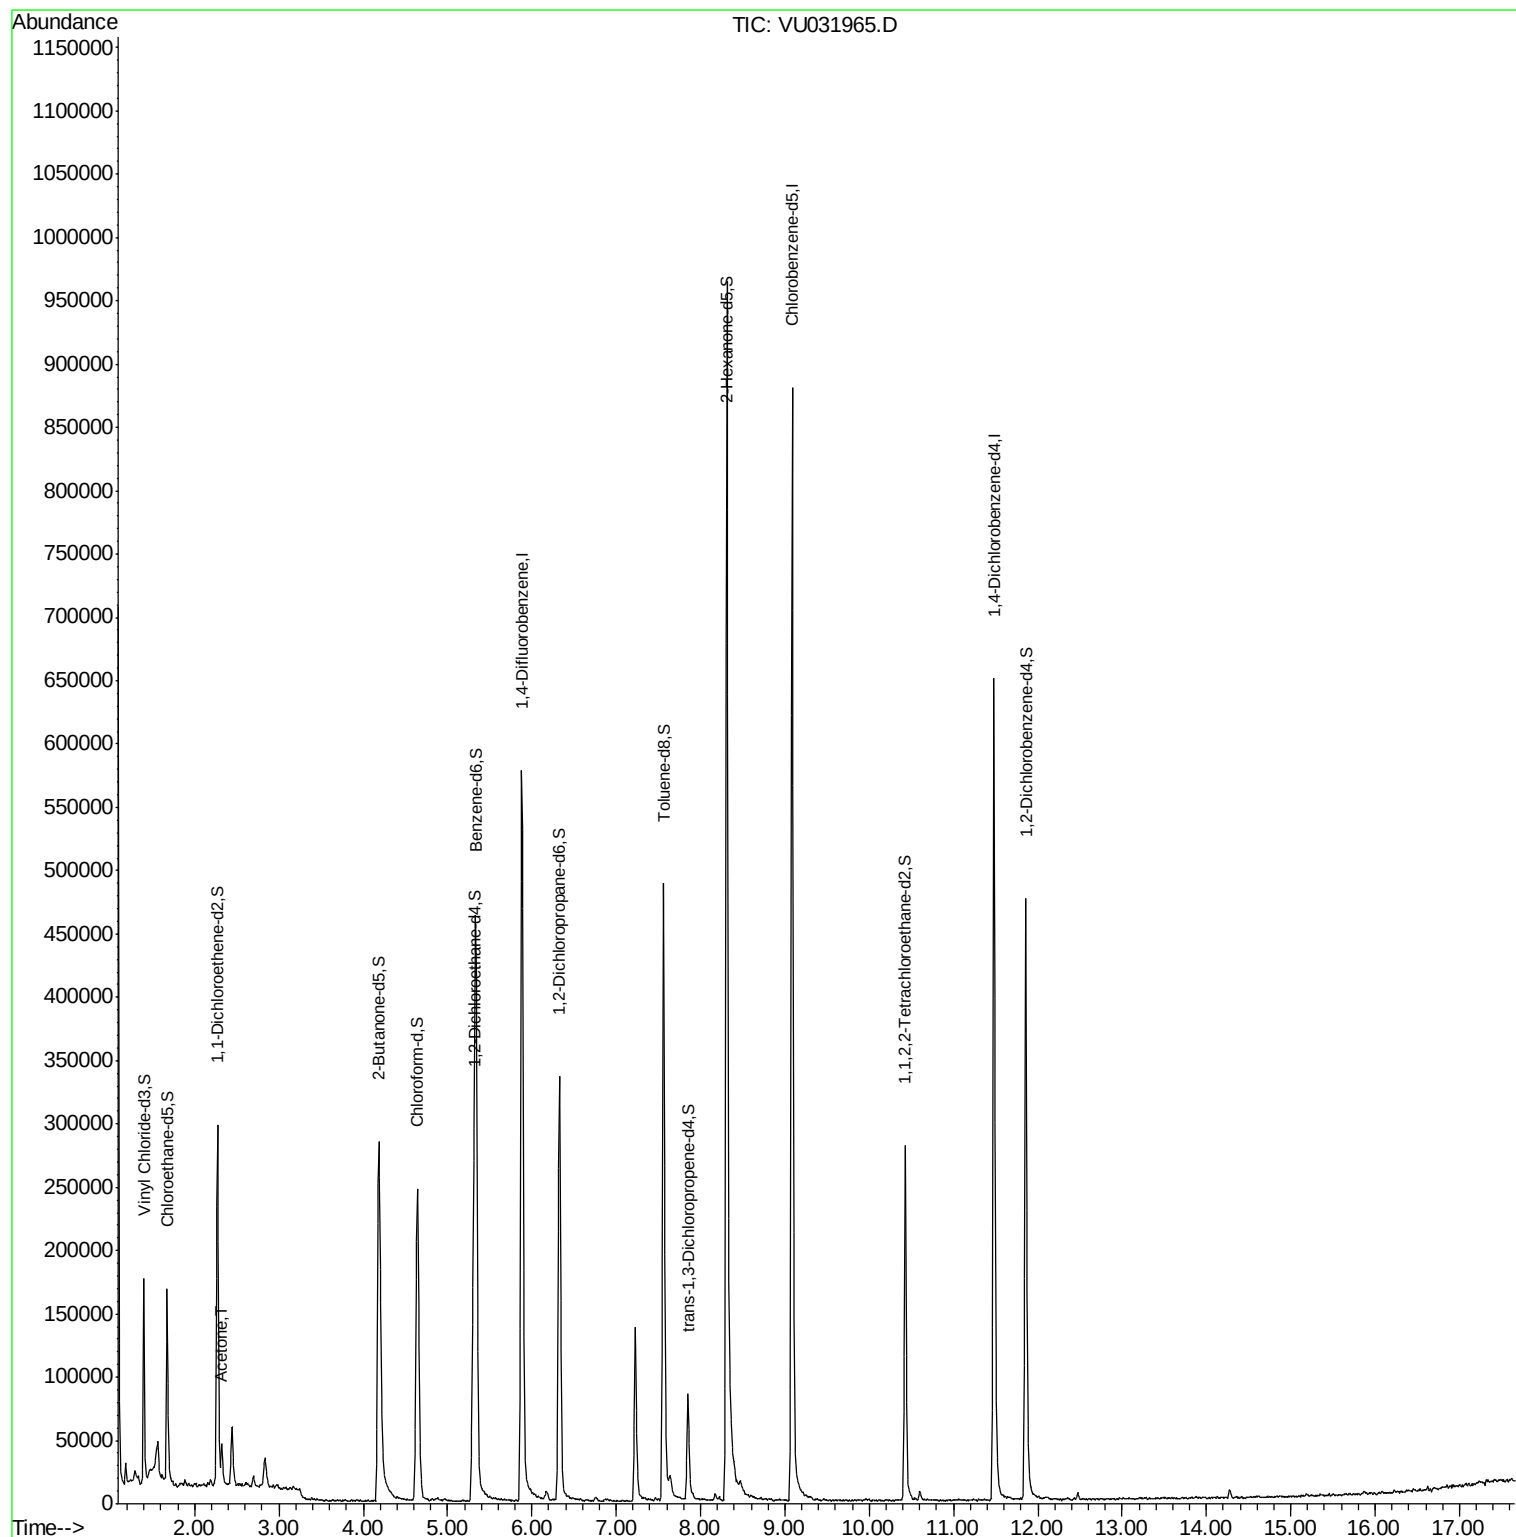

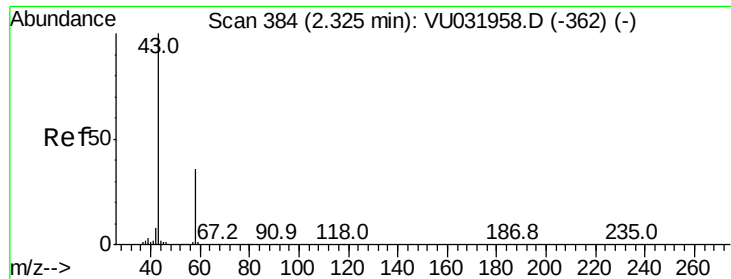

#13

Acetone

Concen: 3.421 ug/L

RT: 2.32 min Scan# 382

Delta R.T. -0.01 min

Lab File: VU031965.D

Acq: 13 May 2019 12:29

Instrument :
MSVOA_U
ClientSampleId :
DB889

Tot Ion: 43 Resp: 30493

Ion Ratio Lower Upper

43 100

58 33.3 0.0 53.6

