


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051320\
 Data File : VU038133.D
 Acq On : 13 May 2020 09:18
 Operator : JC/MD
 Sample : BFB22
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 14 07:24:50 2020

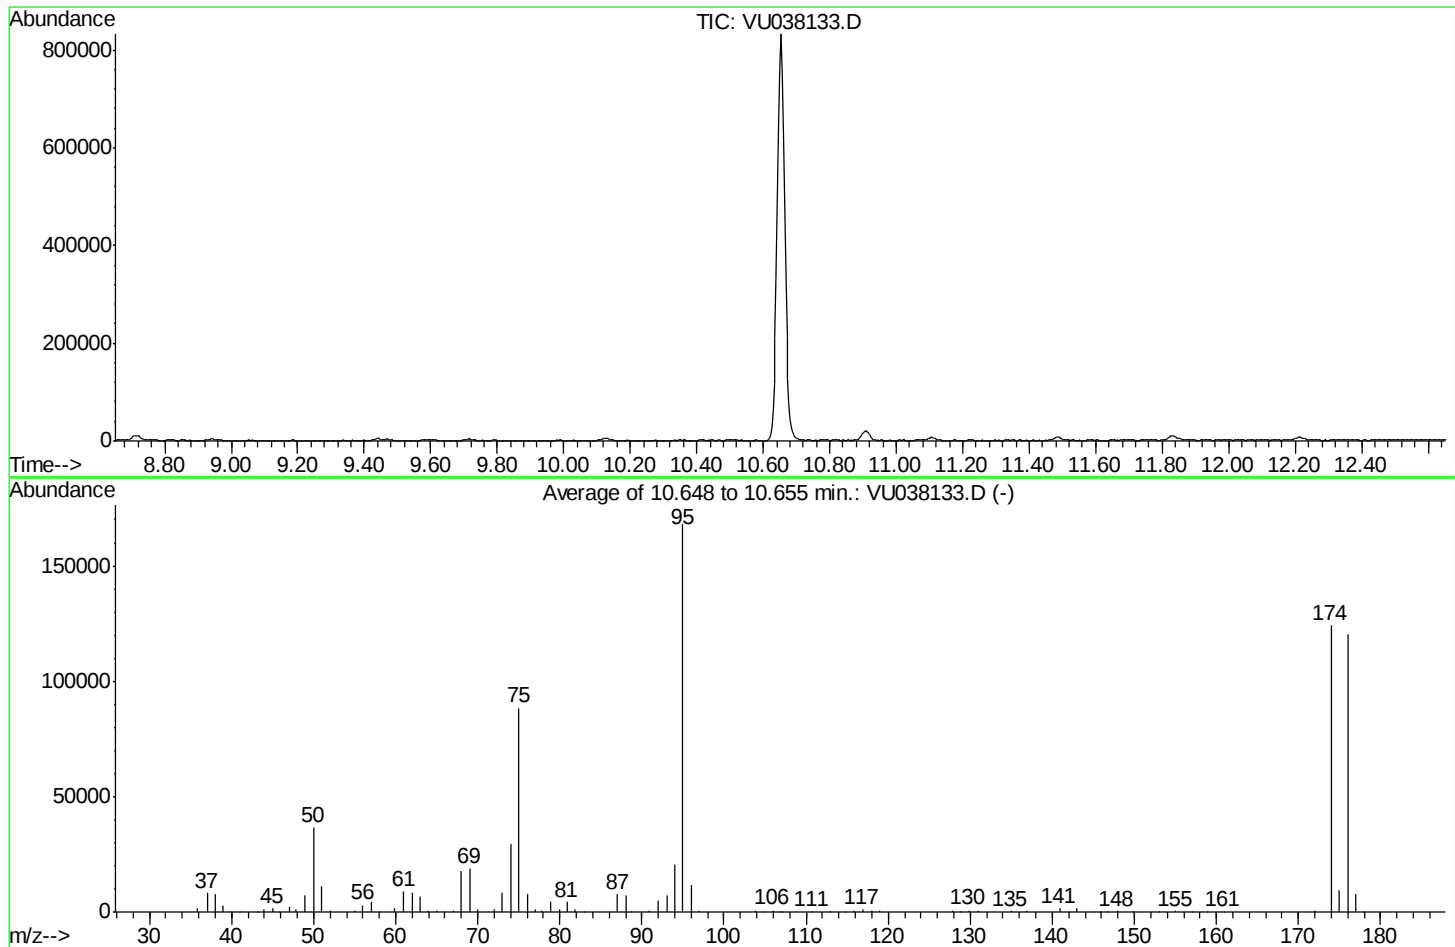

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	36581	PASS
75	95	30	80	52.6	88384	PASS
95	95	100	100	100.0	167957	PASS
96	95	5	9	6.9	11538	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	123984	PASS
175	174	5	9	7.6	9442	PASS
176	174	95	101	97.3	120629	PASS
177	176	5	9	6.7	8039	PASS

m/z	Abundance
35.90	1455.0
37.00	7810.0
38.00	7623.0
39.00	3088.0
40.00	430.0
40.90	117.0
43.10	130.0
43.90	1977.0
45.00	1641.0
45.80	128.0
47.00	2363.0
47.90	904.0
49.00	6726.0
50.00	35208.0
51.00	11034.0
52.00	440.0
55.00	551.0
56.00	2632.0
57.00	4400.0
57.90	208.0
59.90	1412.0
61.00	8371.0
62.00	7992.0
63.00	6323.0
64.10	390.0
65.00	584.0
65.90	103.0
67.00	437.0
68.00	17576.0
69.00	17624.0
70.00	1223.0
72.00	1007.0
73.00	7632.0
74.00	27408.0
75.00	83560.0
76.00	7423.0
77.00	1029.0
77.90	685.0
78.90	4427.0
80.00	1343.0
80.90	4121.0
81.90	1162.0
83.00	137.0
86.00	247.0
87.00	7522.0
88.00	7083.0
88.70	402.0
90.80	580.0
92.00	4472.0
93.00	6745.0
94.00	19464.0
95.00	159552.0
96.00	11003.0
97.10	280.0
103.90	485.0
105.00	246.0
106.00	603.0
106.80	118.0
107.10	127.0
114.70	154.0
115.90	508.0
116.90	966.0
117.90	530.0
118.90	874.0
127.90	349.0
128.80	143.0
129.80	539.0
130.90	311.0
134.90	371.0
136.90	259.0
141.00	1311.0
142.00	111.0
142.90	1317.0
145.00	158.0
145.90	220.0
146.70	149.0
147.90	355.0
155.00	392.0
156.90	225.0
158.90	164.0
160.90	153.0
171.90	554.0
174.00	113976.0
175.00	9186.0
176.00	112336.0
177.00	7550.0
177.90	229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
35.90	1524.0
37.00	8596.0
38.00	8106.0
39.00	3003.0
39.90	366.0
41.00	122.0
43.20	128.0
43.90	1970.0
45.00	1627.0
45.80	129.0
47.00	2387.0
47.90	1021.0
49.00	7184.0
50.00	38016.0
51.00	11688.0
52.00	417.0
55.00	577.0
56.00	2919.0
57.00	4804.0
58.00	182.0
59.90	1574.0
61.00	9042.0
62.00	8706.0
63.00	6844.0
63.90	491.0
65.10	655.0
66.00	133.0
67.00	450.0
68.00	18424.0
69.00	19128.0
70.00	1188.0
72.00	1034.0
73.00	8562.0
74.00	30256.0
75.00	91352.0
76.00	8062.0
77.10	997.0
77.80	580.0
78.90	4863.0
80.00	1381.0
80.90	4528.0
81.90	1340.0
83.00	156.0
86.00	175.0
87.00	7817.0
88.00	7564.0
90.90	586.0
92.00	4980.0
93.00	7277.0
94.00	21144.0
95.00	173440.0
96.00	12006.0
97.00	313.0
103.90	498.0
104.90	275.0
105.90	628.0
107.10	167.0
110.70	110.0
112.80	144.0
114.70	142.0
115.90	523.0
116.90	1051.0
118.00	573.0
118.90	820.0
127.90	394.0
128.90	246.0
129.90	611.0
130.90	337.0
135.00	408.0
136.80	308.0
140.90	1519.0
142.10	146.0
142.90	1449.0
145.00	208.0
145.90	270.0
146.70	169.0
147.90	331.0
152.90	119.0
155.00	516.0
157.00	222.0
159.00	200.0
160.90	187.0
171.90	543.0
174.00	127408.0
175.00	9793.0
176.00	124144.0
177.00	8261.0
177.90	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
35.90	1489.0
37.00	8479.0
38.00	7572.0
39.00	2879.0
39.90	344.0
41.00	101.0
43.20	149.0
44.00	1967.0
45.00	1508.0
47.00	2263.0
47.90	973.0
49.00	7164.0
50.00	36520.0
51.00	11158.0
52.00	325.0
55.00	523.0
56.00	2851.0
57.00	4725.0
58.00	188.0
59.90	1643.0
61.00	8796.0
62.00	8633.0
63.00	6587.0
63.90	603.0
65.10	666.0
66.00	119.0
67.10	474.0
68.00	17720.0
69.00	19224.0
70.00	1135.0
72.00	961.0
73.00	8390.0
74.00	30432.0
75.00	90240.0
76.00	8015.0
77.00	844.0
77.70	465.0
78.90	4827.0
79.90	1412.0
80.90	4598.0
81.90	1304.0
83.00	131.0
87.00	7843.0
88.00	7267.0
90.90	582.0
92.00	4926.0
93.00	7183.0
94.00	21048.0
95.00	170880.0
96.00	11607.0
96.90	373.0
103.90	532.0
104.90	283.0
105.90	695.0
107.00	168.0
110.70	110.0
112.80	191.0
115.90	516.0
116.90	984.0
118.00	567.0
118.90	725.0
127.90	414.0
128.90	332.0
129.90	586.0
130.90	312.0
134.90	387.0
136.80	339.0
140.90	1534.0
142.10	201.0
142.90	1517.0
145.00	172.0
145.80	275.0
146.70	117.0
147.90	283.0
149.90	115.0
152.90	131.0
155.00	494.0
157.00	212.0
159.00	191.0
160.90	167.0
172.00	496.0
174.00	130568.0
175.00	9347.0
176.00	125408.0
177.00	8308.0
177.90	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

Scan 2881 (10.603 min): VU038133.D
BFB22

m/z	Abundance
39.90	367.0
43.90	844.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22