

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
 Data File : VU043700.D
 Acq On : 13 May 2021 13:09
 Operator : SY/MD
 Sample : M2376-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG1Y7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	72	83	92	rBV2	170484	203502	13.87%	3.849%
2	1.919	173	180	192	rVB	33154	42000	2.86%	0.794%
3	2.379	312	323	334	rVB	40120	63973	4.36%	1.210%
4	2.575	372	384	399	rBV2	67831	121530	8.29%	2.299%
5	3.880	770	790	812	rBV	244006	576209	39.28%	10.899%
6	4.678	1012	1038	1069	rBV2	571003	1466772	100.00%	27.744%
7	5.073	1146	1161	1186	rVB	70188	156420	10.66%	2.959%
8	5.735	1345	1367	1387	rBV2	129591	350911	23.92%	6.637%
9	6.256	1513	1529	1548	rBV	127406	237071	16.16%	4.484%
10	6.549	1610	1620	1634	rVB2	17397	31374	2.14%	0.593%
11	6.700	1653	1667	1688	rVB	94236	180198	12.29%	3.408%
12	7.575	1927	1939	1953	rBV	45119	79339	5.41%	1.501%
13	7.906	2027	2042	2059	rBV	136881	237073	16.16%	4.484%
14	8.185	2117	2129	2145	rBV2	30464	51518	3.51%	0.974%
15	8.642	2257	2271	2300	rBV	299316	563442	38.41%	10.658%
16	9.423	2502	2514	2536	rBV	186196	312502	21.31%	5.911%
17	10.764	2919	2931	2949	rVB	76477	121754	8.30%	2.303%
18	11.819	3247	3259	3272	rBV	164159	262147	17.87%	4.959%
19	12.198	3366	3377	3390	rBV	143680	229069	15.62%	4.333%




Sum of corrected areas: 5286804

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
Data File : VU043700.D
Acq On : 13 May 2021 13:09
Operator : SY/MD
Sample : M2376-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

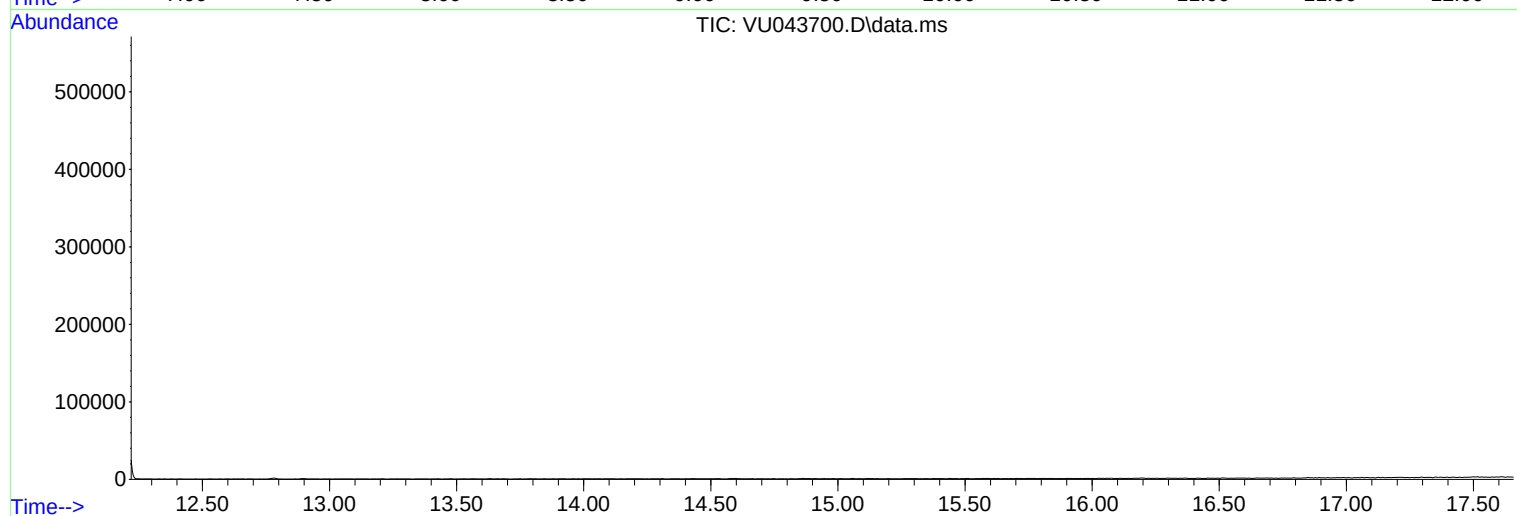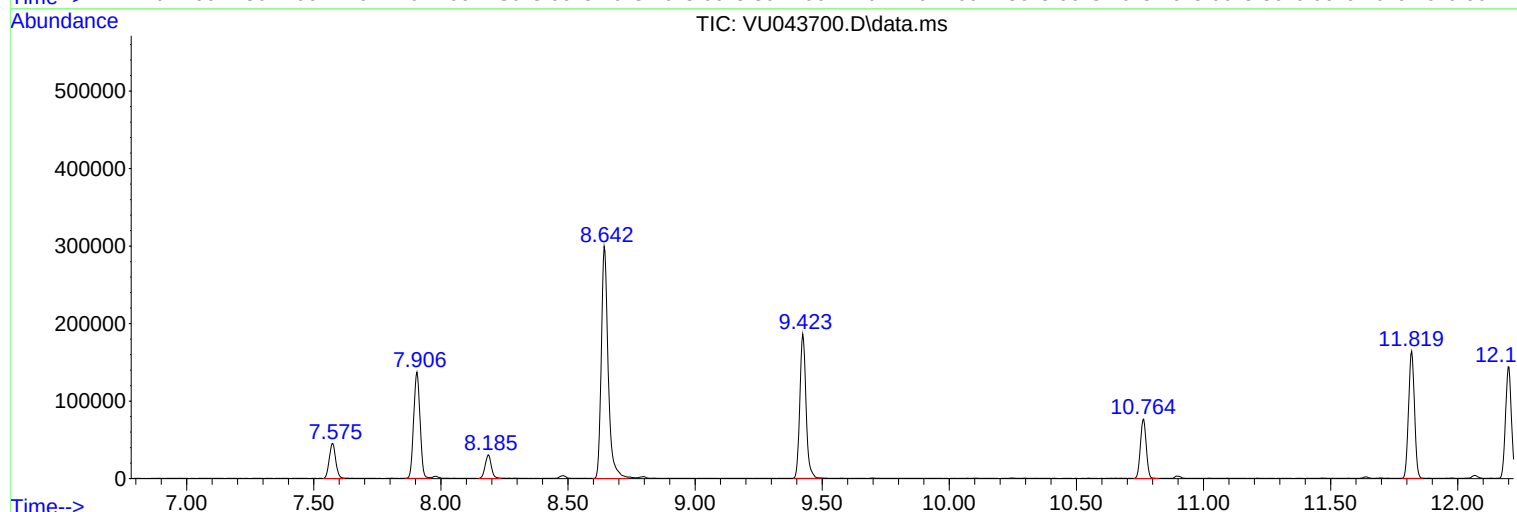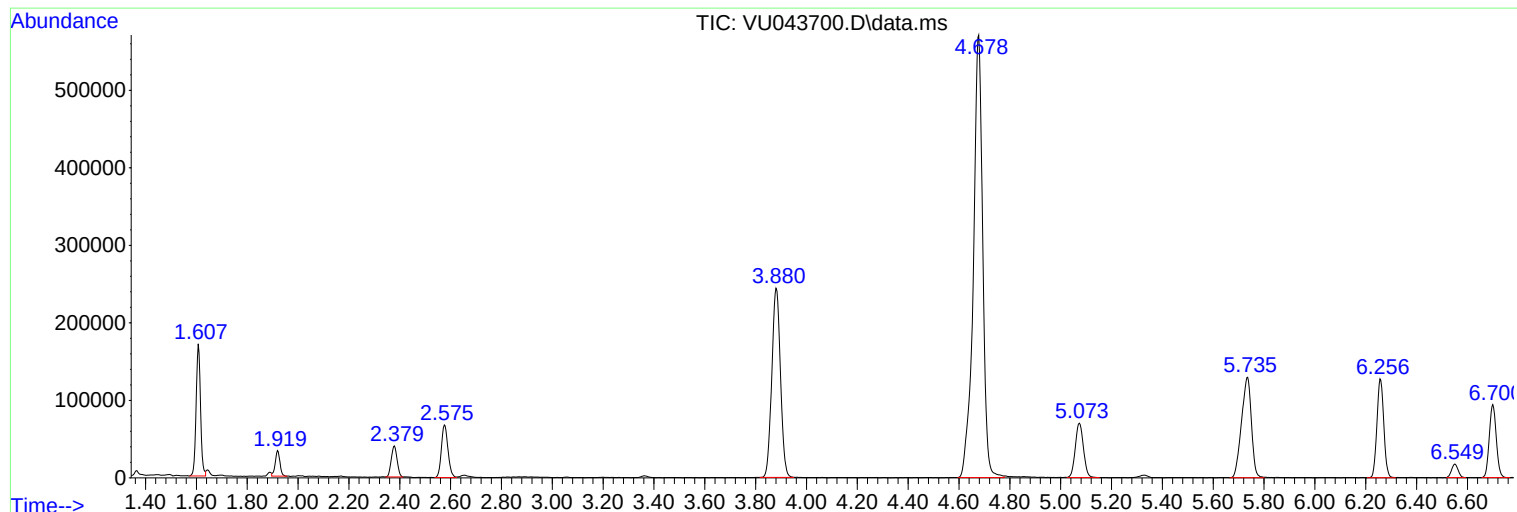

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
Data File : VU043700.D
Acq On : 13 May 2021 13:09
Operator : SY/MD
Sample : M2376-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Y7









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.379	1.35 ug/L	63973	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HC12F3	000354-23-4	95
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	38
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	17
4			Benzyl nitrile	117	C8H7N	000140-29-4	9
5			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	9

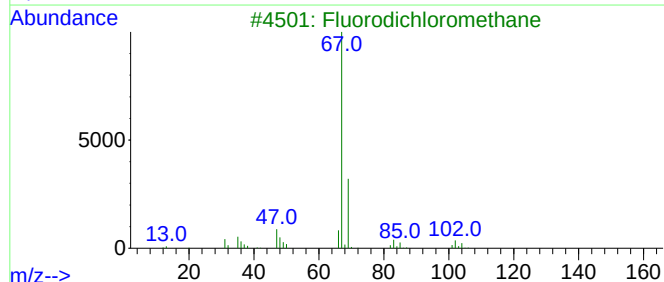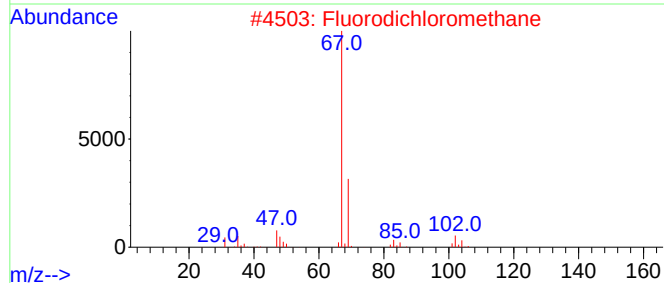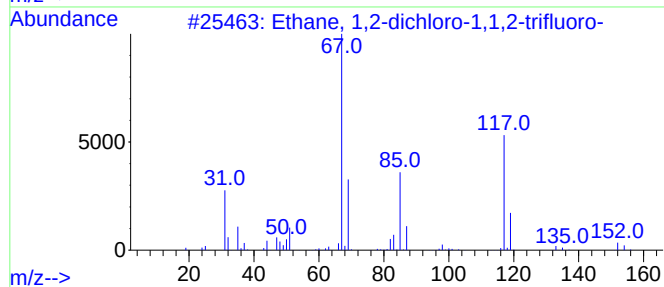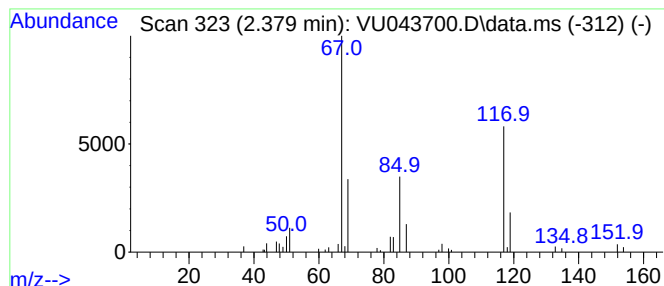

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
Data File : VU043700.D
Acq On : 13 May 2021 13:09
Operator : SY/MD
Sample : M2376-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,2-dic...	2.379	1.4	ug/L	63973	1	6.256	237071	5.0