

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
 Data File : VU043702.D
 Acq On : 13 May 2021 13:57
 Operator : SY/MD
 Sample : M2376-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG127

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	72	83	95	rBV2	67506	86291	15.31%	2.576%
2	1.919	172	180	191	rVB	32545	42163	7.48%	1.259%
3	2.575	372	384	397	rBV	60722	100077	17.75%	2.988%
4	2.652	399	408	421	rVB3	3784	8024	1.42%	0.240%
5	3.366	619	630	642	rVB3	4441	7893	1.40%	0.236%
6	3.880	773	790	814	rVB2	15608	36663	6.50%	1.094%
7	4.642	1011	1027	1063	rBV	86652	282516	50.11%	8.434%
8	5.073	1146	1161	1180	rBV	70591	153026	27.14%	4.568%
9	5.735	1340	1367	1392	rBV3	129755	349802	62.05%	10.442%
10	6.256	1516	1529	1547	rBV	126342	237278	42.09%	7.083%
11	6.546	1610	1619	1631	rBV6	6826	12848	2.28%	0.384%
12	6.700	1653	1667	1684	rVB	93727	180072	31.94%	5.376%
13	7.575	1926	1939	1954	rBV2	45399	78545	13.93%	2.345%
14	7.906	2029	2042	2056	rBV	140132	237186	42.07%	7.081%
15	8.185	2118	2129	2144	rBV	28308	47372	8.40%	1.414%
16	8.642	2257	2271	2305	rBV	301230	563745	100.00%	16.829%
17	9.423	2502	2514	2533	rBV	184389	302325	53.63%	9.025%
18	10.764	2919	2931	2946	rVB	75791	121276	21.51%	3.620%
19	11.819	3247	3259	3274	rBV	167064	267078	47.38%	7.973%
20	12.198	3364	3377	3394	rVB	145693	235663	41.80%	7.035%




Sum of corrected areas: 3349843

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
Data File : VU043702.D
Acq On : 13 May 2021 13:57
Operator : SY/MD
Sample : M2376-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG127

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

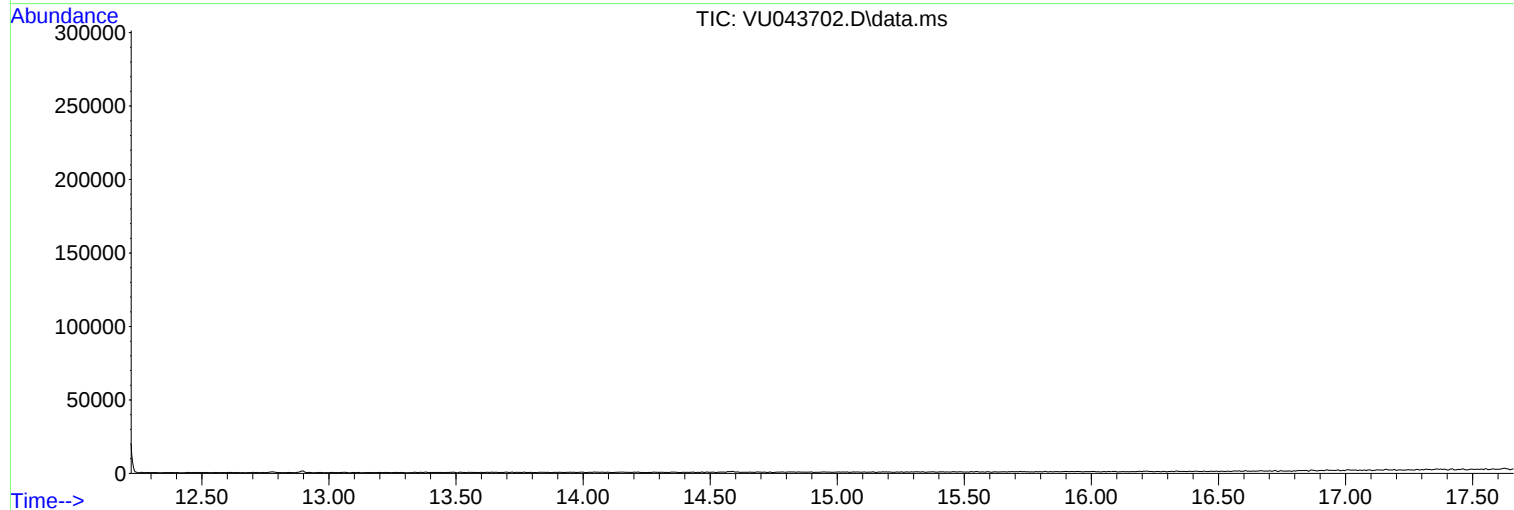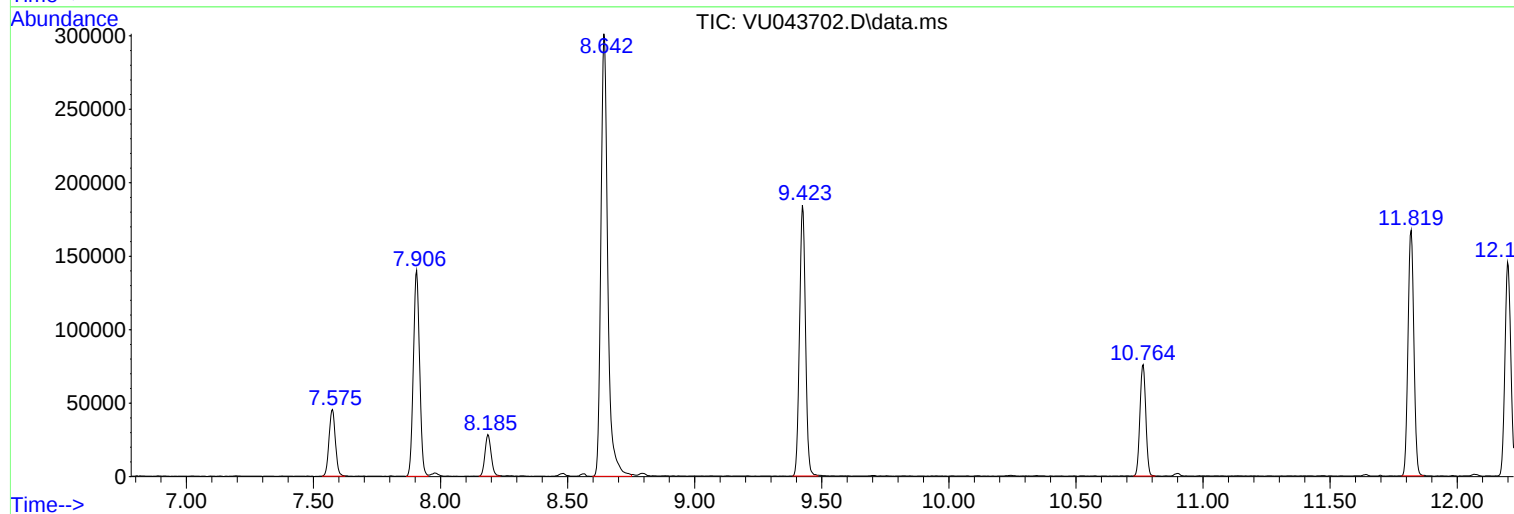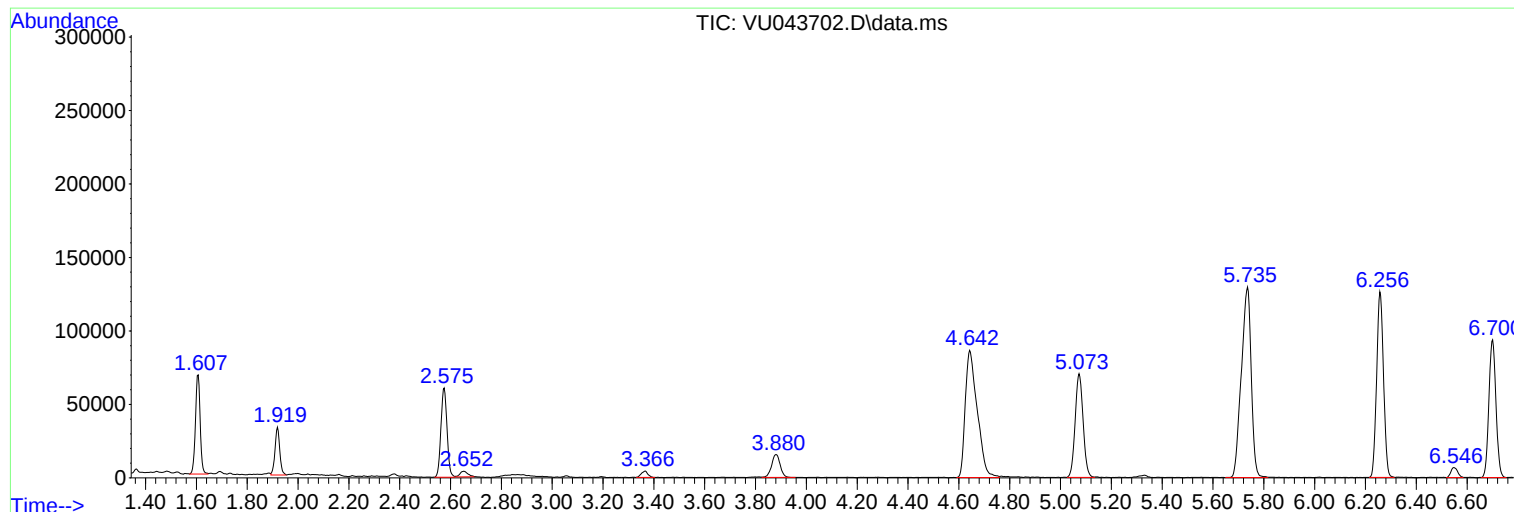

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
Data File : VU043702.D
Acq On : 13 May 2021 13:57
Operator : SY/MD
Sample : M2376-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
Data File : VU043702.D
Acq On : 13 May 2021 13:57
Operator : SY/MD
Sample : M2376-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
