
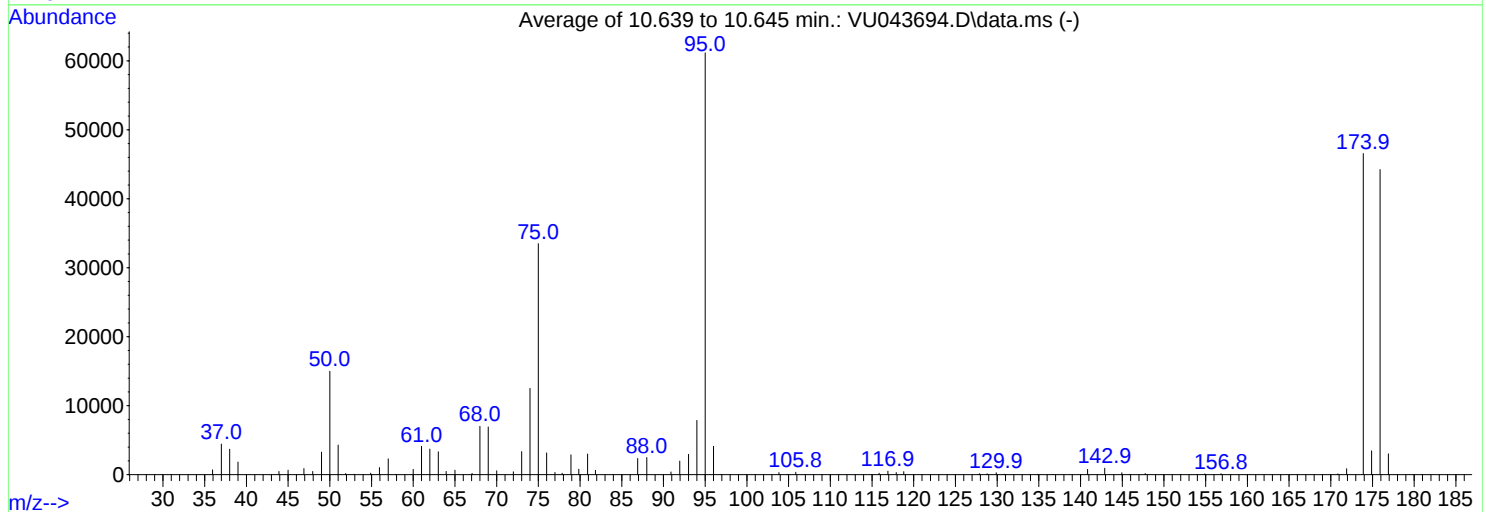


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051321\
 Data File : VU043694.D
 Acq On : 13 May 2021 10:14
 Operator : SY/MD
 Sample : BFB43
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB143

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri May 14 01:48:16 2021

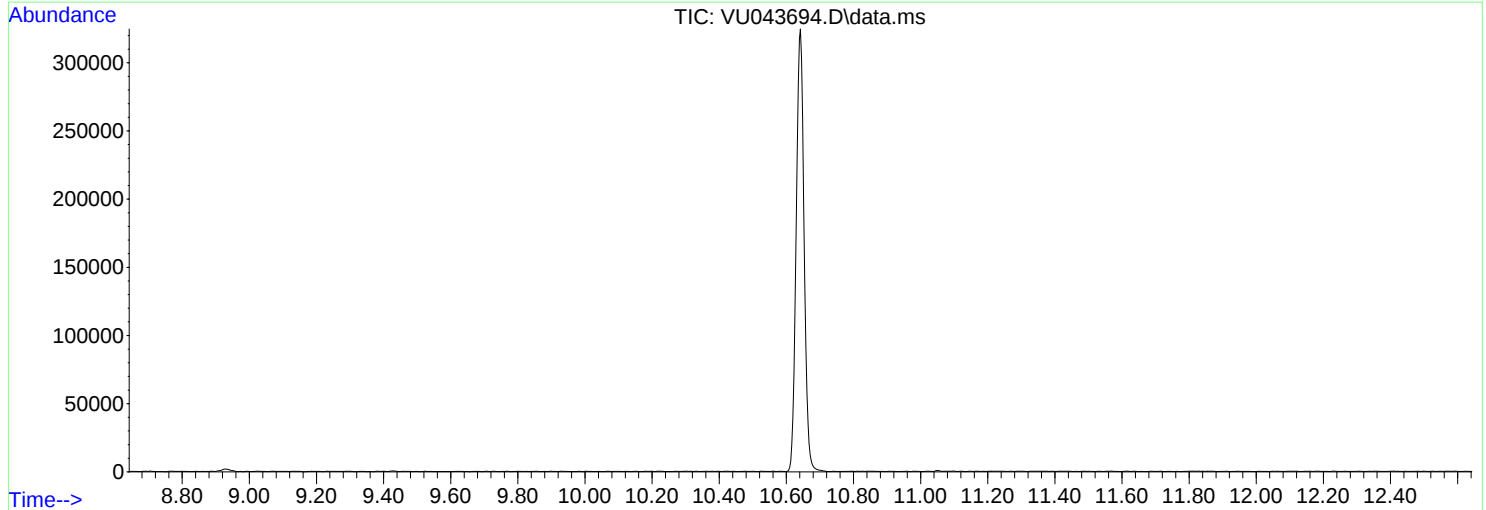

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	14996	PASS
75	95	30	80	54.8	33493	PASS
95	95	100	100	100.0	61157	PASS
96	95	5	9	6.7	4115	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.1	46552	PASS
175	174	5	9	7.4	3461	PASS
176	174	95	101	95.1	44251	PASS
177	176	5	9	6.8	3028	PASS

m/z	Abundance
35.90	679.0
37.00	4192.0
38.00	3379.0
39.00	1629.0
39.90	110.0
44.00	795.0
45.00	569.0
46.90	860.0
47.90	427.0
49.00	3074.0
50.00	13999.0
51.00	3995.0
51.90	153.0
52.90	113.0
55.00	217.0
56.00	970.0
57.00	2130.0
57.90	114.0
60.00	773.0
61.00	3743.0
62.00	3515.0
63.00	3085.0
63.90	476.0
65.00	580.0
67.10	192.0
68.00	6781.0
69.00	6603.0
70.00	494.0
72.00	408.0
73.00	3336.0
74.00	11911.0
75.00	31984.0
76.00	3012.0
77.00	302.0
77.90	210.0
78.90	2856.0
79.90	760.0
80.90	2820.0
81.80	617.0
86.90	2247.0
88.00	2355.0
90.90	380.0
91.90	1928.0
93.00	2839.0
94.00	7574.0
95.00	58480.0
96.00	3992.0
96.90	138.0
103.80	267.0
105.90	338.0
115.90	218.0
116.90	539.0
117.90	267.0
118.80	398.0
127.90	233.0
128.80	135.0
129.90	262.0
130.90	110.0
140.90	773.0
142.90	870.0
144.90	295.0
147.80	164.0
154.90	120.0
156.80	126.0
170.80	105.0
171.90	752.0
173.90	46112.0
174.90	3459.0
175.90	43224.0
176.90	2992.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
39.90	125.0
43.90	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
36.00	699.0
37.00	4506.0
38.00	3869.0
39.00	2021.0
39.90	104.0
43.90	720.0
45.00	740.0
46.90	908.0
48.00	498.0
49.00	3389.0
50.00	15589.0
51.00	4490.0
51.90	173.0
54.80	188.0
55.90	1031.0
57.00	2414.0
60.00	713.0
61.00	4315.0
62.00	3792.0
63.00	3442.0
64.00	424.0
65.00	719.0
67.00	182.0
68.00	7059.0
69.00	7054.0
70.00	611.0
72.00	423.0
73.00	3248.0
74.00	12716.0
75.00	34000.0
76.00	3257.0
77.00	360.0
77.80	228.0
78.90	2788.0
79.80	826.0
80.90	3075.0
81.90	658.0
86.90	2345.0
88.00	2484.0
90.90	392.0
92.00	1993.0
93.00	2980.0
94.00	7888.0
95.00	61920.0
96.00	4098.0
103.90	337.0
104.80	112.0
105.80	342.0
115.80	223.0
116.90	483.0
117.90	313.0
118.80	467.0
127.70	167.0
128.80	135.0
129.90	271.0
134.80	108.0
136.70	103.0
140.80	709.0
142.90	954.0
145.00	249.0
147.70	146.0
154.90	133.0
156.90	129.0
170.90	141.0
171.90	958.0
173.90	45600.0
174.90	3377.0
175.90	43880.0
176.90	2936.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
35.90	682.0
37.00	4577.0
38.00	3808.0
39.00	1883.0
40.00	106.0
44.00	758.0
45.00	657.0
46.00	101.0
46.90	885.0
48.00	482.0
49.00	3366.0
50.00	15401.0
51.00	4368.0
51.90	181.0
52.90	105.0
54.90	200.0
56.00	1030.0
57.00	2384.0
60.00	787.0
61.00	4231.0
62.00	3814.0
63.00	3431.0
64.00	474.0
65.00	667.0
67.10	201.0
68.00	7200.0
69.00	7077.0
70.00	566.0
72.00	450.0
73.00	3422.0
74.00	12871.0
75.00	34496.0
76.00	3225.0
77.00	335.0
77.80	221.0
78.90	2965.0
79.90	818.0
80.90	3074.0
81.90	642.0
86.90	2426.0
88.00	2639.0
90.90	419.0
91.90	2017.0
93.00	3034.0
94.00	8105.0
95.00	63072.0
96.00	4256.0
103.80	308.0
105.80	369.0
115.80	211.0
116.90	541.0
117.90	332.0
118.80	449.0
127.90	204.0
128.80	154.0
129.90	284.0
130.80	100.0
140.90	788.0
142.90	930.0
144.90	293.0
145.90	109.0
147.80	165.0
154.90	127.0
156.90	138.0
170.80	133.0
171.90	876.0
173.90	47944.0
174.90	3546.0
175.90	45648.0
176.90	3156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143