

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
 Data File : VU048555.D
 Acq On : 13 May 2022 11:04
 Operator : SY/MD
 Sample : VU0513MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK125

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	96	rVB	101874	117304	10.96%	1.395%
2	1.912	170	178	195	rVB	83269	108849	10.17%	1.294%
3	2.511	359	364	368	rBV2	346	354	0.03%	0.004%
4	2.568	370	382	403	rVV	206795	336447	31.42%	4.000%
5	2.678	412	416	418	rBV	235	224	0.02%	0.003%
6	2.916	487	490	491	rBV	368	161	0.02%	0.002%
7	2.986	510	512	515	rVB	304	146	0.01%	0.002%
8	3.044	522	530	531	rBV2	2083	1794	0.17%	0.021%
9	3.115	548	552	557	rVB2	372	420	0.04%	0.005%
10	3.141	557	560	561	rBV2	289	158	0.01%	0.002%
11	3.154	561	564	566	rBV	195	152	0.01%	0.002%
12	3.356	622	627	630	rBV2	580	599	0.06%	0.007%
13	3.443	651	654	656	rBV	264	185	0.02%	0.002%
14	3.456	656	658	662	rVB2	381	273	0.03%	0.003%
15	3.485	662	667	670	rBV	204	242	0.02%	0.003%
16	3.510	672	675	678	rBV	198	175	0.02%	0.002%
17	3.761	751	753	755	rBV	314	191	0.02%	0.002%
18	3.800	761	765	770	rBV2	251	311	0.03%	0.004%
19	3.858	781	783	786	rVB	366	198	0.02%	0.002%
20	3.874	786	788	790	rBV	295	174	0.02%	0.002%
21	3.893	790	794	798	rVB2	326	311	0.03%	0.004%
22	4.035	833	838	839	rBV	219	163	0.02%	0.002%
23	4.144	868	872	875	rVV2	328	277	0.03%	0.003%
24	4.173	879	881	885	rVV	219	173	0.02%	0.002%
25	4.237	898	901	904	rBV	297	202	0.02%	0.002%
26	4.327	927	929	932	rBV	296	249	0.02%	0.003%
27	4.350	932	936	941	rVV2	313	389	0.04%	0.005%
28	4.379	942	945	951	rVV	307	293	0.03%	0.003%
29	4.408	951	954	956	rVB	344	230	0.02%	0.003%
30	4.424	956	959	962	rBV	189	181	0.02%	0.002%
31	4.475	971	975	976	rBV	228	146	0.01%	0.002%
32	4.620	1008	1020	1054	rBV	118186	292263	27.30%	3.475%
33	5.063	1142	1158	1180	rBV	208684	453874	42.39%	5.396%
34	5.215	1200	1205	1206	rBV2	376	263	0.02%	0.003%
35	5.266	1219	1221	1223	rBV	278	152	0.01%	0.002%
36	5.279	1223	1225	1228	rBV2	357	259	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
 Data File : VU048555.D
 Acq On : 13 May 2022 11:04
 Operator : SY/MD
 Sample : VU0513MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK125

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

37	5.446	1273	1277	1282	rBV2	221	181	0.02%	0.002%
38	5.501	1289	1294	1295	rBV	219	197	0.02%	0.002%
39	5.520	1297	1300	1301	rBV	482	279	0.03%	0.003%
40	5.578	1315	1318	1319	rBV	242	146	0.01%	0.002%
41	5.726	1340	1364	1384	rBV2	388548	1070640	100.00%	12.728%
42	5.928	1421	1427	1431	rVB3	383	505	0.05%	0.006%
43	6.006	1448	1451	1454	rBV2	278	219	0.02%	0.003%
44	6.073	1467	1472	1475	rBV2	346	250	0.02%	0.003%
45	6.092	1475	1478	1479	rBV	370	170	0.02%	0.002%
46	6.150	1492	1496	1500	rVB2	233	206	0.02%	0.002%
47	6.250	1512	1527	1546	rBV	307498	576860	53.88%	6.858%
48	6.433	1582	1584	1589	rBV2	253	206	0.02%	0.002%
49	6.530	1600	1614	1626	rBV9	4019	8741	0.82%	0.104%
50	6.690	1650	1664	1684	rBV	246053	477672	44.62%	5.679%
51	6.912	1730	1733	1737	rVB	239	164	0.02%	0.002%
52	6.938	1738	1741	1744	rVB2	330	236	0.02%	0.003%
53	6.960	1746	1748	1750	rBV	239	150	0.01%	0.002%
54	7.083	1783	1786	1788	rBV	352	262	0.02%	0.003%
55	7.169	1809	1813	1816	rBV2	633	637	0.06%	0.008%
56	7.272	1842	1845	1849	rBV2	268	215	0.02%	0.003%
57	7.353	1866	1870	1875	rVB2	221	198	0.02%	0.002%
58	7.378	1876	1878	1881	rVB2	279	150	0.01%	0.002%
59	7.398	1881	1884	1886	rBV2	261	176	0.02%	0.002%
60	7.430	1891	1894	1896	rBV2	296	237	0.02%	0.003%
61	7.469	1903	1906	1908	rBV	264	195	0.02%	0.002%
62	7.568	1924	1937	1955	rBV	141986	249677	23.32%	2.968%
63	7.681	1970	1972	1978	rVB5	701	442	0.04%	0.005%
64	7.787	2000	2005	2006	rBV2	955	751	0.07%	0.009%
65	7.829	2016	2018	2020	rBV	327	203	0.02%	0.002%
66	7.899	2026	2040	2056	rBV	480398	828920	77.42%	9.855%
67	8.179	2115	2127	2147	rBV2	105786	180752	16.88%	2.149%
68	8.501	2224	2227	2231	rBV	369	262	0.02%	0.003%
69	8.552	2238	2243	2248	rVV4	749	878	0.08%	0.010%
70	8.632	2257	2268	2308	rBV	366019	667153	62.31%	7.932%
71	8.867	2339	2341	2343	rVV	338	162	0.02%	0.002%
72	8.880	2343	2345	2350	rVB2	488	273	0.03%	0.003%
73	8.922	2355	2358	2363	rVB3	680	620	0.06%	0.007%
74	9.015	2384	2387	2390	rBV	254	196	0.02%	0.002%
75	9.417	2499	2512	2538	rBV	453419	754085	70.43%	8.965%
76	9.571	2553	2560	2567	rBV3	1407	1891	0.18%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
 Data File : VU048555.D
 Acq On : 13 May 2022 11:04
 Operator : SY/MD
 Sample : VU0513MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK125

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis

77	9.693	2592	2598	2607	rVB3	1841	2459	0.23%	0.029%
78	10.115	2720	2729	2738	rBV7	2010	3237	0.30%	0.038%
79	10.185	2748	2751	2755	rVB	285	195	0.02%	0.002%
80	10.359	2802	2805	2806	rBV	243	168	0.02%	0.002%
81	10.484	2837	2844	2847	rBV2	926	994	0.09%	0.012%
82	10.639	2884	2892	2896	rBV4	1800	2398	0.22%	0.029%
83	10.671	2899	2902	2909	rVB2	1505	1370	0.13%	0.016%
84	10.755	2916	2928	2947	rBV	379519	616987	57.63%	7.335%
85	11.025	3009	3012	3015	rBV2	301	215	0.02%	0.003%
86	11.581	3183	3185	3192	rVB2	433	386	0.04%	0.005%
87	11.748	3232	3237	3245	rVB4	2388	2895	0.27%	0.034%
88	11.812	3245	3257	3273	rBV	478808	765647	71.51%	9.102%
89	11.915	3287	3289	3292	rBV	470	286	0.03%	0.003%
90	12.192	3363	3375	3394	rBV	523816	851376	79.52%	10.122%
91	12.346	3421	3423	3428	rVB2	375	263	0.02%	0.003%
92	12.632	3510	3512	3514	rBV2	333	175	0.02%	0.002%
93	12.761	3550	3552	3556	rBV2	253	191	0.02%	0.002%
94	13.053	3639	3643	3648	rBV3	363	423	0.04%	0.005%
95	13.404	3748	3752	3754	rBV3	476	338	0.03%	0.004%
96	13.848	3883	3890	3895	rBV7	2981	4072	0.38%	0.048%
97	13.970	3925	3928	3931	rBV2	458	342	0.03%	0.004%
98	14.092	3961	3966	3975	rVB	6435	8588	0.80%	0.102%
99	14.195	3996	3998	4001	rBV2	612	382	0.04%	0.005%
100	14.333	4035	4041	4051	rVB5	3307	5081	0.47%	0.060%




Sum of corrected areas: 8411407

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
Data File : VU048555.D
Acq On : 13 May 2022 11:04
Operator : SY/MD
Sample : VU0513MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

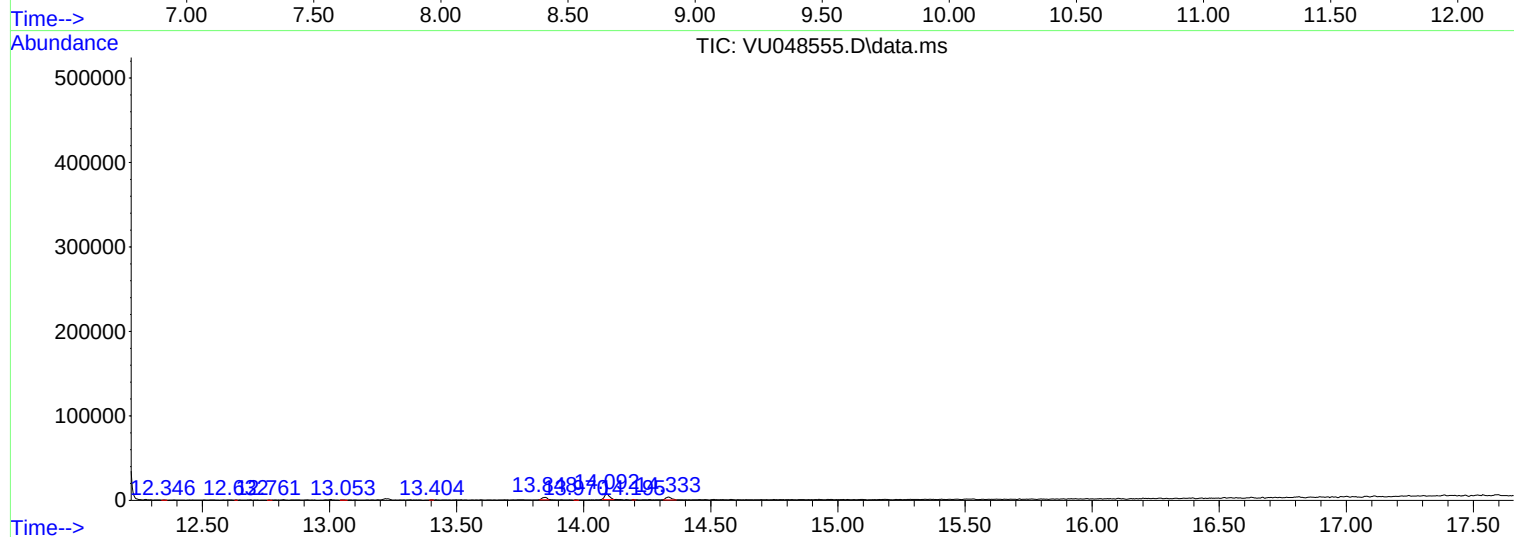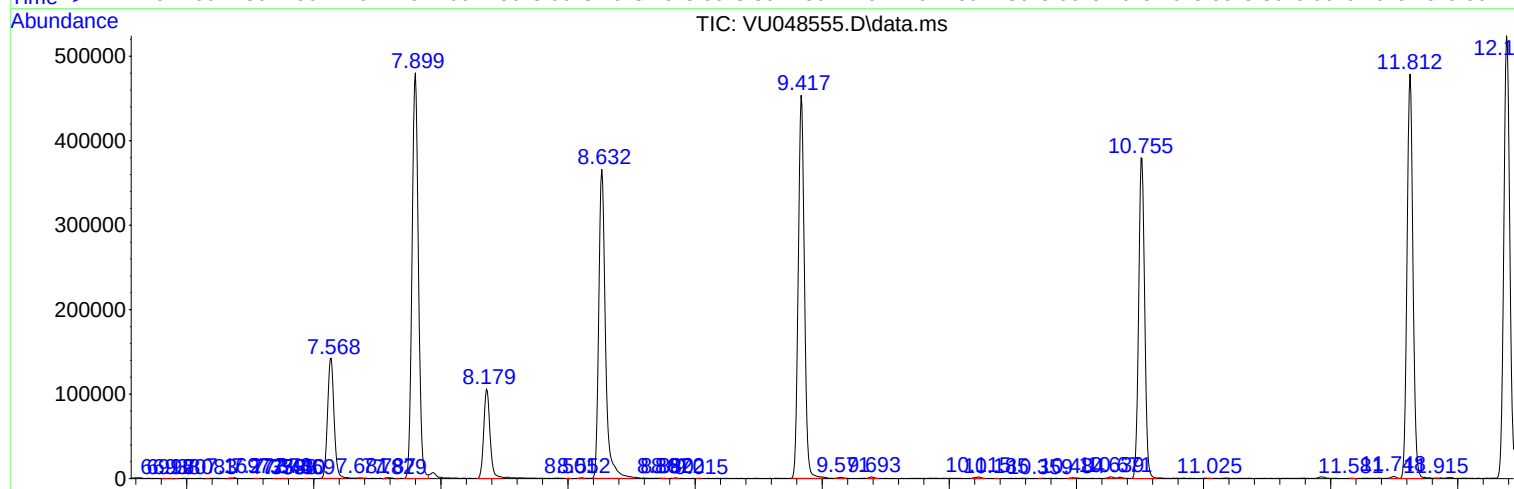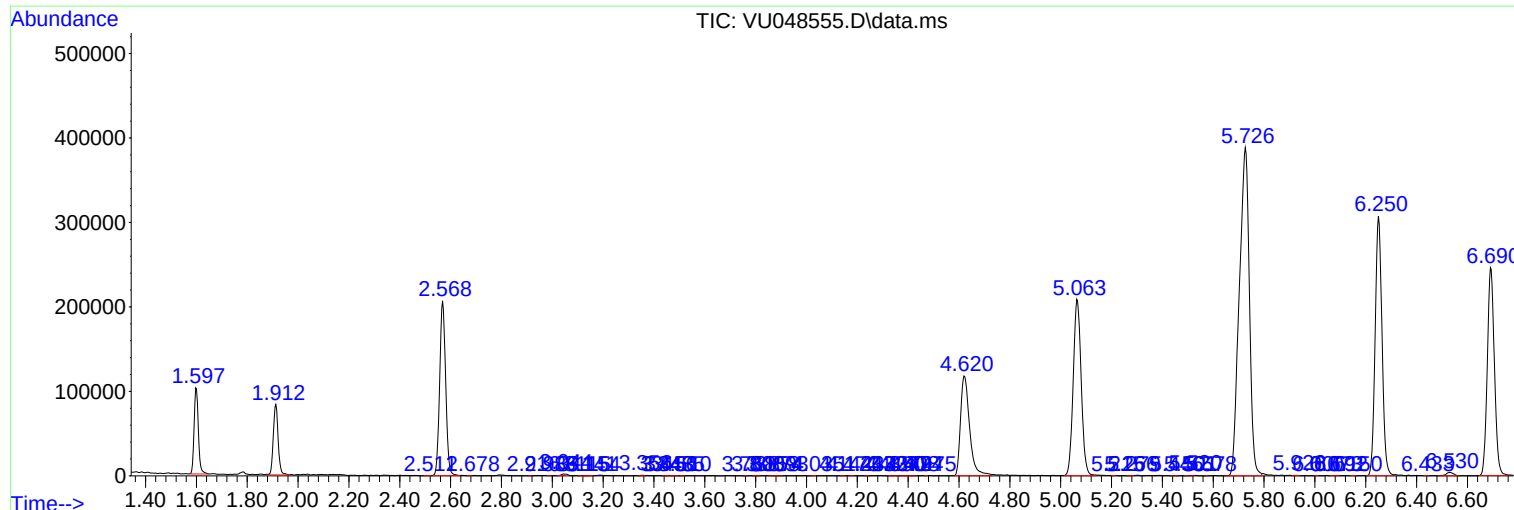

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
Data File : VU048555.D
Acq On : 13 May 2022 11:04
Operator : SY/MD
Sample : VU0513MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
Data File : VU048555.D
Acq On : 13 May 2022 11:04
Operator : SY/MD
Sample : VU0513MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc