


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051322\
 Data File : VU048553.D
 Acq On : 13 May 2022 09:30
 Operator : SY/MD
 Sample : BFB086
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB086

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM050622WMA.M
 Title : VOC Analysis
 Last Update : Mon May 16 14:13:08 2022

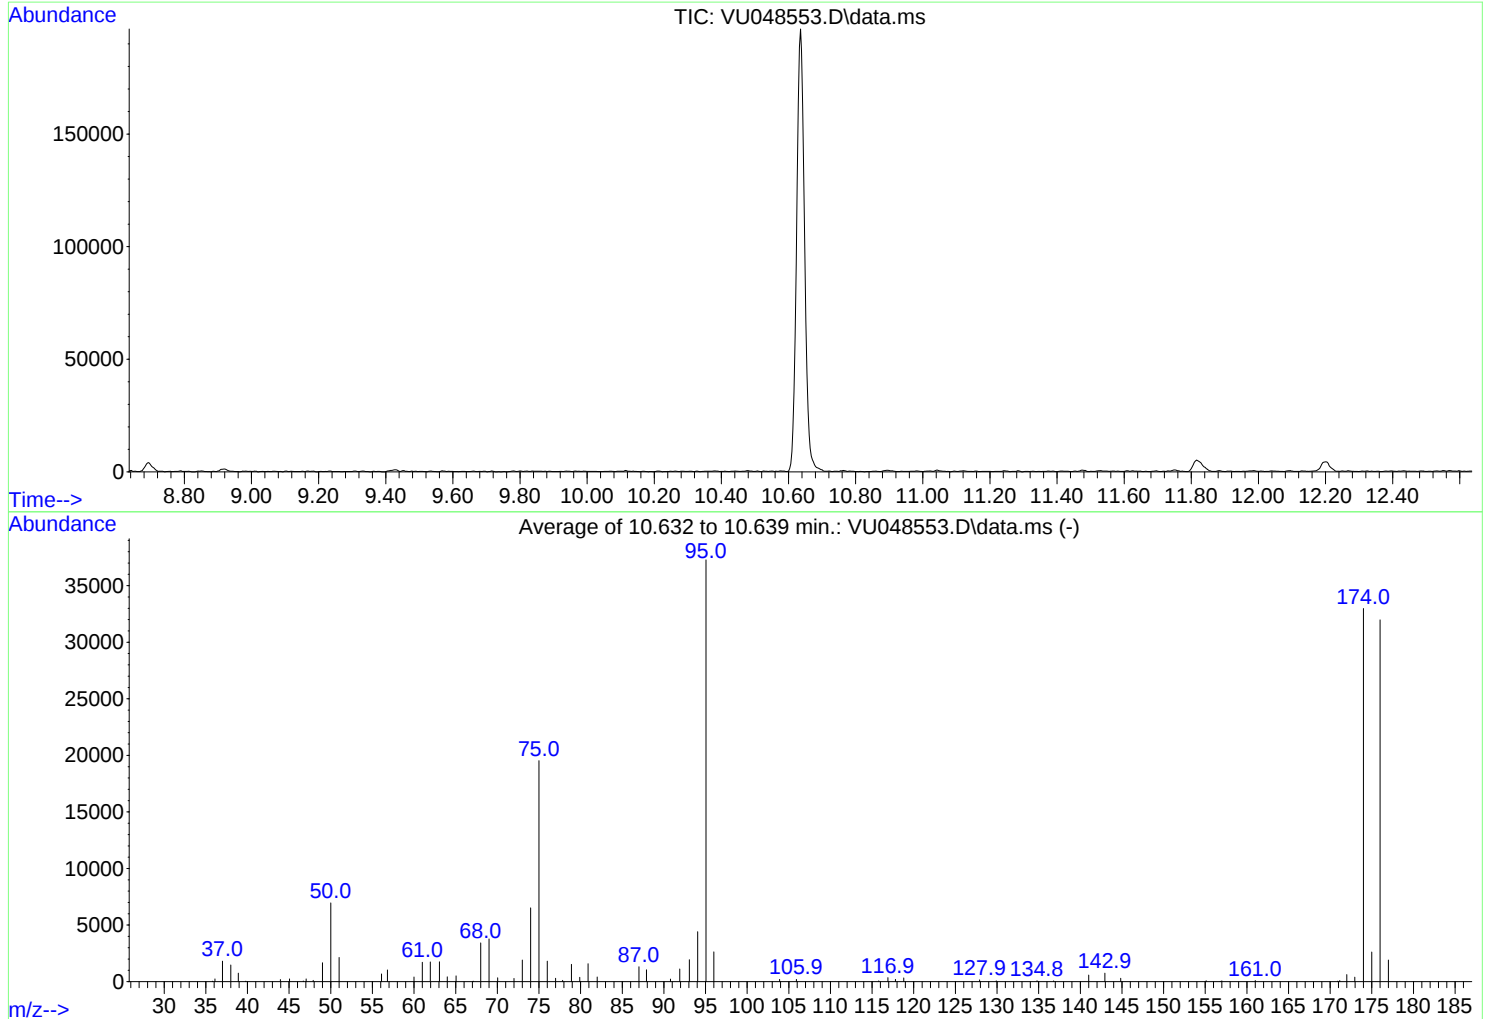

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	6955	PASS
75	95	30	80	52.4	19539	PASS
95	95	100	100	100.0	37283	PASS
96	95	5	9	7.0	2628	PASS
173	174	0.00	2	1.2	402	PASS
174	95	50	120	88.5	32984	PASS
175	174	5	9	7.9	2613	PASS
176	174	95	101	97.0	31979	PASS
177	176	5	9	6.0	1914	PASS

m/z	Abundance
43.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
36.00	289.0
37.00	1694.0
38.00	1536.0
38.90	673.0
44.00	401.0
45.00	240.0
47.00	335.0
47.90	117.0
49.00	1561.0
50.00	6784.0
51.00	2046.0
56.10	760.0
56.80	1002.0
60.00	337.0
61.00	1527.0
61.90	1796.0
63.00	1849.0
64.00	411.0
65.10	453.0
67.10	136.0
68.00	3547.0
69.00	3644.0
70.00	362.0
72.00	299.0
73.00	2077.0
74.00	6479.0
75.00	19832.0
76.00	1829.0
77.00	286.0
77.80	111.0
78.90	1489.0
80.00	433.0
80.90	1432.0
82.10	384.0
87.00	1253.0
87.90	990.0
90.80	240.0
91.90	1190.0
93.10	1877.0
94.00	4567.0
95.00	37592.0
96.00	2560.0
103.90	180.0
105.90	197.0
116.90	364.0
117.80	192.0
118.80	338.0
128.00	118.0
129.90	116.0
134.80	137.0
136.80	116.0
141.00	538.0
142.90	754.0
144.80	331.0
155.10	156.0
156.80	104.0
171.20	170.0
172.00	574.0
172.90	447.0
174.00	32208.0
175.00	2626.0
176.00	30472.0
177.00	2100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
36.10	241.0
37.00	1895.0
38.00	1508.0
38.90	783.0
44.00	425.0
45.10	264.0
47.10	230.0
47.90	118.0
49.00	1801.0
50.00	7162.0
51.00	2206.0
56.10	750.0
56.80	1108.0
60.00	440.0
61.00	1798.0
61.90	1768.0
63.10	1752.0
64.00	423.0
65.00	526.0
68.00	3479.0
69.00	3814.0
70.00	319.0
72.00	290.0
73.00	1992.0
74.00	6747.0
75.00	19976.0
76.00	1896.0
77.00	323.0
77.90	118.0
78.90	1536.0
79.90	377.0
80.90	1637.0
82.00	417.0
87.00	1360.0
87.90	1096.0
90.80	238.0
91.90	1156.0
93.10	2004.0
94.00	4564.0
95.00	38264.0
96.00	2712.0
103.90	200.0
105.90	222.0
115.80	100.0
116.90	372.0
117.80	203.0
118.80	323.0
127.80	121.0
128.10	104.0
129.90	116.0
134.80	115.0
136.80	103.0
141.00	593.0
142.90	779.0
144.80	321.0
155.10	103.0
157.00	100.0
161.00	124.0
171.10	138.0
172.00	663.0
172.90	401.0
174.00	34016.0
175.00	2717.0
176.00	33184.0
177.00	1960.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086

m/z	Abundance
35.80	147.0
36.20	199.0
37.00	1855.0
38.00	1388.0
38.90	798.0
39.80	108.0
44.00	434.0
45.00	198.0
46.70	177.0
47.10	156.0
47.90	105.0
49.00	1660.0
50.00	6918.0
51.00	2175.0
56.10	513.0
56.80	998.0
60.00	454.0
61.00	1795.0
62.00	1677.0
63.10	1642.0
64.00	420.0
65.00	542.0
68.00	3222.0
69.00	3869.0
70.10	331.0
72.00	274.0
73.00	1658.0
74.00	6350.0
75.00	18808.0
76.00	1721.0
77.00	283.0
77.90	130.0
78.90	1540.0
79.80	342.0
80.90	1703.0
81.90	420.0
87.00	1357.0
87.90	1040.0
90.80	209.0
91.90	1001.0
93.00	1936.0
94.10	4106.0
95.10	35992.0
96.00	2612.0
103.90	195.0
105.90	185.0
115.80	116.0
116.90	343.0
117.80	198.0
118.80	313.0
127.80	121.0
141.00	606.0
143.00	736.0
144.90	239.0
157.00	100.0
161.00	162.0
170.90	112.0
172.00	630.0
173.00	359.0
174.00	32728.0
175.00	2495.0
176.00	32280.0
177.00	1682.0

Instrument :
MSVOA_U
ClientSampleId :
BFB086