

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU051418\
 Data File : VU023848.D
 Acq On : 14 May 2018 11:28
 Operator : MD/SY
 Sample : VU0514WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 15 04:20:00 2018
 Quant Method : W:\HPCHEM1\MSVOA U\METHOD\524U043018DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu May 03 10:23:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.75	96	38323	1.00	ug/l	0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	11231	0.90	ug/l	0.00
Spiked Amount	1.000		Recovery	=	90.00%	
68) 1,2-Dichlorobenzene-d4	11.87	152	13003	1.07	ug/l	0.00
Spiked Amount	1.000		Recovery	=	107.00%	


Target Compounds Ovalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU051418\
Data File : VU023848.D
Acq On : 14 May 2018 11:28
Operator : MD/SY
Sample : VU0514WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1





Quant Time: May 15 04:20:00 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\524U043018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu May 03 10:23:54 2018
Response via : Initial Calibration

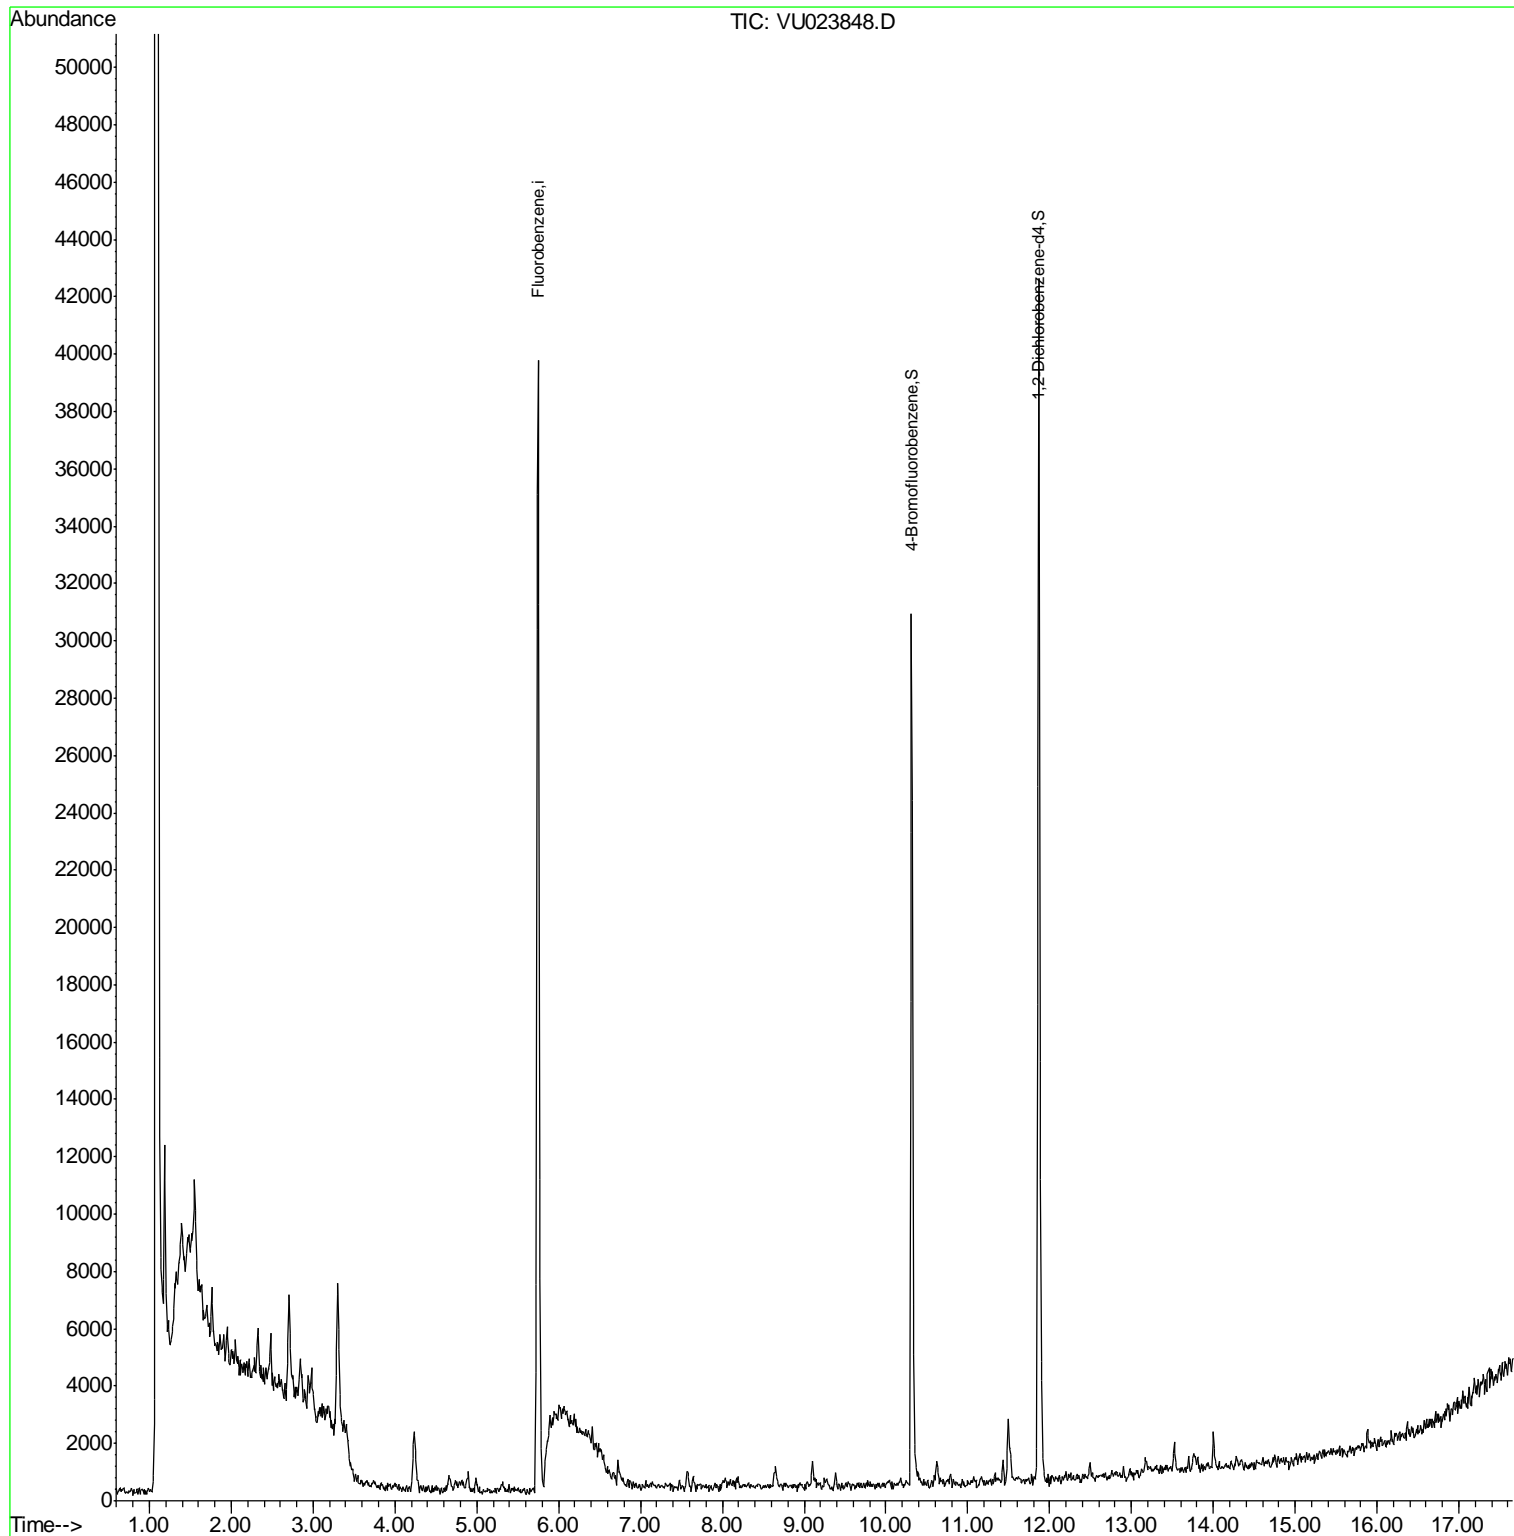

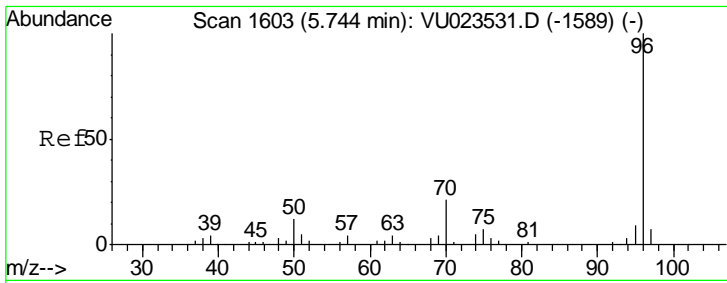




#1
 Fluorobenzene
 Concen: 1.000 ug/l
 RT: 5.75 min Scan# 1604
 Delta R.T. 0.00 min
 Lab File: VU023848.D
 Acq: 14 May 2018 11:28


Tgt Ion	Resp	Lower	Upper
96	38323		
70	20.1	16.2	24.4
95	9.3	6.9	10.3
97	6.4	0.0	0.0

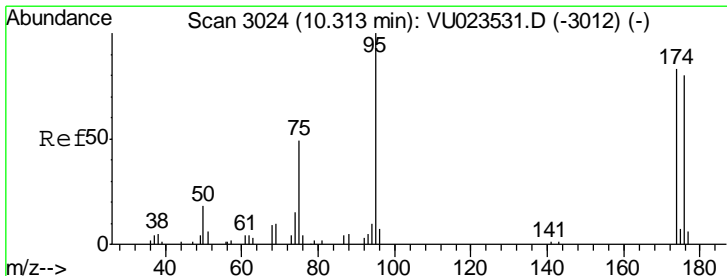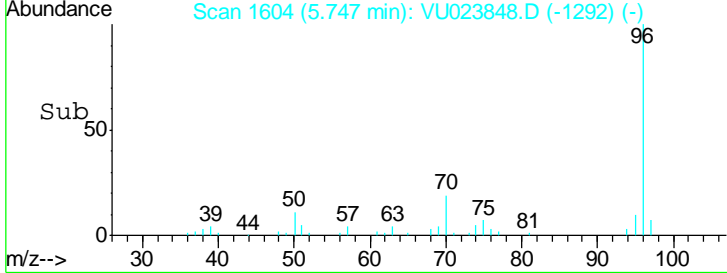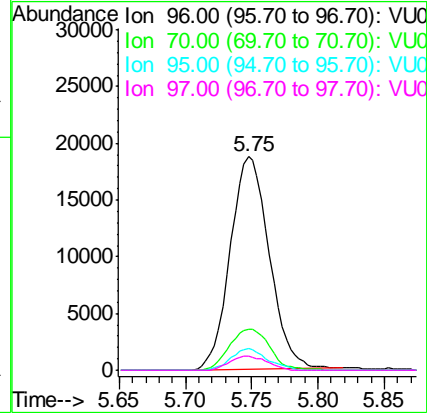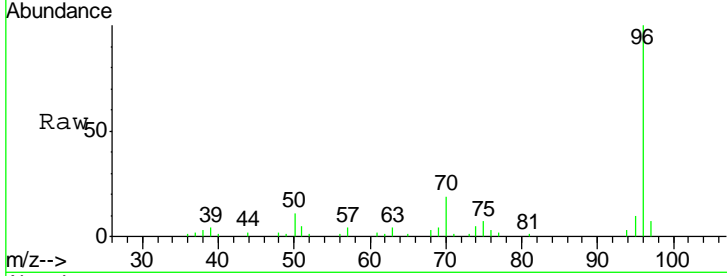

#57
 4-Bromofluorobenzene
 Concen: N.D. ug/l
 RT: 10.31 min Scan# 3024
 Delta R.T. -0.00 min
 Lab File: VU023848.D
 Acq: 14 May 2018 11:28


Tgt Ion	Resp	Lower	Upper
95	11231		
174	90.8	65.6	98.4
176	85.5	62.0	93.0

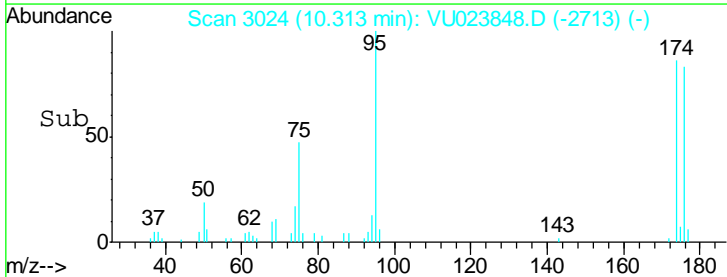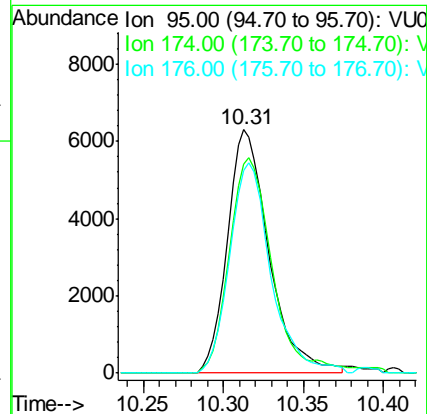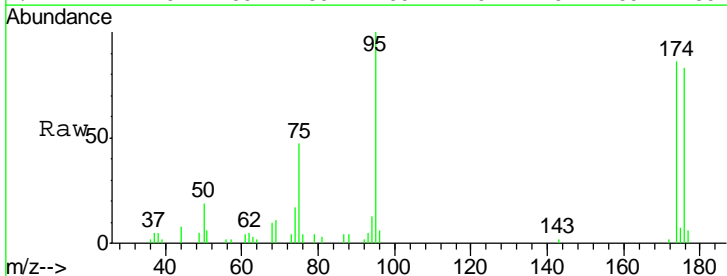

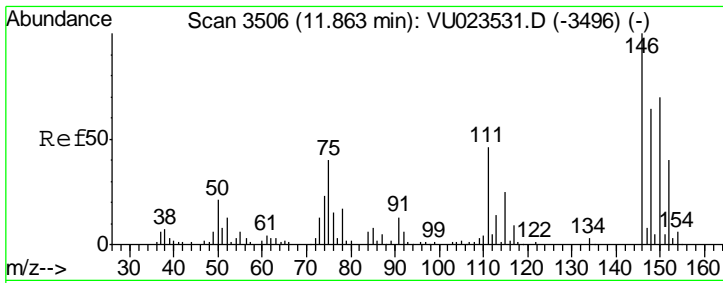

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.87 min Scan# 3507
 Delta R.T. 0.00 min
 Lab File: VU023848.D
 Acq: 14 May 2018 11:28

Tot Ion	Resp	Lower	Upper
152	13003		
152	100		
115	61.0	0.0	118.8
150	156.7	0.0	0.0#

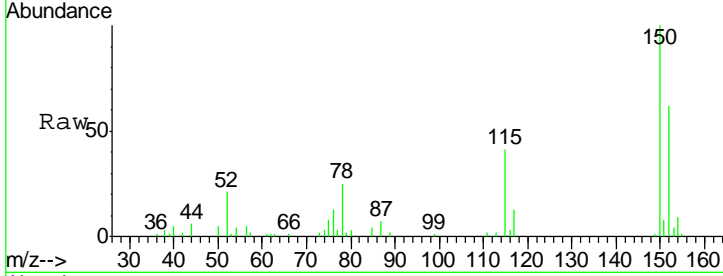

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

