

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU051418\
Data File : VU023852.D
Acq On : 14 May 2018 14:47
Operator : MD/SY
Sample : J2808-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 15 04:36:59 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\524U043018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu May 03 10:23:54 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.75	96	36440	1.00	ug/l	0.00


System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	10294	0.87	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.00%	
68) 1,2-Dichlorobenzene-d4	11.87	152	11999	1.04	ug/l	0.00
Spiked Amount 1.000			Recovery	=	104.00%	


Target Compounds	Ovalue
-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU051418\
Data File : VU023852.D
Acq On : 14 May 2018 14:47
Operator : MD/SY
Sample : J2808-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 15 04:36:59 2018
Quant Method : W:\HPCHEM1\MSVOA U\METHOD\524U043018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu May 03 10:23:54 2018
Response via : Initial Calibration

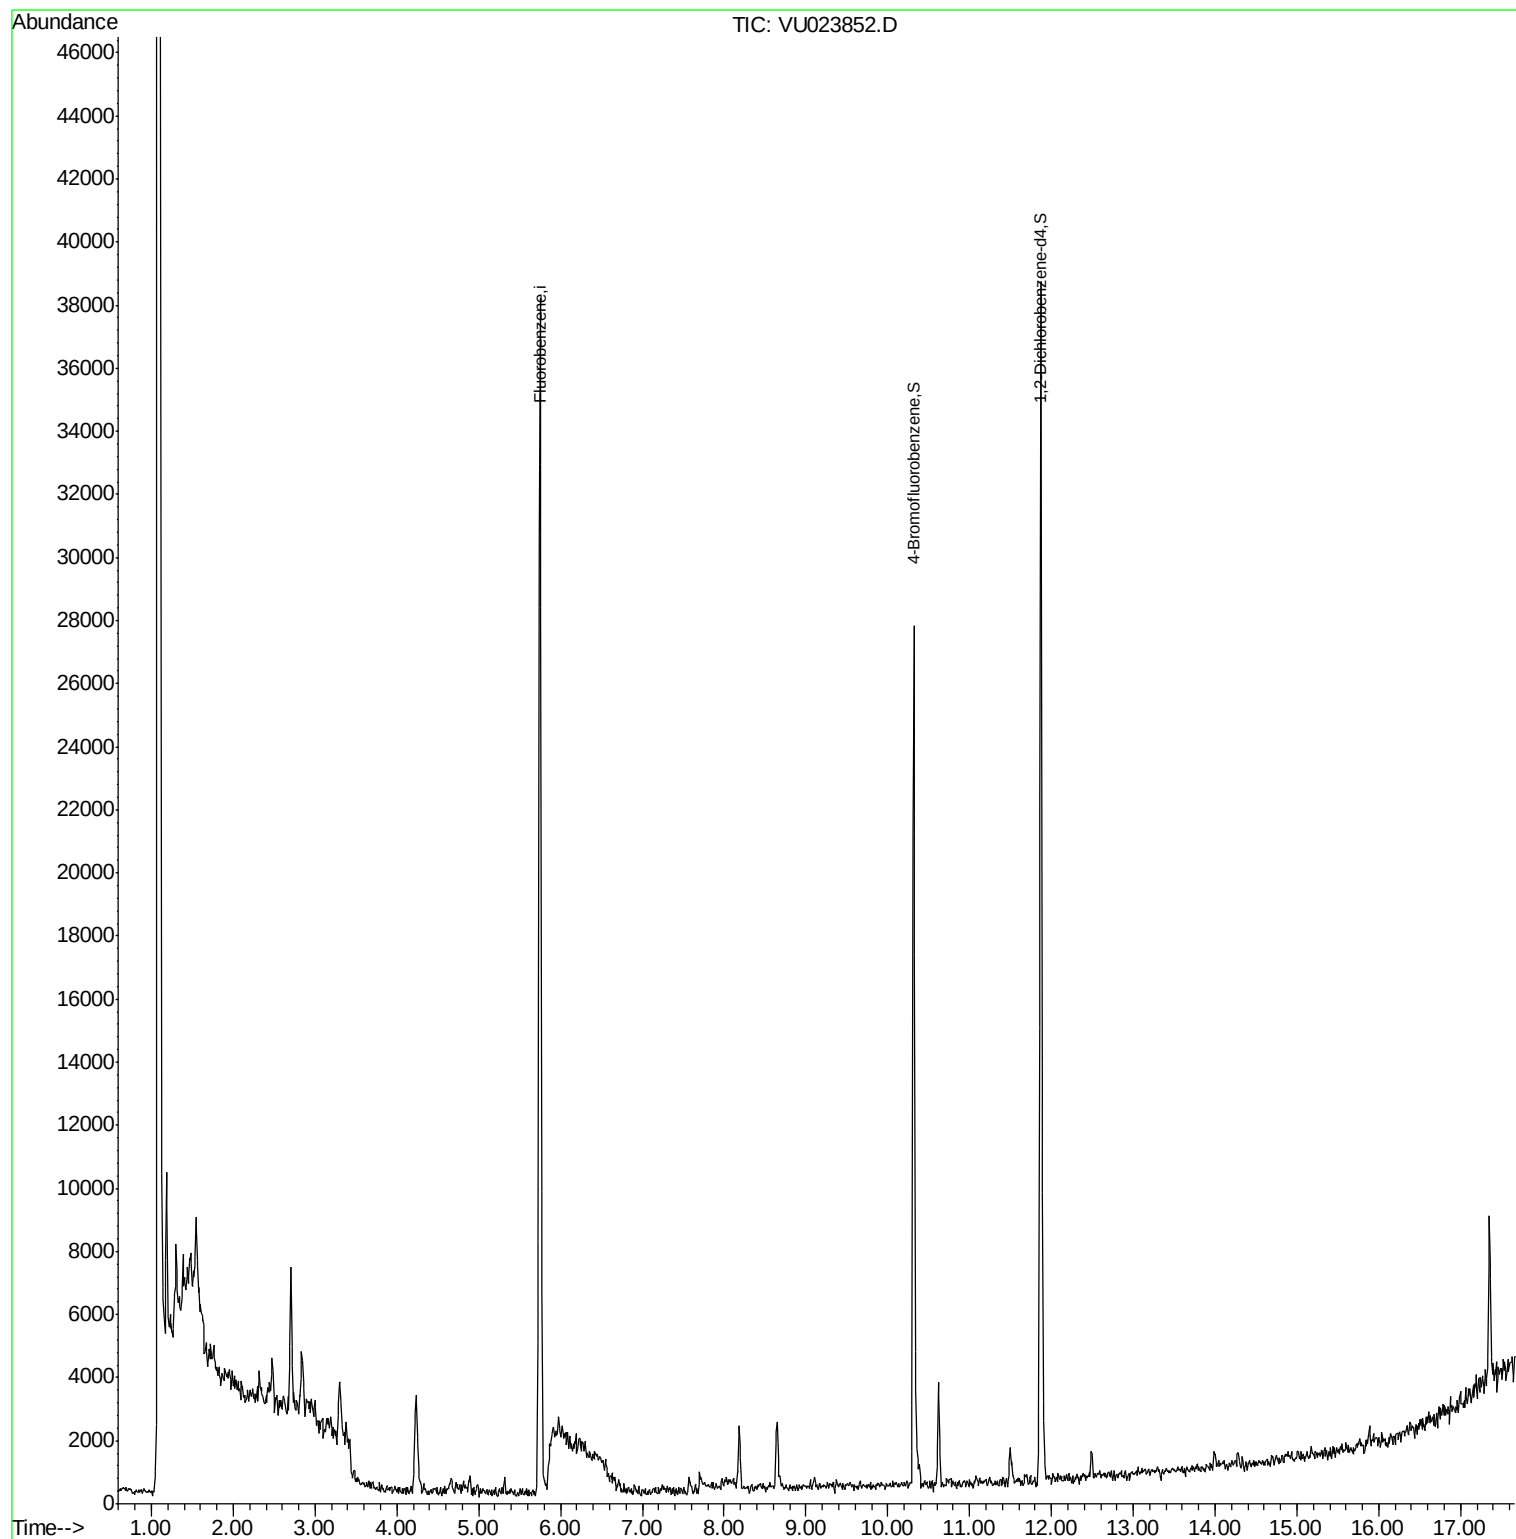

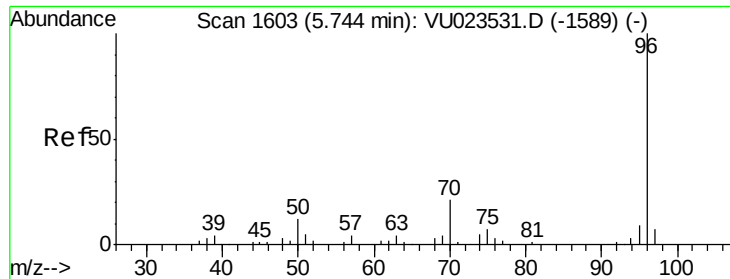

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.75 min Scan# 1604





Delta R.T. 0.00 min

Lab File: VU023852.D

Acq: 14 May 2018 14:47

Tot Ion: 96 Resp: 36440

Ion	Ratio	Lower	Upper
96	100		
70	20.5	16.2	24.4
95	9.0	6.9	10.3
97	6.3	0.0	0.0#

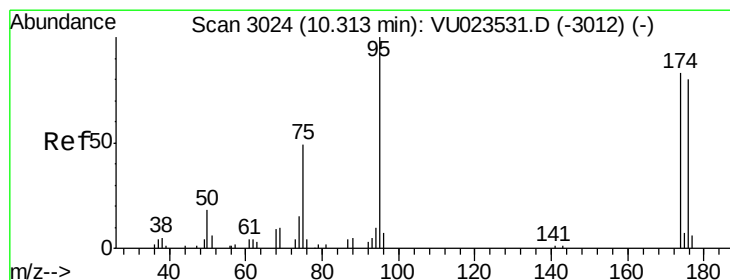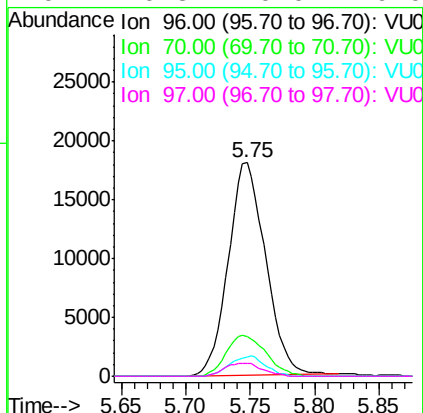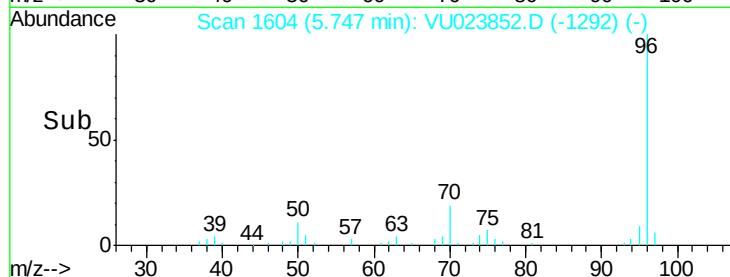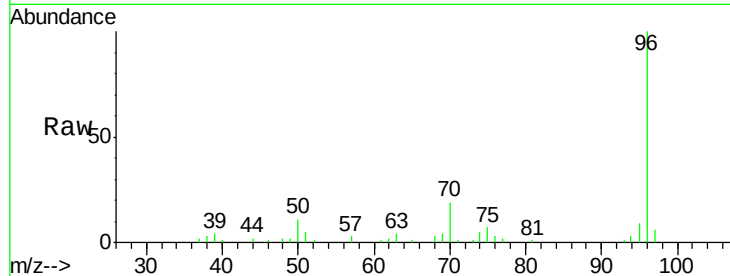

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 3024




Delta R.T. 0.00 min


Lab File: VU023852.D

Acq: 14 May 2018 14:47

Tgt Ion: 95 Resp: 10294


Ion	Ratio	Lower	Upper
95	100		
174	85.6	65.6	98.4
176	86.1	62.0	93.0

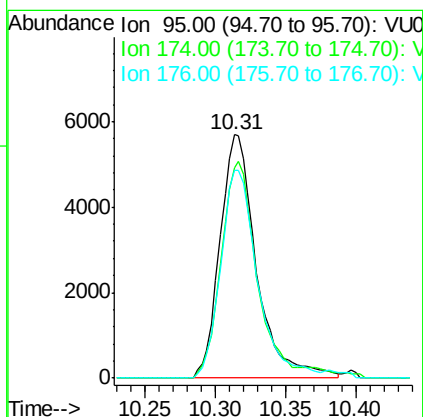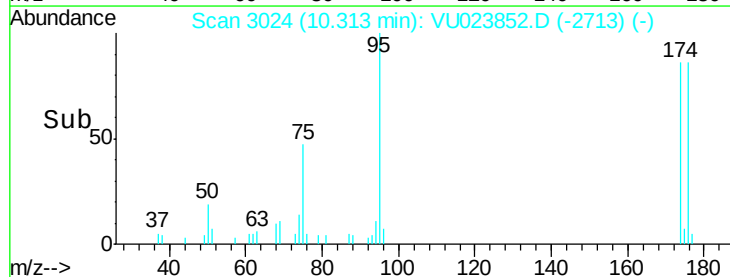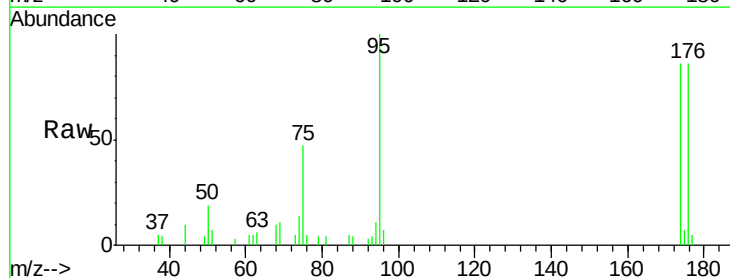

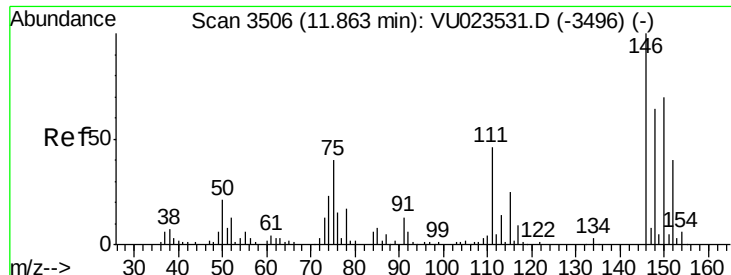

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.87 min Scan# 3508
 Delta R.T. 0.01 min
 Lab File: VU023852.D
 Acq: 14 May 2018 14:47

Tot Ion	Ratio	Lower	Upper
152	100		
115	61.5	0.0	118.8
150	155.7	0.0	0.0#

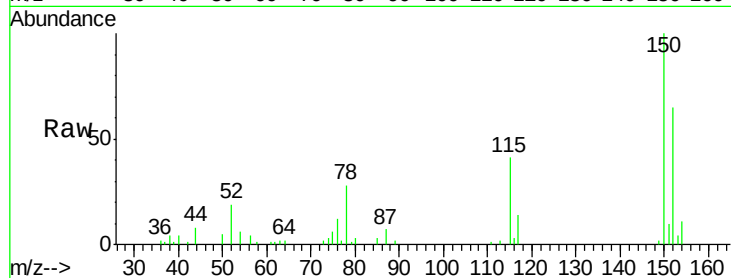

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

