


Data Path : W:\HPCHEM1\MSVOA U\Data\VU051418\
 Data File : VU023846.D
 Acq On : 14 May 2018 10:18
 Operator : MD/SY
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_U\METHOD\524U043018DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu May 03 10:23:54 2018

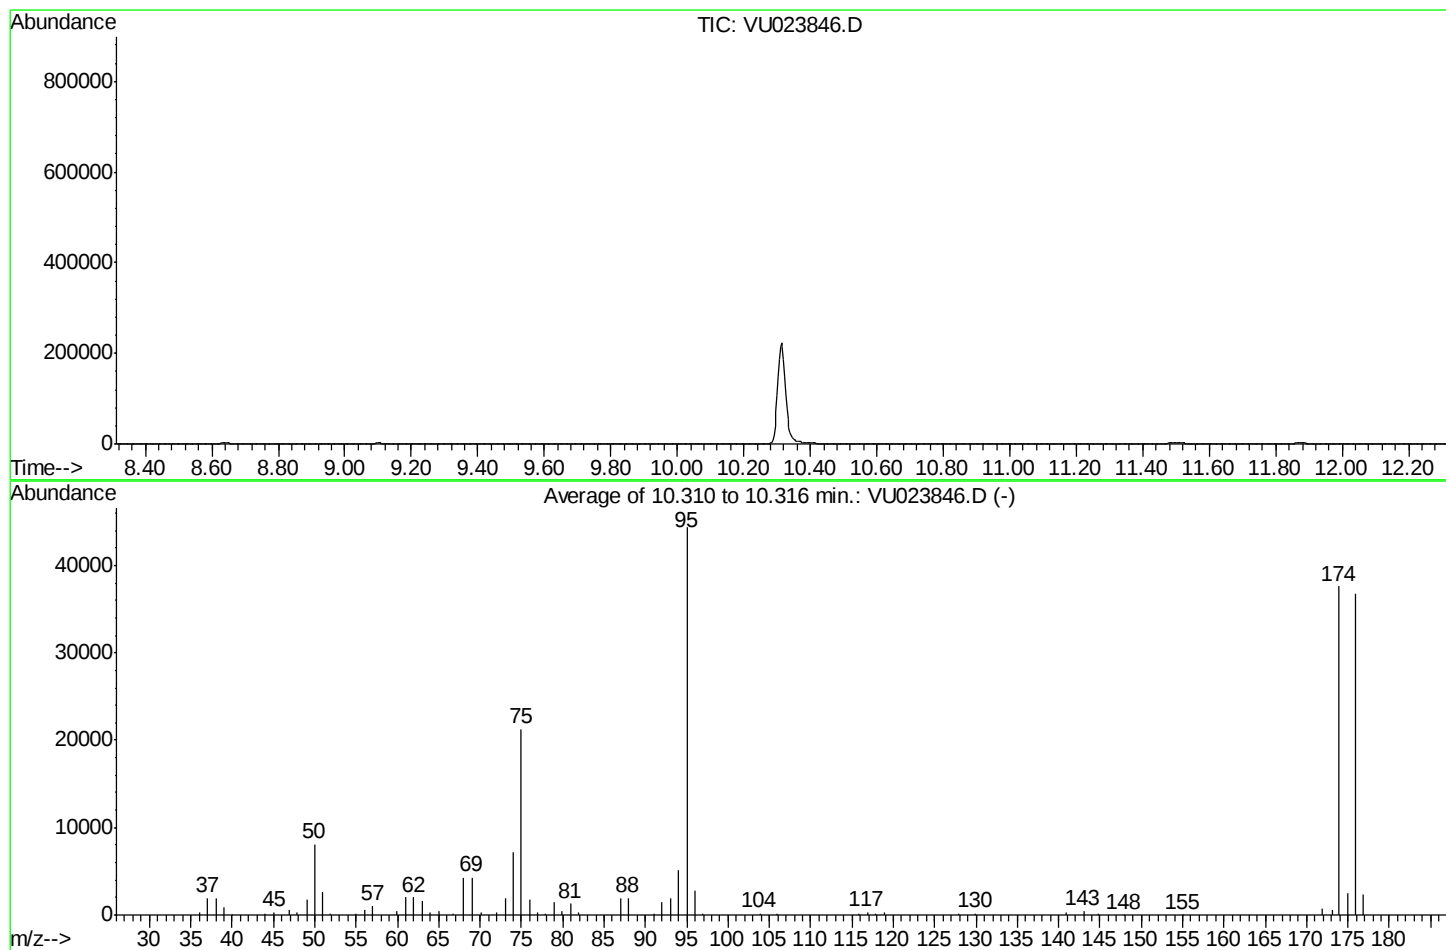

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	8062	PASS
75	95	30	60	47.9	21264	PASS
95	95	100	100	100.0	44357	PASS
96	95	5	9	6.3	2792	PASS
173	174	0.00	2	1.5	555	PASS
174	95	50	100	84.7	37592	PASS
175	174	5	9	6.8	2549	PASS
176	174	95	101	97.6	36704	PASS
177	176	5	9	6.6	2411	PASS