
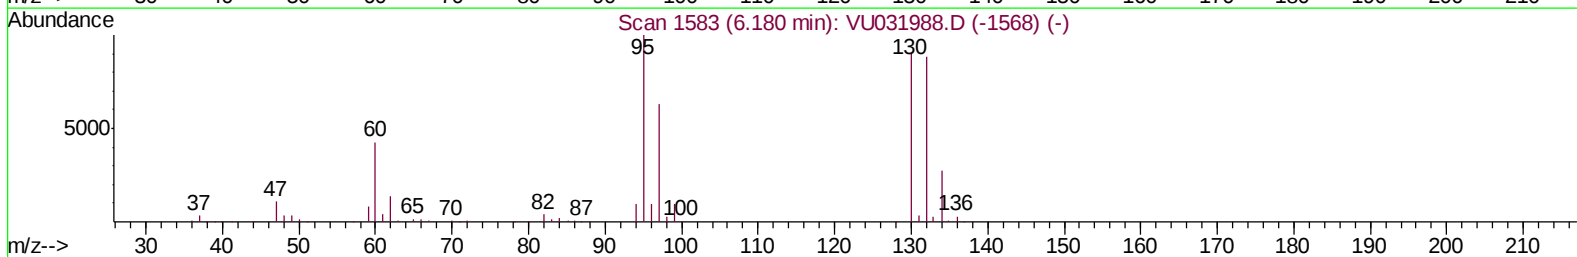
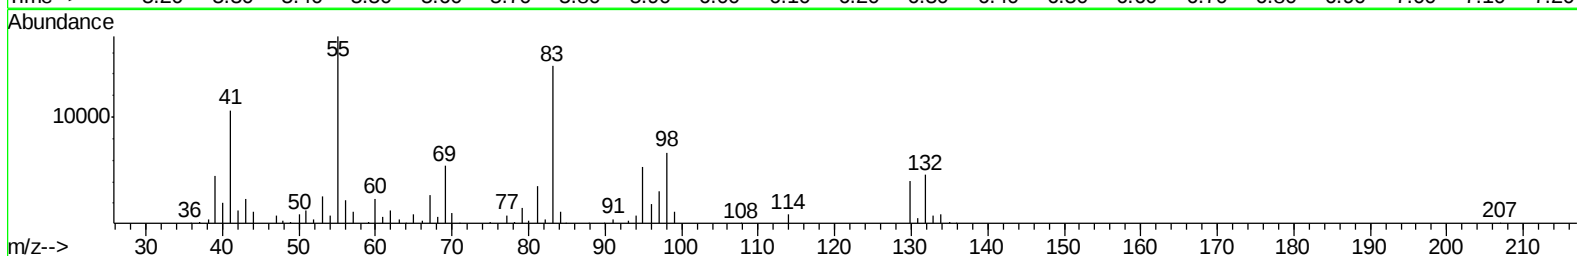


Data File : VU032011.D
Acq On : 14 May 2019 21:45
Operator : JC/SP
Sample : K2738-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Quant Time: May 15 04:32:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 15 04:26:34 2019
Response via : Initial Calibration

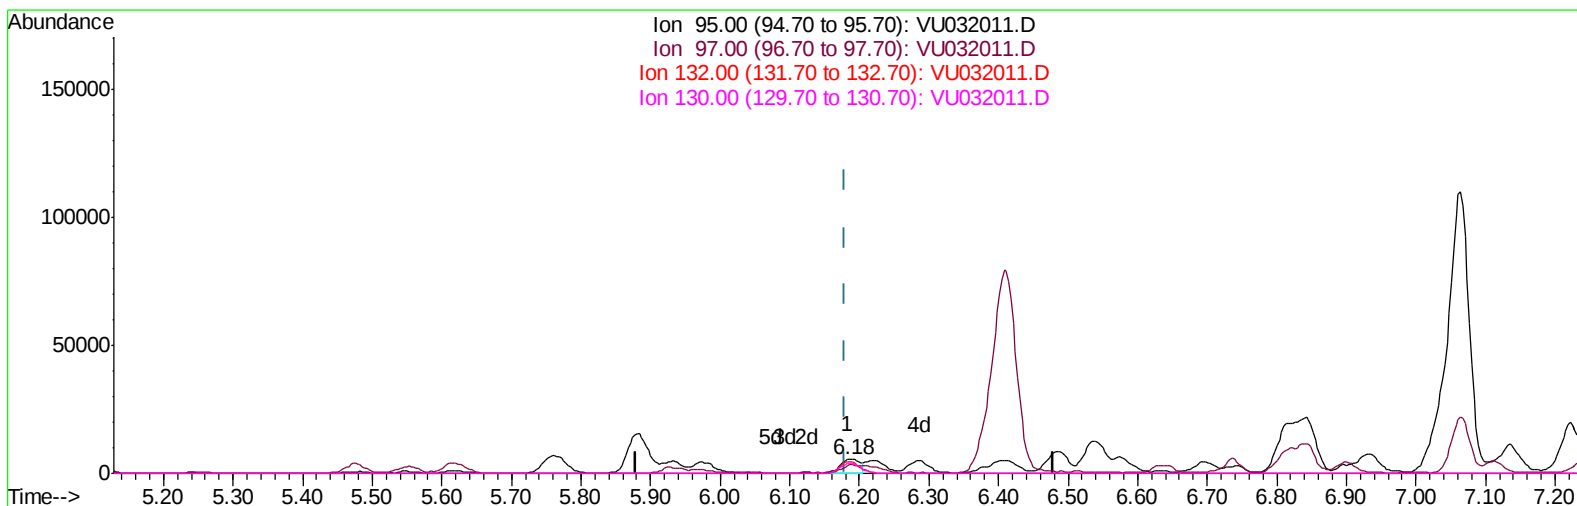

TIC: VU032011.D

(34) Trichloroethene (T)

6.183min (+0.003) 1.22ug/L m

response 11403

Ion	Exp%	Act%
95.00	100	100
97.00	64.10	58.97
132.00	90.70	86.72
130.00	94.60	75.29