

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051419\
 Data File : VU032004.D
 Acq On : 14 May 2019 19:00
 Operator : JC/SP
 Sample : K2738-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB888

Quant Time: May 15 05:21:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 15 04:26:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	1176266	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	1173967	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	542493	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	402860	39.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.06%
7) Chloroethane-d5	1.68	69	340879	40.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.58%
11) 1,1-Dichloroethene-d2	2.27	63	549942	29.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.44%#
21) 2-Butanone-d5	4.17	46	639554	88.49	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.49%
24) Chloroform-d	4.64	84	698031	40.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.80%
26) 1,2-Dichloroethane-d4	5.30	65	452520	41.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.16%
32) Benzene-d6	5.34	84	1499299	44.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.22%
36) 1,2-Dichloropropane-d6	6.32	67	495686	44.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.40%
41) Toluene-d8	7.56	98	1470311	48.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.58%
43) trans-1,3-Dichloropropene-	7.85	79	225033	45.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.98%
47) 2-Hexanone-d5	8.31	63	434340	95.51	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.51%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	712806	42.95	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.90%
64) 1,2-Dichlorobenzene-d4	11.86	152	511184	44.78	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.56%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.32	43	92174	12.405	ug/L	89
17) trans-1,2-Dichloroethene	2.98	96	25371	2.807	ug/L	93
22) 2-Butanone	4.28	43	27563	3.216	ug/L	80
29) Cyclohexane	4.99	56	4534004	315.077	ug/L	98
33) Benzene	5.39	78	17215	0.448	ug/L	100
35) Methylcyclohexane	6.41	83	7187299	492.183	ug/L	97
42) Toluene	7.64	91	29457	0.746	ug/L	93
46) Tetrachloroethene	8.22	164	4363	0.649	ug/L	95
52) Ethylbenzene	9.24	91	1562900	37.011	ug/L	100
53) m,p-Xylene	9.37	106	91452	5.934	ug/L	96
56) Isopropylbenzene	10.16	105	9068982	232.617	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051419\
Data File : VU032004.D
Acq On : 14 May 2019 19:00
Operator : JC/SP
Sample : K2738-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB888

Quant Time: May 15 05:21:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 15 04:26:34 2019
Response via : Initial Calibration

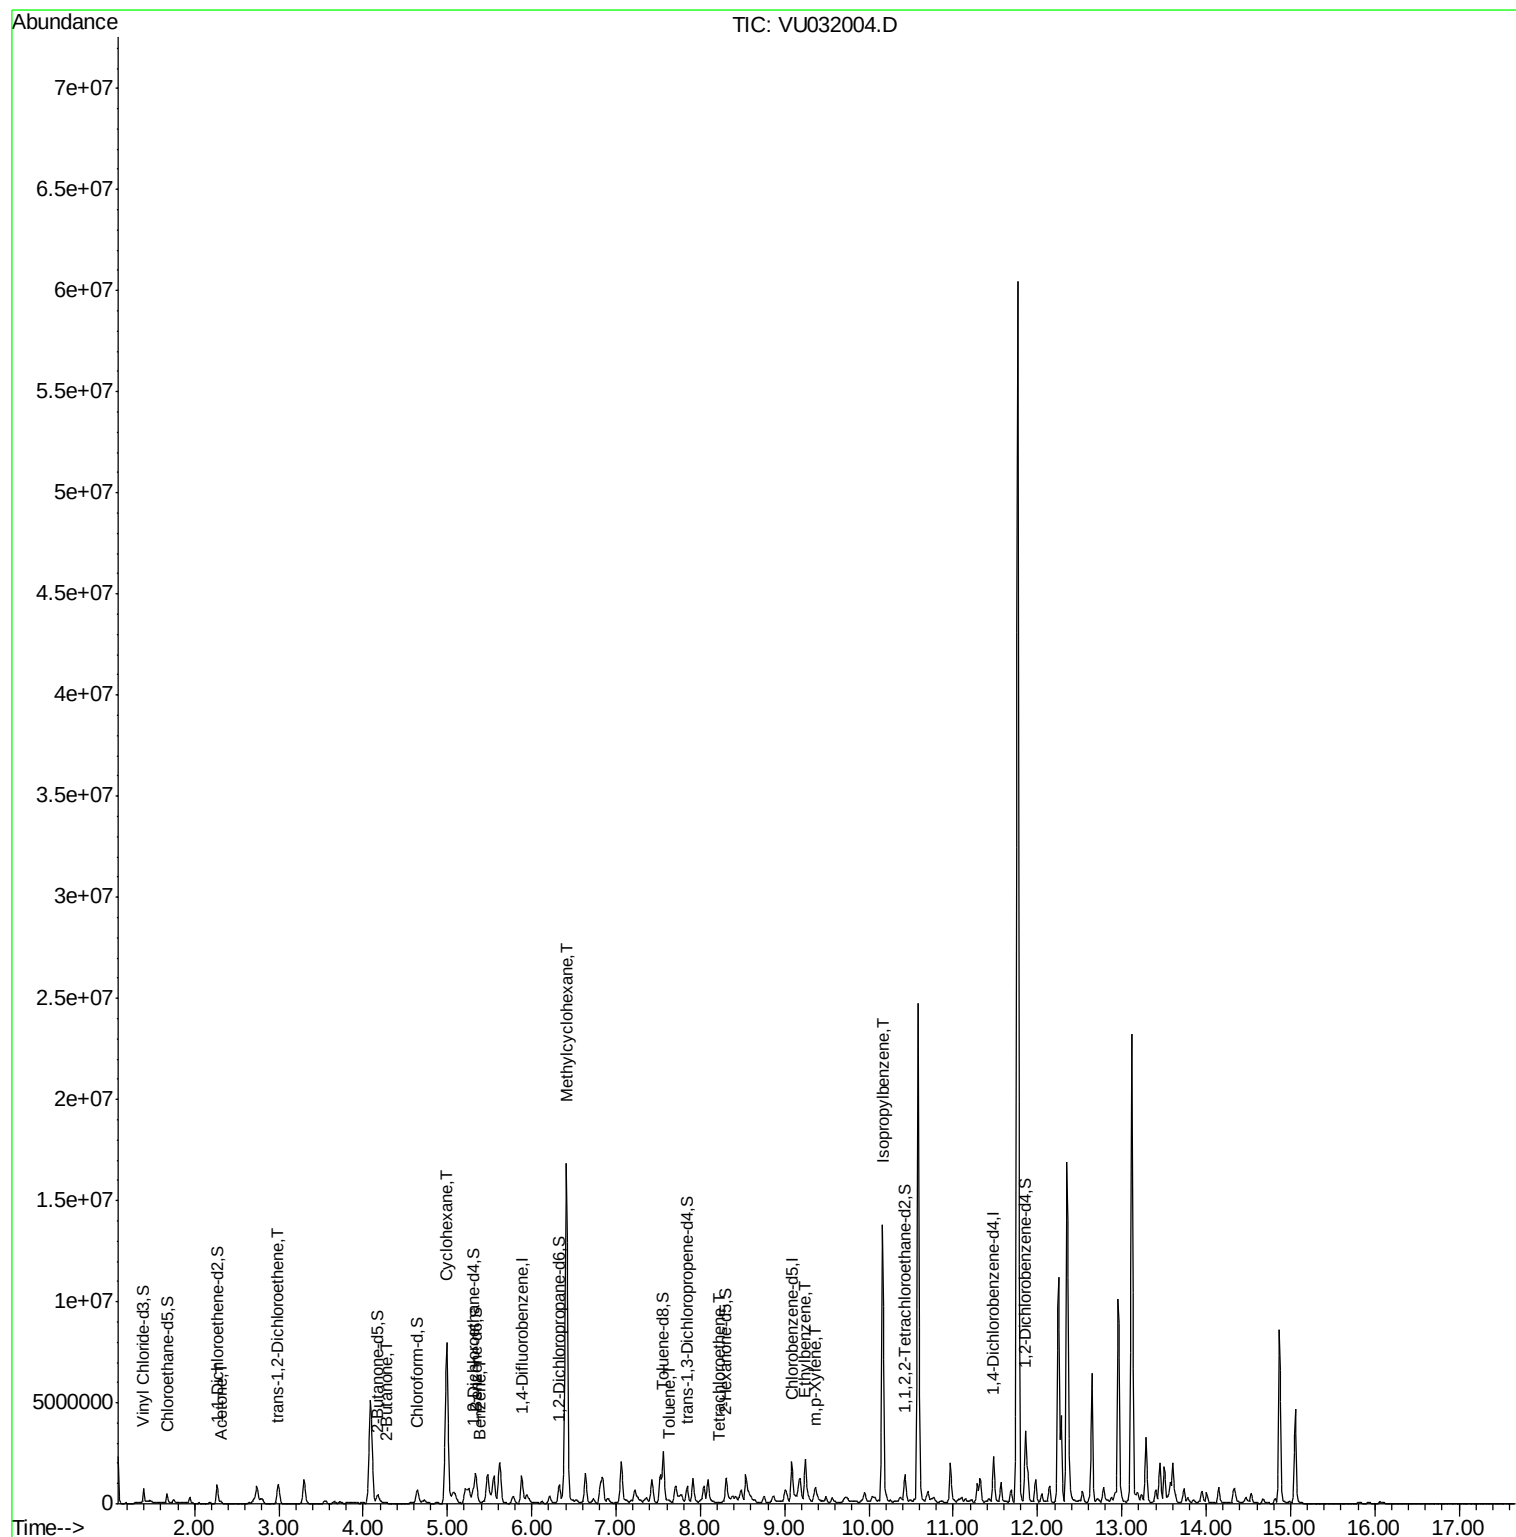

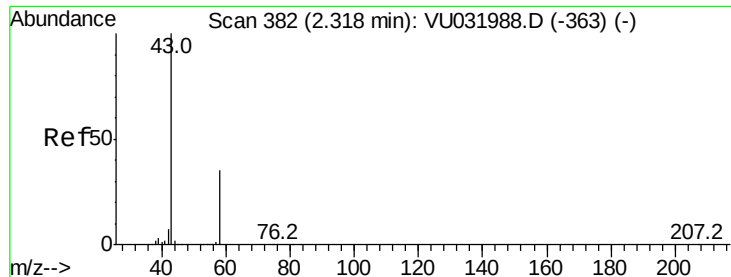

#13

Acetone

Concen: 12.405 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00

Instrument :

MSVOA_U

ClientSampled :


DB888

Tot Ion: 43 Resp: 92174

Ion Ratio Lower Upper




43 100

58 28.0 0.0 68.2

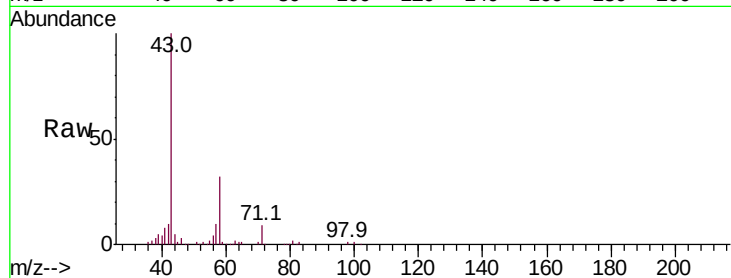

Abundance Ion 43.00 (42.70 to 43.70): VU031988.D (-363) (-)

Ion 58.00 (57.70 to 58.70): VU031988.D (-363) (-)

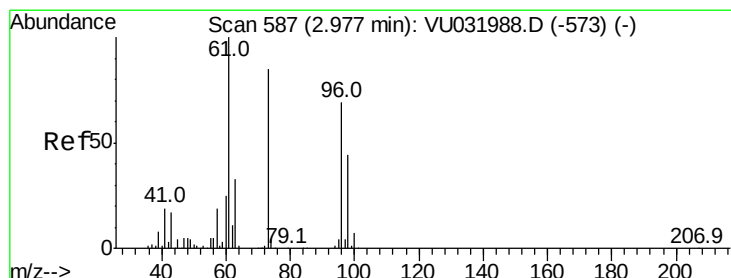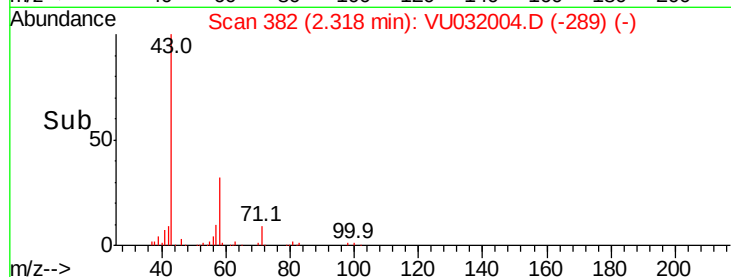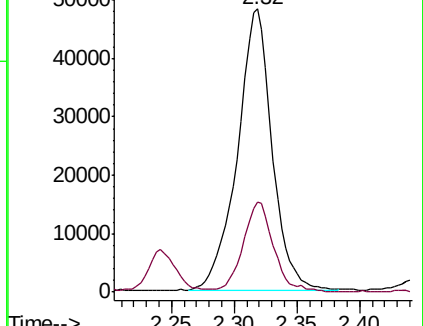

#17

trans-1,2-Dichloroethene

Concen: 2.807 ug/L

RT: 2.98 min Scan# 588

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00


Tgt Ion: 96 Resp: 25371

Ion Ratio Lower Upper

96 100

61 154.4 103.2 191.6



98 56.2 45.7 84.9

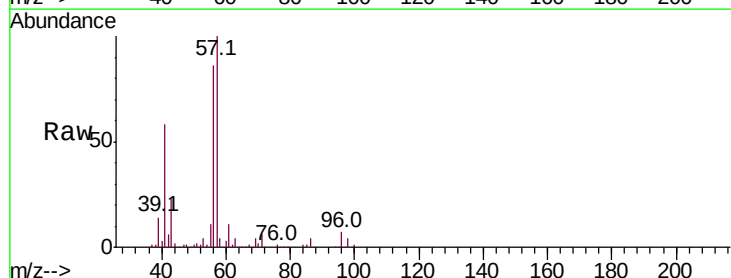


Abundance Ion 96.00 (95.70 to 96.70): VU031988.D (-573) (-)

Ion 61.00 (60.70 to 61.70): VU031988.D (-573) (-)

Ion 98.00 (97.70 to 98.70): VU031988.D (-573) (-)

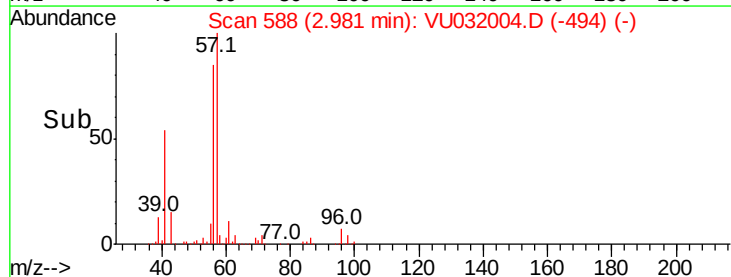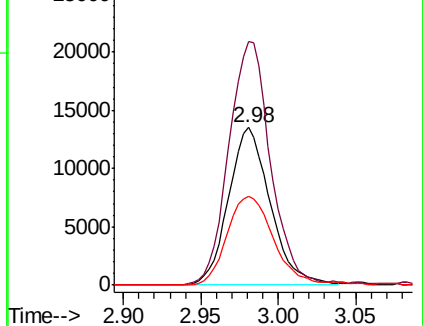

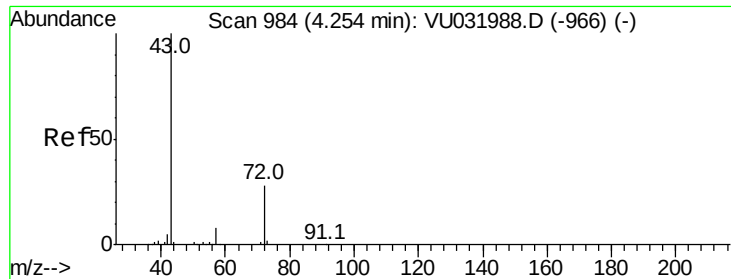

#22

2-Butanone

Concen: 3.216 ug/L

RT: 4.28 min Scan# 991

Delta R.T. 0.02 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00

Instrument :

MSVOA_U

ClientSampled :





DB888

Tot Ion: 43 Resp: 27563

Ion Ratio Lower Upper

43 100

72 17.3 13.9 41.7

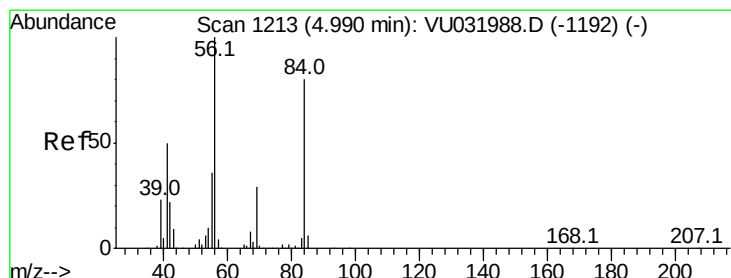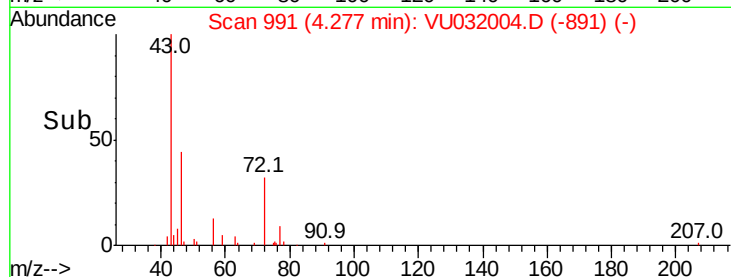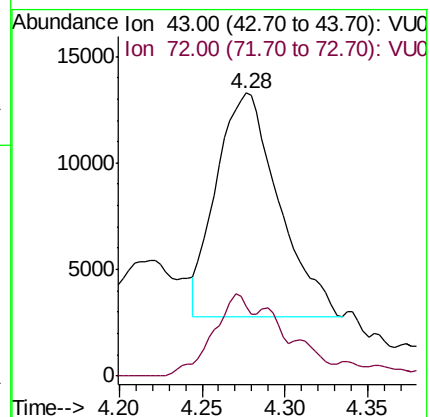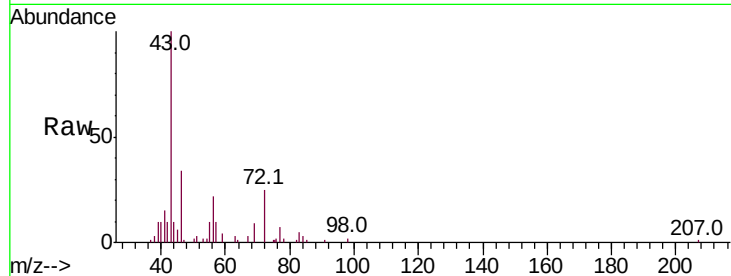

#29

Cyclohexane

Concen: 315.077 ug/L

RT: 4.99 min Scan# 1213

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00




Tgt Ion: 56 Resp: 4534004


Ion Ratio Lower Upper

56 100

69 33.0 24.8 37.2

84 80.9 65.5 98.3

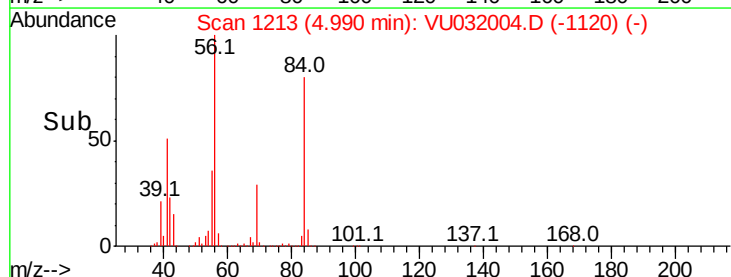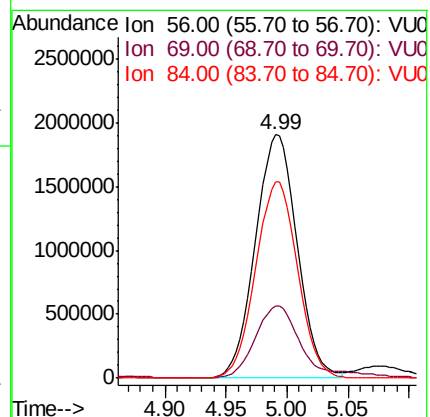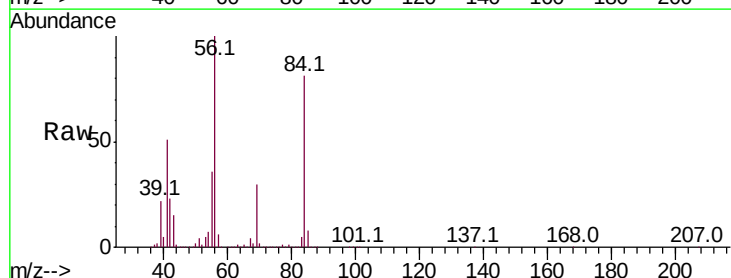

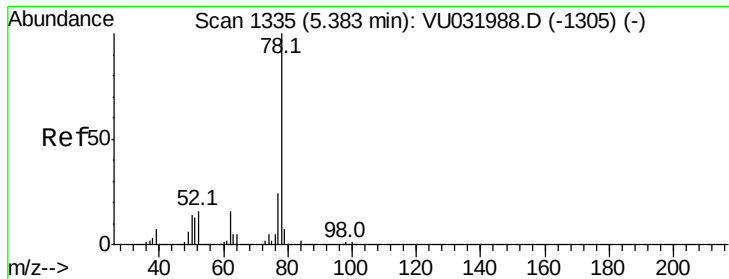

#33

Benzene

Concen: 0.448 ug/L

RT: 5.39 min Scan# 1337

Delta R.T. 0.01 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00


Instrument :

MSVOA_U




ClientSampleId :

DB888

Tgt Ion: 78 Resp: 17215

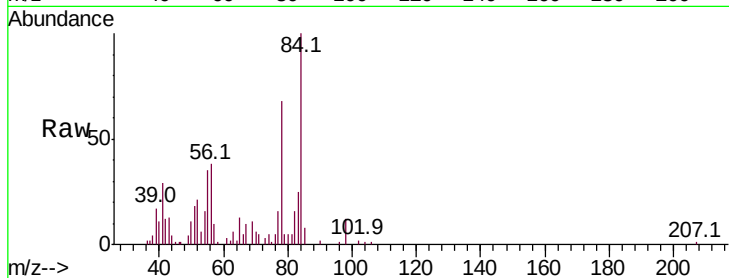

Abundance Ion 78.00 (77.70 to 78.70): VU0

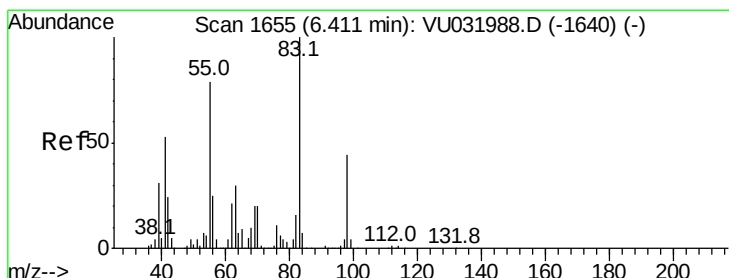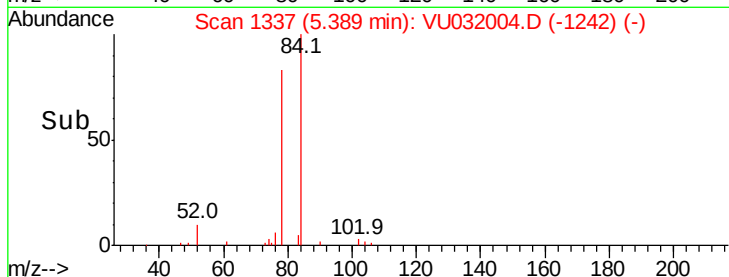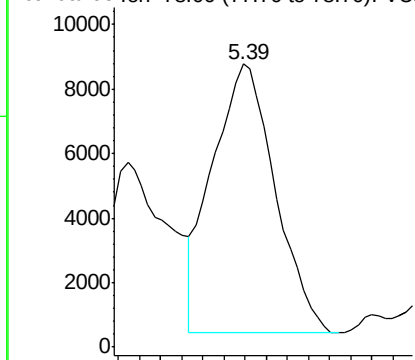

#35

Methylcyclohexane

Concen: 492.183 ug/L

RT: 6.41 min Scan# 1655

Delta R.T. 0.00 min

Lab File: VU032004.D


Acq: 14 May 2019 19:00

Tgt Ion: 83 Resp: 7187299

Ion	Ratio	Lower	Upper
83	100		

55	83.1	64.0	96.0
----	------	------	------



98	44.0	35.6	53.4
----	------	------	------

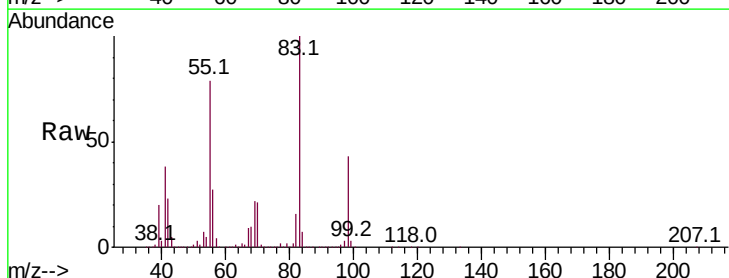


Abundance Ion 83.00 (82.70 to 83.70): VU0

Ion 55.00 (54.70 to 55.70): VU0

Ion 98.00 (97.70 to 98.70): VU0

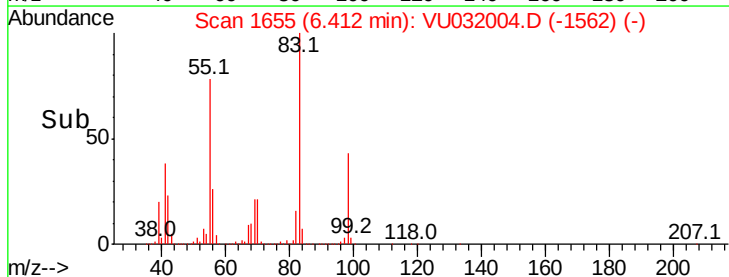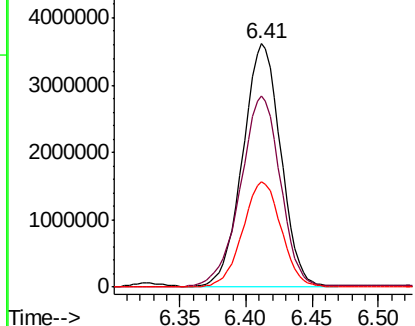

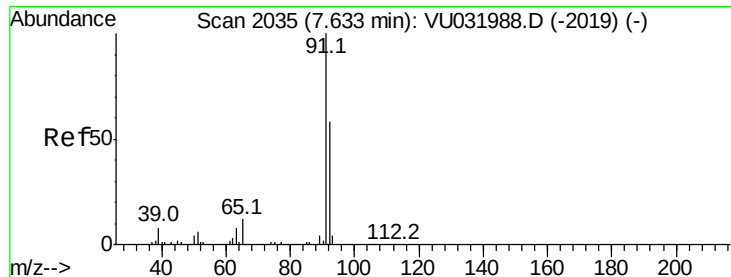

#42

Toluene

Concen: 0.746 ug/L

RT: 7.64 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :


DB888

Tot Ion: 91 Resp: 29457

Ion Ratio Lower Upper




91 100

92 52.2 40.2 74.6

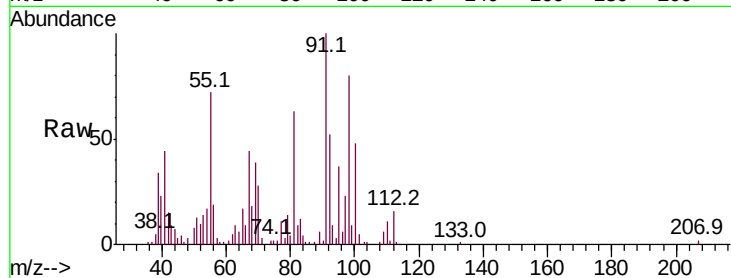

Abundance Ion 91.00 (90.70 to 91.70): VU031988.D (-2019) (-)

Ion 92.00 (91.70 to 92.70): VU031988.D (-2019) (-)

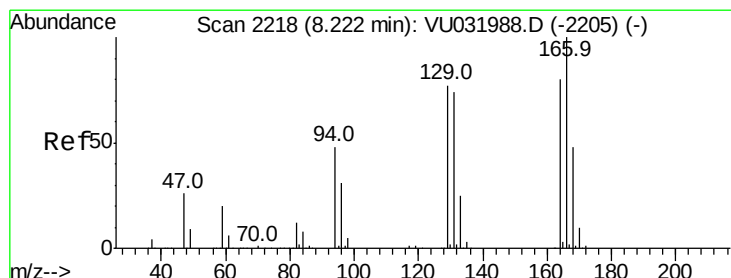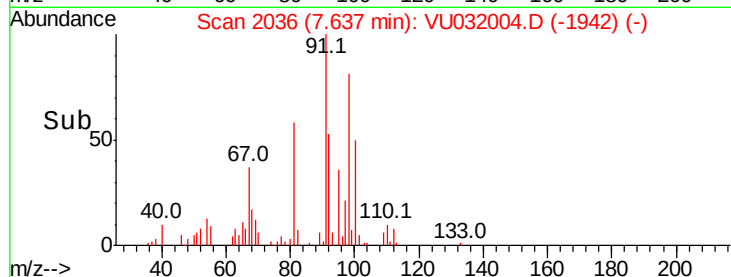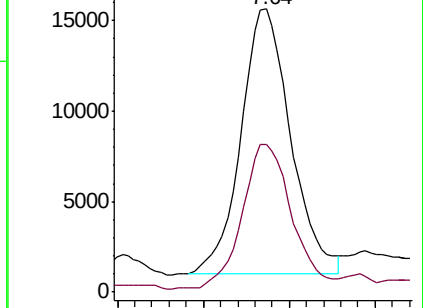

#46

Tetrachloroethene

Concen: 0.649 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00

Tgt Ion: 164 Resp: 4363


Ion Ratio Lower Upper

164 100

129 98.7 70.9 131.7

131 92.5 67.4 125.2

166 120.3 90.2 167.4


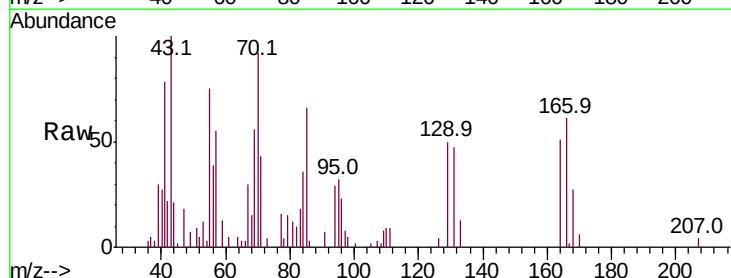



Abundance Ion 164.00 (163.70 to 164.70): VU031988.D (-2205) (-)

Ion 129.00 (128.70 to 129.70): VU031988.D (-2205) (-)

Ion 131.00 (130.70 to 131.70): VU031988.D (-2205) (-)

Ion 166.00 (165.70 to 166.70): VU031988.D (-2205) (-)

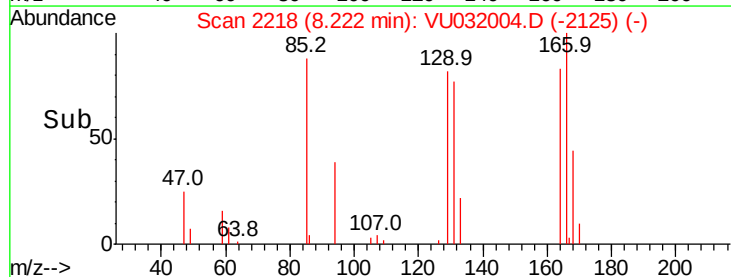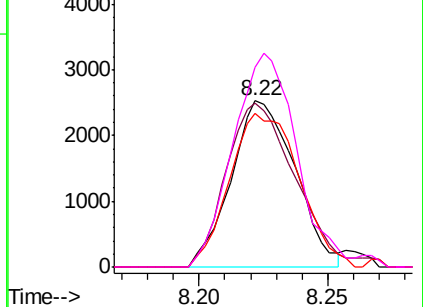

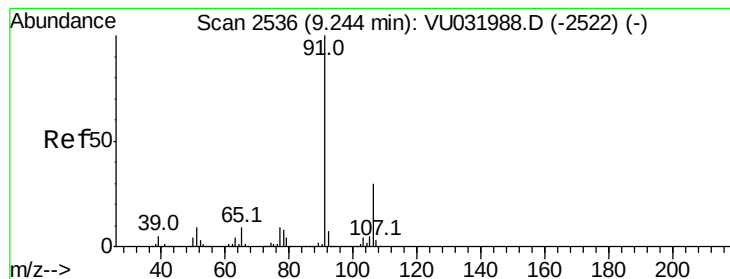

#52

Ethylbenzene

Concen: 37.011 ug/L

RT: 9.24 min Scan# 2536

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :





DB888

Tot Ion: 91 Resp: 1562900

Ion Ratio Lower Upper

91 100

106 30.5 21.3 39.5

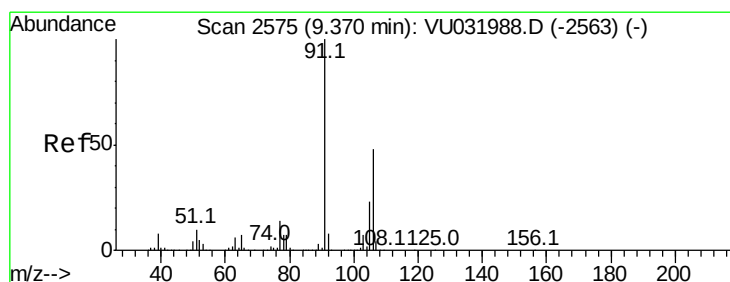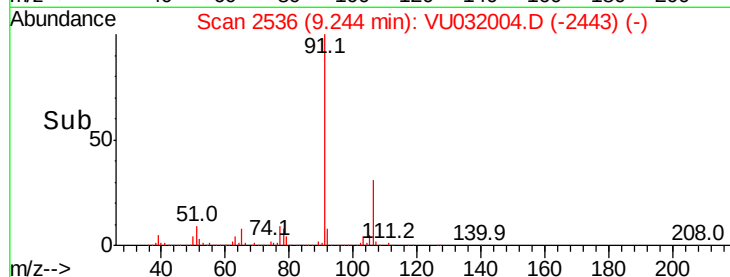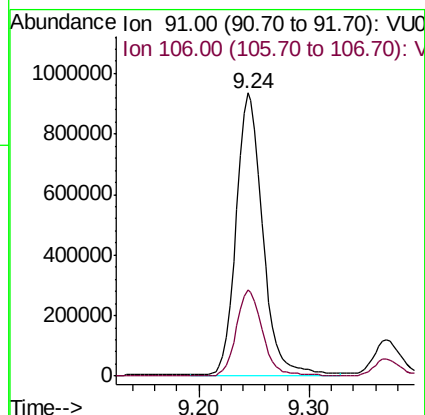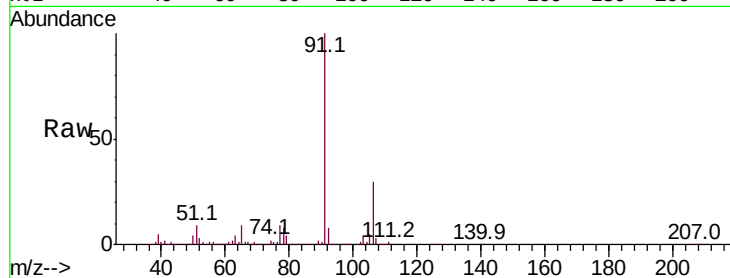

#53

m,p-Xylene

Concen: 5.934 ug/L

RT: 9.37 min Scan# 2575

Delta R.T. 0.00 min

Lab File: VU032004.D




Acq: 14 May 2019 19:00


Tgt Ion: 106 Resp: 91452

Ion Ratio Lower Upper

106 100

91 213.3 144.8 269.0

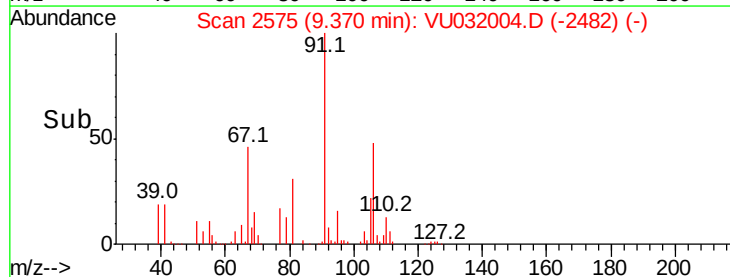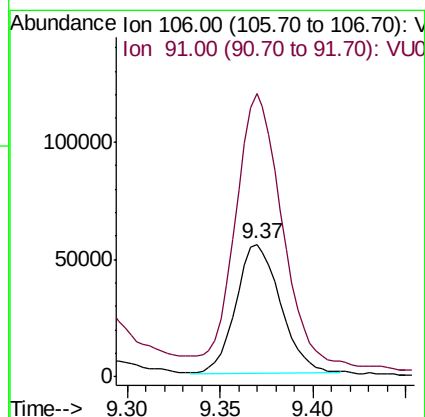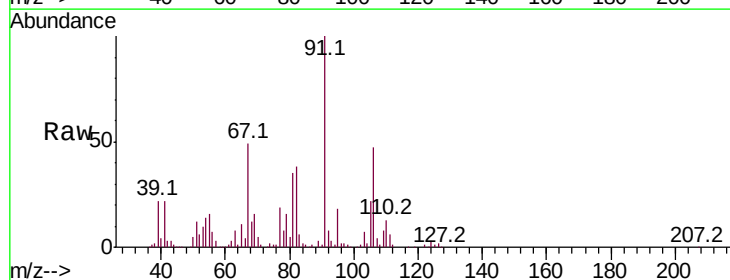

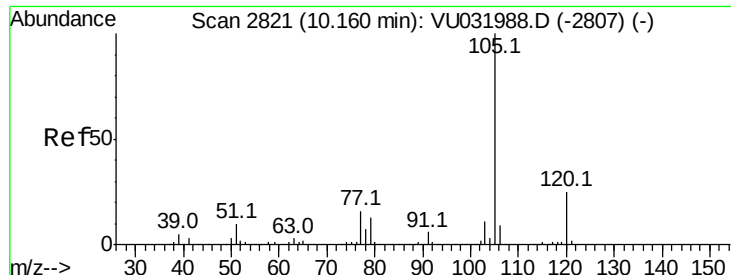

#56

Isopropylbenzene

Concen: 232.617 ug/L

RT: 10.16 min Scan# 2821

Delta R.T. 0.00 min

Lab File: VU032004.D

Acq: 14 May 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :

DB888


Tot Ion:105 Resp: 9068982

Ion Ratio Lower Upper

105 100

120 25.5 20.5 30.7

77 16.3 13.0 19.4

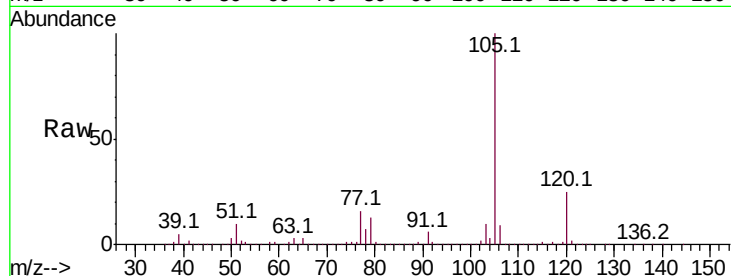

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VU0

