

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051419\
 Data File : VU032007.D
 Acq On : 14 May 2019 20:11
 Operator : JC/SP
 Sample : K2738-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB893

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	39	rVB3	21072	21058	0.48%	0.057%
2	1.396	88	95	107	rBV	626751	667264	15.21%	1.801%
3	1.675	174	182	198	rVB	457206	611176	13.93%	1.649%
4	2.267	356	366	378	rBV	987997	1489288	33.94%	4.019%
5	2.444	412	421	434	rBV2	16092	32575	0.74%	0.088%
6	2.543	449	452	455	rBV6	1020	897	0.02%	0.002%
7	2.695	496	499	510	rVB9	3247	3816	0.09%	0.010%
8	2.830	530	541	553	rBV2	6766	14226	0.32%	0.038%
9	2.981	575	588	601	rBV3	16690	32629	0.74%	0.088%
10	3.029	601	603	606	rVV2	1119	626	0.01%	0.002%
11	3.045	606	608	613	rVV2	1062	992	0.02%	0.003%
12	3.090	617	622	625	rBV4	1324	1239	0.03%	0.003%
13	3.193	649	654	657	rVB4	849	814	0.02%	0.002%
14	3.225	662	664	670	rBV4	916	1000	0.02%	0.003%
15	3.293	681	685	686	rBV3	1074	781	0.02%	0.002%
16	3.322	691	694	697	rVB3	975	614	0.01%	0.002%
17	3.441	728	731	736	rVB2	1203	1031	0.02%	0.003%
18	3.527	756	758	764	rVB3	1187	1036	0.02%	0.003%
19	3.566	764	770	777	rBV3	893	1052	0.02%	0.003%
20	3.646	792	795	799	rVB3	883	646	0.01%	0.002%
21	3.685	799	807	810	rBV3	876	1177	0.03%	0.003%
22	3.791	837	840	844	rBV3	909	683	0.02%	0.002%
23	3.839	852	855	858	rVV2	900	636	0.01%	0.002%
24	3.871	861	865	871	rVB4	601	671	0.02%	0.002%
25	4.068	921	926	928	rBV4	977	902	0.02%	0.002%
26	4.096	933	935	941	rVB4	1926	1643	0.04%	0.004%
27	4.170	946	958	965	rBV	394494	873584	19.91%	2.358%
28	4.643	1087	1105	1132	rBV	698962	1665500	37.96%	4.495%
29	5.077	1237	1240	1245	rVB6	1178	1009	0.02%	0.003%
30	5.241	1287	1291	1296	rBV5	857	975	0.02%	0.003%
31	5.334	1296	1320	1359	rBV2	1455671	4387865	100.00%	11.842%
32	5.881	1477	1490	1536	rBV	1266268	2620109	59.71%	7.071%
33	6.183	1571	1584	1610	rBV	253517	527351	12.02%	1.423%
34	6.325	1615	1628	1653	rBV	957339	1933940	44.07%	5.219%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051419\
 Data File : VU032007.D
 Acq On : 14 May 2019 20:11
 Operator : JC/SP
 Sample : K2738-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB893

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	6.540	1692	1695	1696	rBV3	1421	796	0.02%	0.002%
36	6.691	1738	1742	1747	rVB5	1048	892	0.02%	0.002%
37	6.768	1764	1766	1772	rVB5	1372	1149	0.03%	0.003%
38	6.826	1781	1784	1787	rVV4	1292	903	0.02%	0.002%
39	6.842	1787	1789	1795	rVB5	1143	823	0.02%	0.002%
40	6.926	1812	1815	1820	rVB6	1103	1014	0.02%	0.003%
41	6.955	1820	1824	1827	rBV3	936	669	0.02%	0.002%
42	7.013	1839	1842	1848	rVB3	973	845	0.02%	0.002%
43	7.093	1864	1867	1871	rVB3	1492	1071	0.02%	0.003%
44	7.119	1871	1875	1878	rBV3	648	714	0.02%	0.002%
45	7.164	1887	1889	1894	rVB3	1058	1023	0.02%	0.003%
46	7.225	1894	1908	1929	rBV2	497578	925444	21.09%	2.498%
47	7.463	1978	1982	1985	rBV4	1863	1581	0.04%	0.004%
48	7.559	1996	2012	2063	rBV	1850906	3470069	79.08%	9.365%
49	7.846	2090	2101	2134	rBV	343663	615085	14.02%	1.660%
50	8.042	2155	2162	2168	rVB8	2805	3905	0.09%	0.011%
51	8.090	2175	2177	2179	rBV2	1180	608	0.01%	0.002%
52	8.151	2191	2196	2197	rBV3	1296	1047	0.02%	0.003%
53	8.167	2197	2201	2204	rVV4	2692	2421	0.06%	0.007%
54	8.222	2205	2218	2235	rVV	2103587	3650690	83.20%	9.853%
55	8.305	2235	2244	2287	rVB	1198393	2255912	51.41%	6.088%
56	8.894	2423	2427	2429	rBV4	1332	1021	0.02%	0.003%
57	8.948	2441	2444	2447	rBV3	1765	1220	0.03%	0.003%
58	9.083	2473	2486	2512	rBV	1857159	3225000	73.50%	8.704%
59	9.508	2617	2618	2624	rVB5	940	721	0.02%	0.002%
60	9.553	2628	2632	2634	rBV2	1984	1557	0.04%	0.004%
61	9.646	2657	2661	2665	rVB6	1223	1077	0.02%	0.003%
62	9.672	2665	2669	2671	rBV3	1293	1080	0.02%	0.003%
63	9.717	2673	2683	2684	rBV9	5558	7952	0.18%	0.021%
64	9.890	2732	2737	2740	rBV6	2118	2396	0.05%	0.006%
65	9.952	2750	2756	2764	rVB10	6570	8675	0.20%	0.023%
66	10.170	2816	2824	2831	rBV10	3113	5692	0.13%	0.015%
67	10.206	2832	2835	2839	rVV4	1335	1200	0.03%	0.003%
68	10.299	2860	2864	2867	rBV4	1019	1003	0.02%	0.003%
69	10.318	2867	2870	2873	rBV5	1368	957	0.02%	0.003%
70	10.373	2880	2887	2892	rBV6	9106	12032	0.27%	0.032%
71	10.427	2892	2904	2935	rVB	1294487	2156468	49.15%	5.820%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051419\
 Data File : VU032007.D
 Acq On : 14 May 2019 20:11
 Operator : JC/SP
 Sample : K2738-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB893

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	10.556	2942	2944	2948	rBV5	1604	1290	0.03%	0.003%
73	10.588	2952	2954	2963	rVB4	5728	6460	0.15%	0.017%
74	10.810	3018	3023	3027	rBV6	1630	1929	0.04%	0.005%
75	10.861	3032	3039	3054	rVB6	3927	7645	0.17%	0.021%
76	10.980	3066	3076	3085	rVV10	8434	15407	0.35%	0.042%
77	11.045	3089	3096	3100	rBV4	2816	3814	0.09%	0.010%
78	11.138	3122	3125	3126	rBV2	1888	1136	0.03%	0.003%
79	11.267	3159	3165	3171	rBV7	6048	8121	0.19%	0.022%
80	11.308	3175	3178	3180	rBV3	1439	995	0.02%	0.003%
81	11.479	3219	3231	3259	rBV	1653259	2692726	61.37%	7.267%
82	11.765	3314	3320	3330	rVB5	13252	20937	0.48%	0.057%
83	11.855	3336	3348	3377	rBV	1719546	2842643	64.78%	7.672%
84	12.292	3475	3484	3495	rVB5	48603	84594	1.93%	0.228%
85	12.492	3537	3546	3557	rVB2	30878	51210	1.17%	0.138%
86	12.755	3626	3628	3631	rBV3	1590	903	0.02%	0.002%
87	12.778	3631	3635	3642	rVV10	3018	3701	0.08%	0.010%
88	12.967	3690	3694	3699	rBV6	2374	2941	0.07%	0.008%
89	13.125	3736	3743	3754	rBV6	5830	10985	0.25%	0.030%
90	13.254	3775	3783	3794	rBV6	12098	19833	0.45%	0.054%
91	13.540	3870	3872	3876	rVB5	2061	1134	0.03%	0.003%
92	13.566	3876	3880	3881	rBV3	1578	1060	0.02%	0.003%
93	13.649	3903	3906	3909	rBV3	1976	1241	0.03%	0.003%
94	13.787	3947	3949	3952	rVB3	2260	1090	0.02%	0.003%
95	13.839	3962	3965	3967	rVB3	1897	885	0.02%	0.002%
96	13.903	3983	3985	3988	rBV3	1330	875	0.02%	0.002%
97	13.939	3993	3996	4002	rVB4	1852	1632	0.04%	0.004%
98	14.012	4015	4019	4021	rBV4	2072	1764	0.04%	0.005%
99	14.672	4222	4224	4226	rBV2	1616	930	0.02%	0.003%
100	14.816	4267	4269	4271	rBV3	1547	915	0.02%	0.002%


Sum of corrected areas: 37052313

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051419\
Data File : VU032007.D
Acq On : 14 May 2019 20:11
Operator : JC/SP
Sample : K2738-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB893

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

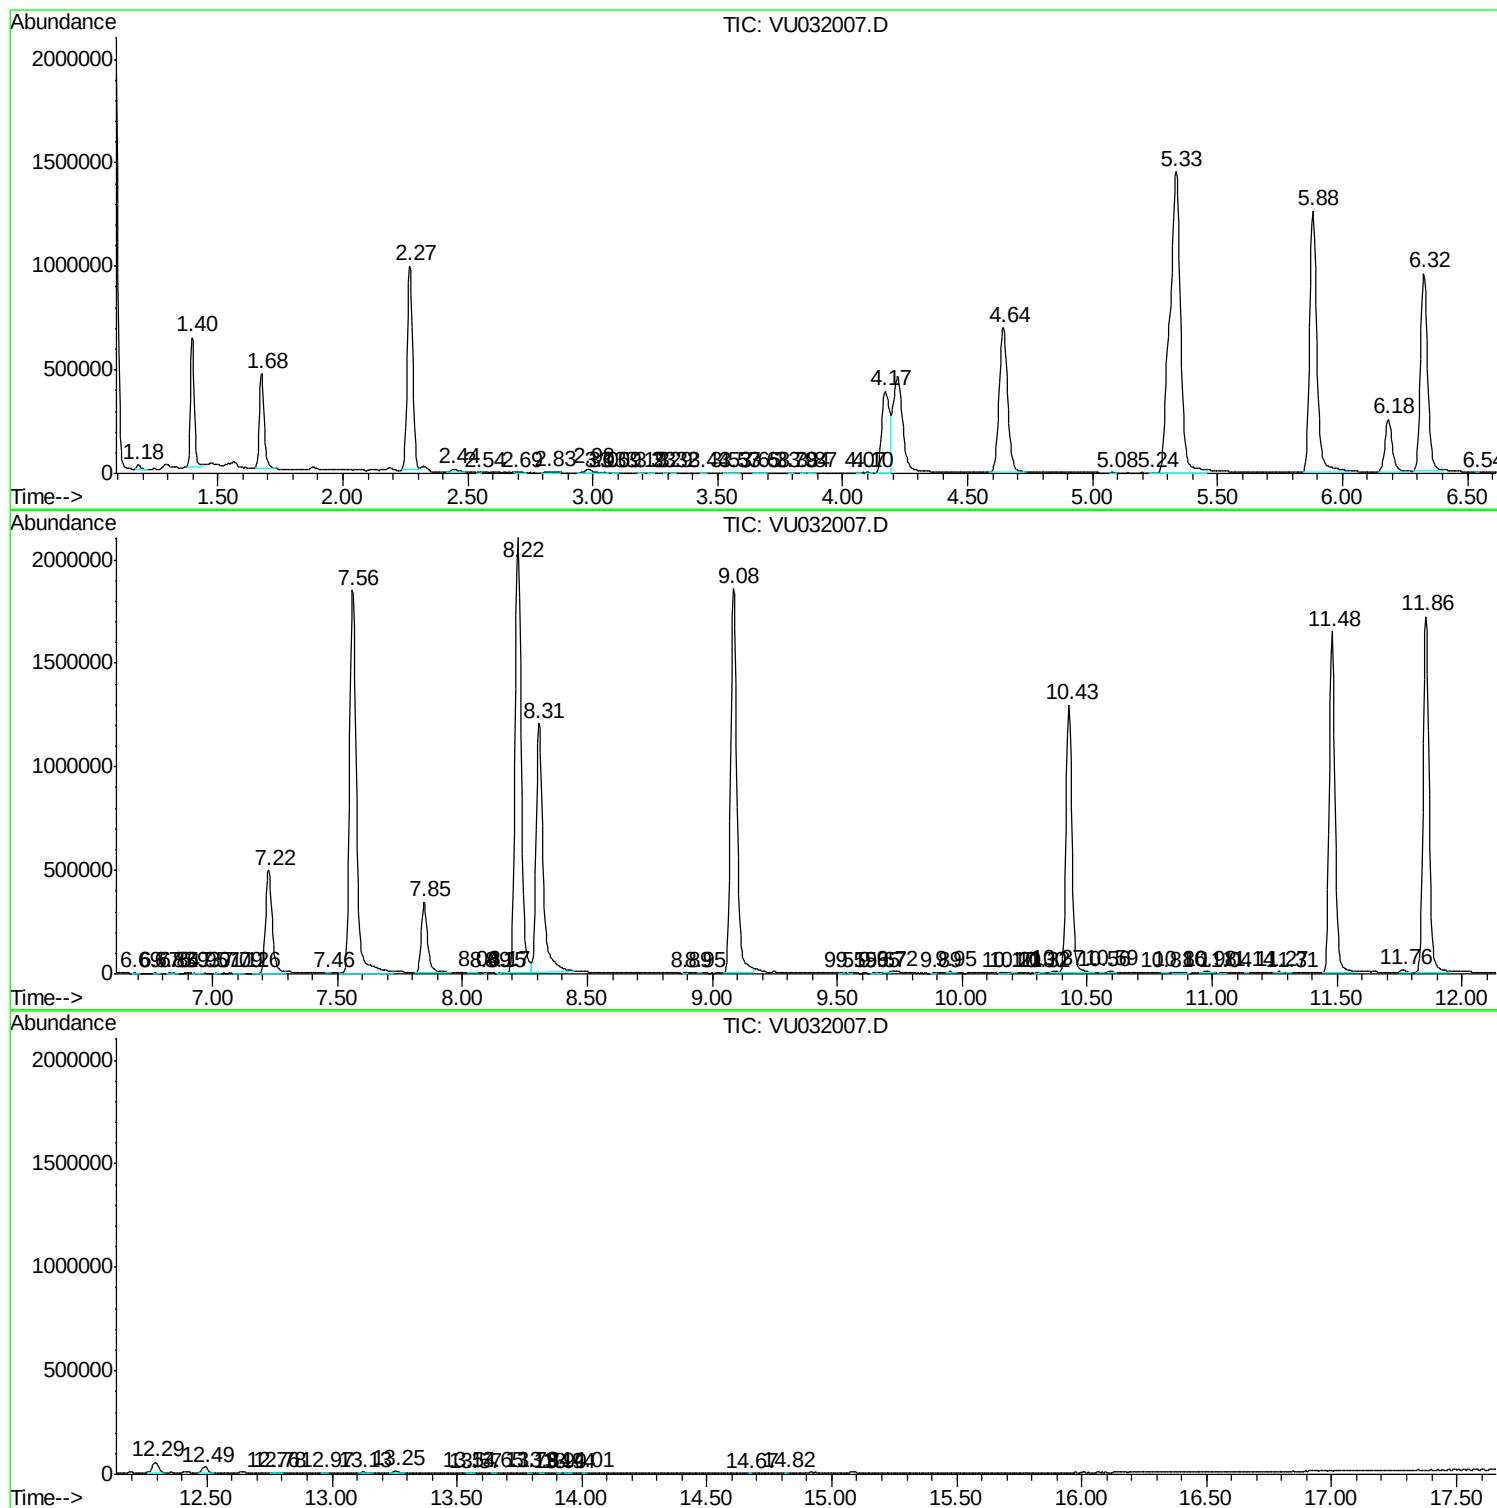

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051419\
Data File : VU032007.D
Acq On : 14 May 2019 20:11
Operator : JC/SP
Sample : K2738-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB893

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051419\
Data File : VU032007.D
Acq On : 14 May 2019 20:11
Operator : JC/SP
Sample : K2738-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB893

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc