


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051419\
 Data File : VU031981.D
 Acq On : 14 May 2019 09:54
 Operator : JC/SP
 Sample : BFB42
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis
 Last Update : Wed May 15 04:26:34 2019

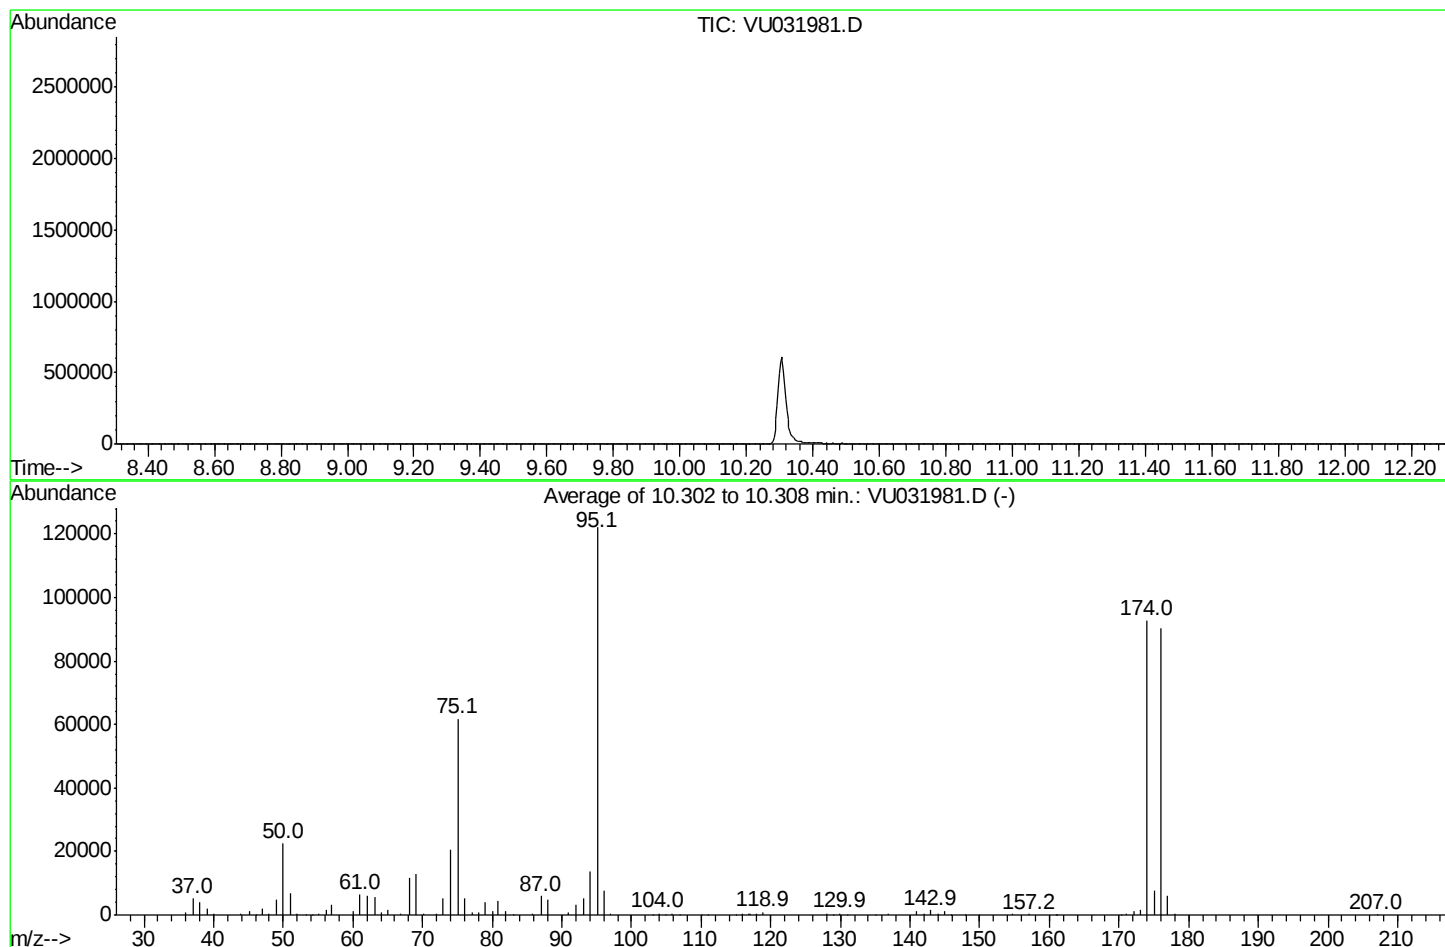

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	22520	PASS
75	95	30	80	50.6	61786	PASS
95	95	100	100	100.0	122093	PASS
96	95	5	9	6.3	7674	PASS
173	174	0.00	2	1.7	1596	PASS
174	95	50	120	75.8	92597	PASS
175	174	5	9	8.1	7533	PASS
176	174	95	101	97.6	90400	PASS
177	176	5	9	6.5	5893	PASS

Scan 2853 (10.263 min): VU031981.D
BFB42

m/z	Abundance
40.00	701.0
43.90	1041.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	869.0
37.00	5372.0
38.00	4014.0
39.10	2147.0
40.00	1055.0
43.90	1313.0
45.10	1161.0
46.10	236.0
47.00	2124.0
48.00	622.0
49.00	4774.0
50.00	22696.0
51.10	6700.0
52.00	447.0
55.00	491.0
56.10	1315.0
57.00	3123.0
60.00	1043.0
61.00	6744.0
62.10	6044.0
63.10	6111.0
64.00	981.0
65.00	1511.0
66.90	348.0
68.00	11803.0
69.10	13120.0
70.10	590.0
72.00	556.0
73.00	5573.0
74.10	20040.0
75.10	62024.0
76.00	5264.0
77.10	907.0
77.90	607.0
79.00	4217.0
80.00	1470.0
80.90	4754.0
81.90	931.0
85.80	187.0
87.00	5874.0
88.00	4826.0
90.90	633.0
92.10	3383.0
93.10	5349.0
94.00	13738.0
95.10	118336.0
96.10	7744.0
96.90	342.0
104.00	395.0
104.80	176.0
105.70	396.0
107.00	227.0
110.90	143.0
114.90	134.0
115.90	489.0
117.10	907.0
118.00	291.0
118.90	791.0
128.00	391.0
129.10	132.0
129.90	556.0
130.90	236.0
135.10	200.0
136.90	254.0
141.00	1112.0
142.00	262.0
143.00	1390.0
143.90	258.0
144.90	1046.0
145.90	130.0
147.80	192.0
149.80	124.0
154.80	207.0
157.20	166.0
160.90	151.0
170.40	179.0
170.90	402.0
172.10	1178.0
173.10	1557.0
174.00	88928.0
175.10	7249.0
176.00	87184.0
177.00	5857.0
178.00	197.0
207.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.10	937.0
37.00	5329.0
38.00	4222.0
39.10	2272.0
39.90	1105.0
43.90	1399.0
45.10	1065.0
46.10	245.0
47.00	2118.0
48.00	551.0
49.10	5136.0
50.00	23368.0
51.10	6972.0
52.00	493.0
53.20	163.0
54.10	175.0
55.00	503.0
56.10	1545.0
57.00	3618.0
60.00	1042.0
61.00	6667.0
62.10	6263.0
63.10	5816.0
64.00	1007.0
65.00	1779.0
66.90	290.0
68.10	11979.0
69.00	13022.0
70.10	584.0
72.10	546.0
73.00	5324.0
74.10	21104.0
75.10	64056.0
76.00	5623.0
77.10	977.0
78.00	692.0
79.00	4231.0
80.00	1284.0
80.90	4546.0
81.90	1178.0
83.10	107.0
85.80	266.0
87.00	6229.0
88.00	5261.0
91.00	672.0
92.10	3562.0
93.10	5736.0
94.00	13992.0
95.10	125712.0
96.10	7953.0
97.00	259.0
103.00	117.0
103.90	433.0
104.90	190.0
105.80	294.0
107.00	172.0
110.00	103.0
110.90	101.0
114.90	164.0
115.90	583.0
117.00	722.0
118.00	347.0
118.90	952.0
128.10	476.0
129.00	105.0
130.00	625.0
130.90	240.0
135.10	137.0
137.00	223.0
141.00	1207.0
142.00	235.0
142.90	1434.0
144.00	236.0
145.00	1097.0
145.90	168.0
147.90	172.0
149.90	204.0
154.70	238.0
157.10	263.0
161.10	117.0
171.00	435.0
172.10	1425.0
173.10	1624.0
174.00	95064.0
175.00	7842.0
176.00	93616.0
177.00	6191.0
178.00	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.10	928.0
37.00	4900.0
38.00	4215.0
39.10	2224.0
40.00	1197.0
44.00	1540.0
45.10	927.0
47.00	1943.0
48.00	500.0
49.10	5124.0
50.00	21496.0
51.10	6627.0
52.00	497.0
53.20	278.0
54.10	202.0
55.00	421.0
56.10	1590.0
57.00	3535.0
60.00	995.0
61.00	5689.0
62.10	5844.0
63.10	4971.0
64.00	936.0
65.10	1948.0
66.90	251.0
68.10	10991.0
69.10	11994.0
70.10	589.0
72.00	602.0
73.00	4834.0
74.10	20144.0
75.10	59280.0
76.00	5170.0
77.10	824.0
78.10	733.0
78.90	3899.0
80.00	1050.0
80.90	3868.0
81.90	1255.0
83.10	142.0
85.90	329.0
87.00	5944.0
88.00	4966.0
91.00	561.0
92.00	3331.0
93.10	5262.0
94.00	13764.0
95.10	122232.0
96.10	7327.0
97.00	197.0
103.00	149.0
104.00	420.0
104.90	208.0
105.90	236.0
115.00	201.0
116.00	534.0
116.80	662.0
118.00	294.0
118.90	910.0
128.10	492.0
128.90	184.0
130.00	579.0
130.90	170.0
137.00	191.0
141.00	1053.0
142.00	175.0
142.90	1485.0
144.00	193.0
145.00	1082.0
146.00	215.0
148.00	193.0
149.90	278.0
154.70	219.0
157.10	254.0
171.10	416.0
172.10	1517.0
173.10	1608.0
174.00	93800.0
175.00	7509.0
176.00	90400.0
177.00	5632.0
178.00	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42