

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051420\
 Data File : VU038177.D
 Acq On : 14 May 2020 18:14
 Operator : JC/MD
 Sample : L2653-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE0

Quant Time: May 15 03:40:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 15 01:05:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	331227	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	324548	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	154062	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	103429	3.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.20%
7) Chloroethane-d5	1.93	69	105664	4.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.60%
11) 1,1-Dichloroethene-d2	2.59	63	140355	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	4.67	46	427775	57.23	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.46%
24) Chloroform-d	5.10	84	210948	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.74	65	126434	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.76	84	433640	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
36) 1,2-Dichloropropane-d6	6.72	67	147049	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.60%
41) Toluene-d8	7.92	98	374251	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.20	79	50999	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	8.65	63	357283	60.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.34%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	127234	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	145140	4.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	15932	3.397 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051420\
Data File : VU038177.D
Acq On : 14 May 2020 18:14
Operator : JC/MD
Sample : L2653-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE0

Quant Time: May 15 03:40:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 15 01:05:40 2020
Response via : Initial Calibration

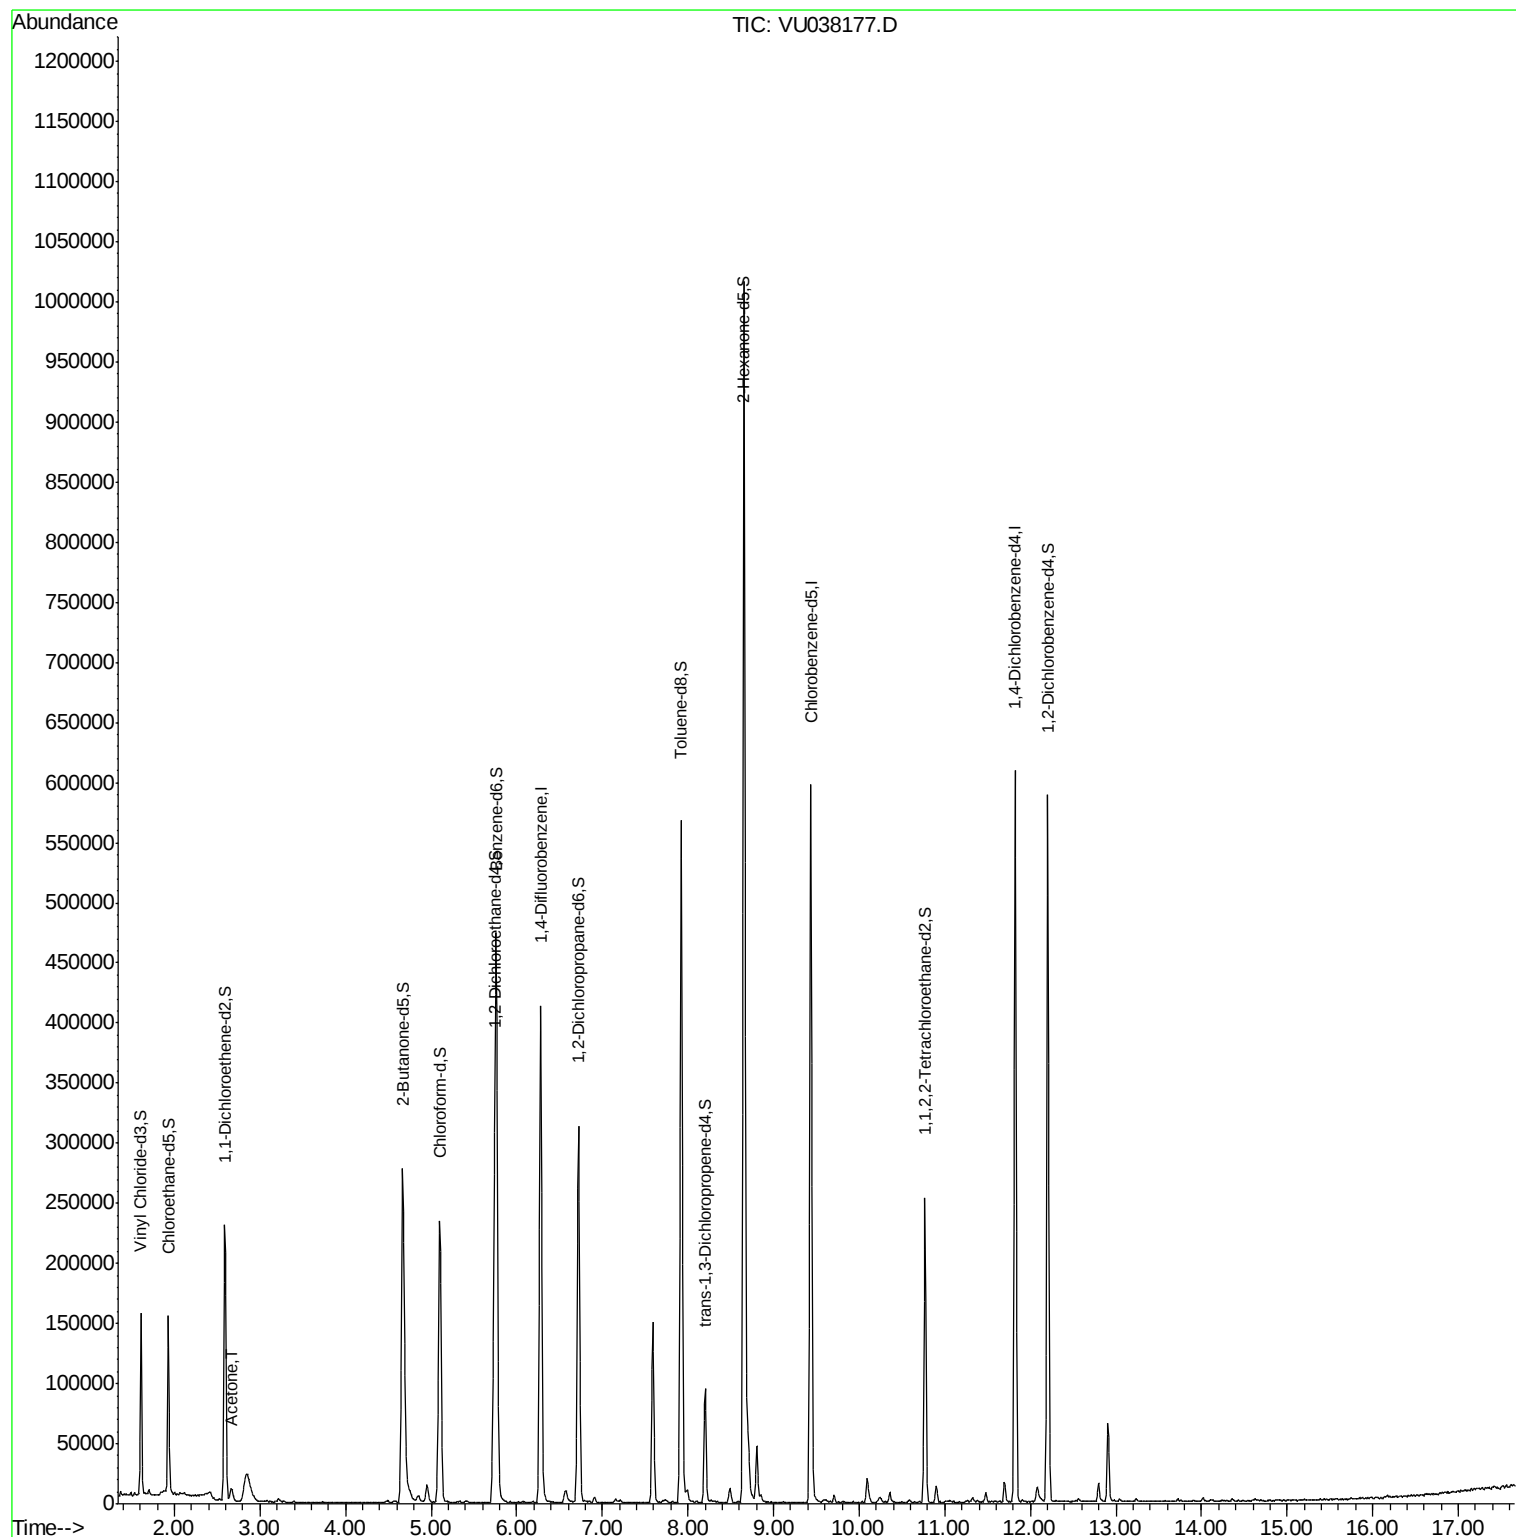

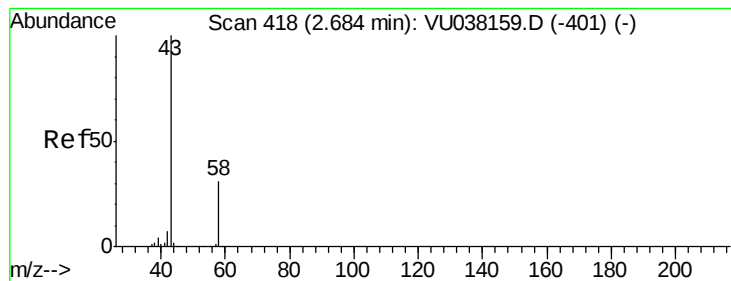

#13

Acetone

Concen: 3.397 ug/L

RT: 2.66 min Scan# 412

Delta R.T. -0.02 min

Lab File: VU038177.D

Acq: 14 May 2020 18:14

Instrument :

MSVOA_U

ClientSampleId :

C0AE0

Tot Ion: 43 Resp: 15932

Ion Ratio Lower Upper

43 100

58 31.9 0.0 63.6

