

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051420\
 Data File : VU038178.D
 Acq On : 14 May 2020 18:37
 Operator : JC/MD
 Sample : L2653-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE1

Quant Time: May 15 03:57:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 15 01:05:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	330713	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	320466	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	150368	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	103400	3.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.40%
7) Chloroethane-d5	1.93	69	103686	3.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.20%
11) 1,1-Dichloroethene-d2	2.59	63	139673	2.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.20%#
20) 2-Butanone-d5	4.67	46	410091	54.95	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.90%
24) Chloroform-d	5.10	84	204656	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.74	65	126047	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.76	84	426223	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.80%
36) 1,2-Dichloropropane-d6	6.72	67	145471	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.92	98	369679	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.20	79	49914	4.02	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.40%
46) 2-Hexanone-d5	8.65	63	341833	58.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.62%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	122686	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	12.20	152	140685	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds				Ovalue
13) Acetone	2.66	43	13767	2.940 ug/L 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051420\
Data File : VU038178.D
Acq On : 14 May 2020 18:37
Operator : JC/MD
Sample : L2653-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE1

Quant Time: May 15 03:57:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 15 01:05:40 2020
Response via : Initial Calibration

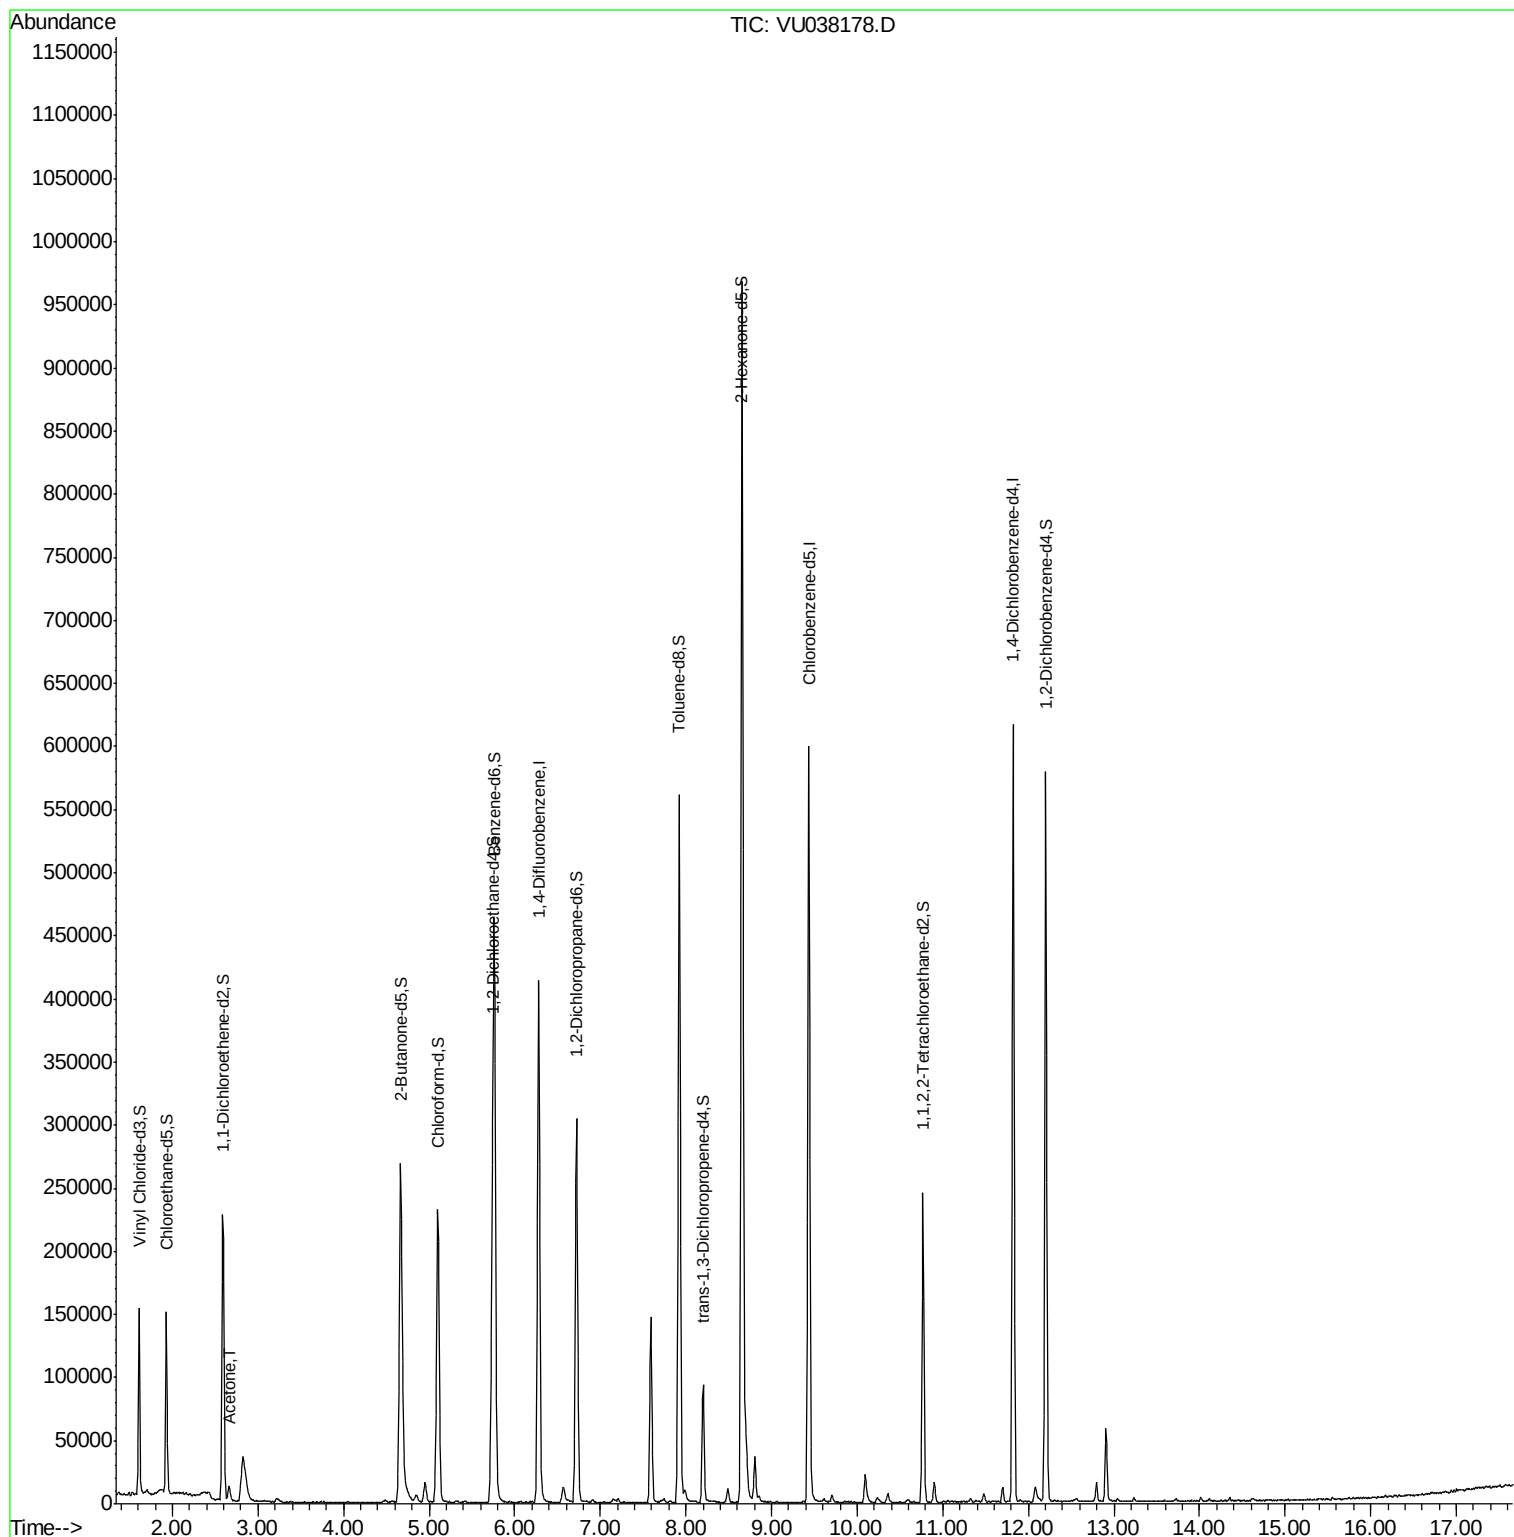

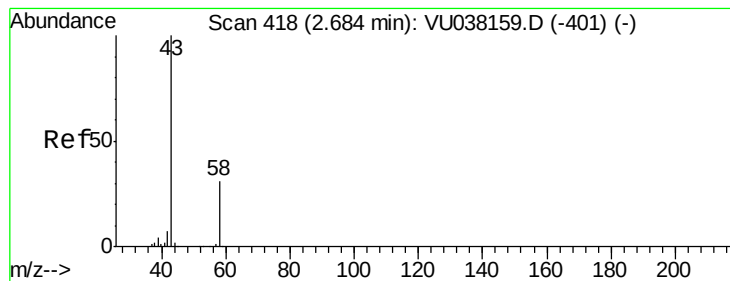

#13
 Acetone
 Concen: 2.940 ug/L
 RT: 2.66 min Scan# 411
 Delta R.T. -0.02 min
 Lab File: VU038178.D
 Acq: 14 May 2020 18:37

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE1

Tot Ion: 43 Resp: 13767
 Ion Ratio Lower Upper
 43 100
 58 36.8 0.0 63.6

