

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051420\
 Data File : VU038181.D
 Acq On : 14 May 2020 19:47
 Operator : JC/MD
 Sample : L2653-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE2

Quant Time: May 15 04:23:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 15 01:05:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	316495	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	309605	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	146591	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	95309	3.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.80%
7) Chloroethane-d5	1.93	69	100777	4.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.40%
11) 1,1-Dichloroethene-d2	2.59	63	134976	2.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.80%#
20) 2-Butanone-d5	4.67	46	427292	59.82	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.64%
24) Chloroform-d	5.10	84	200025	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.74	65	123520	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.76	84	422425	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.72	67	143697	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.92	98	366609	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
43) trans-1,3-Dichloropropene-	8.20	79	48393	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.65	63	351306	62.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	124.04%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	123764	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	140060	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds				Ovalue
13) Acetone	2.66	43	18436	4.114 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051420\
Data File : VU038181.D
Acq On : 14 May 2020 19:47
Operator : JC/MD
Sample : L2653-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE2

Quant Time: May 15 04:23:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 15 01:05:40 2020
Response via : Initial Calibration

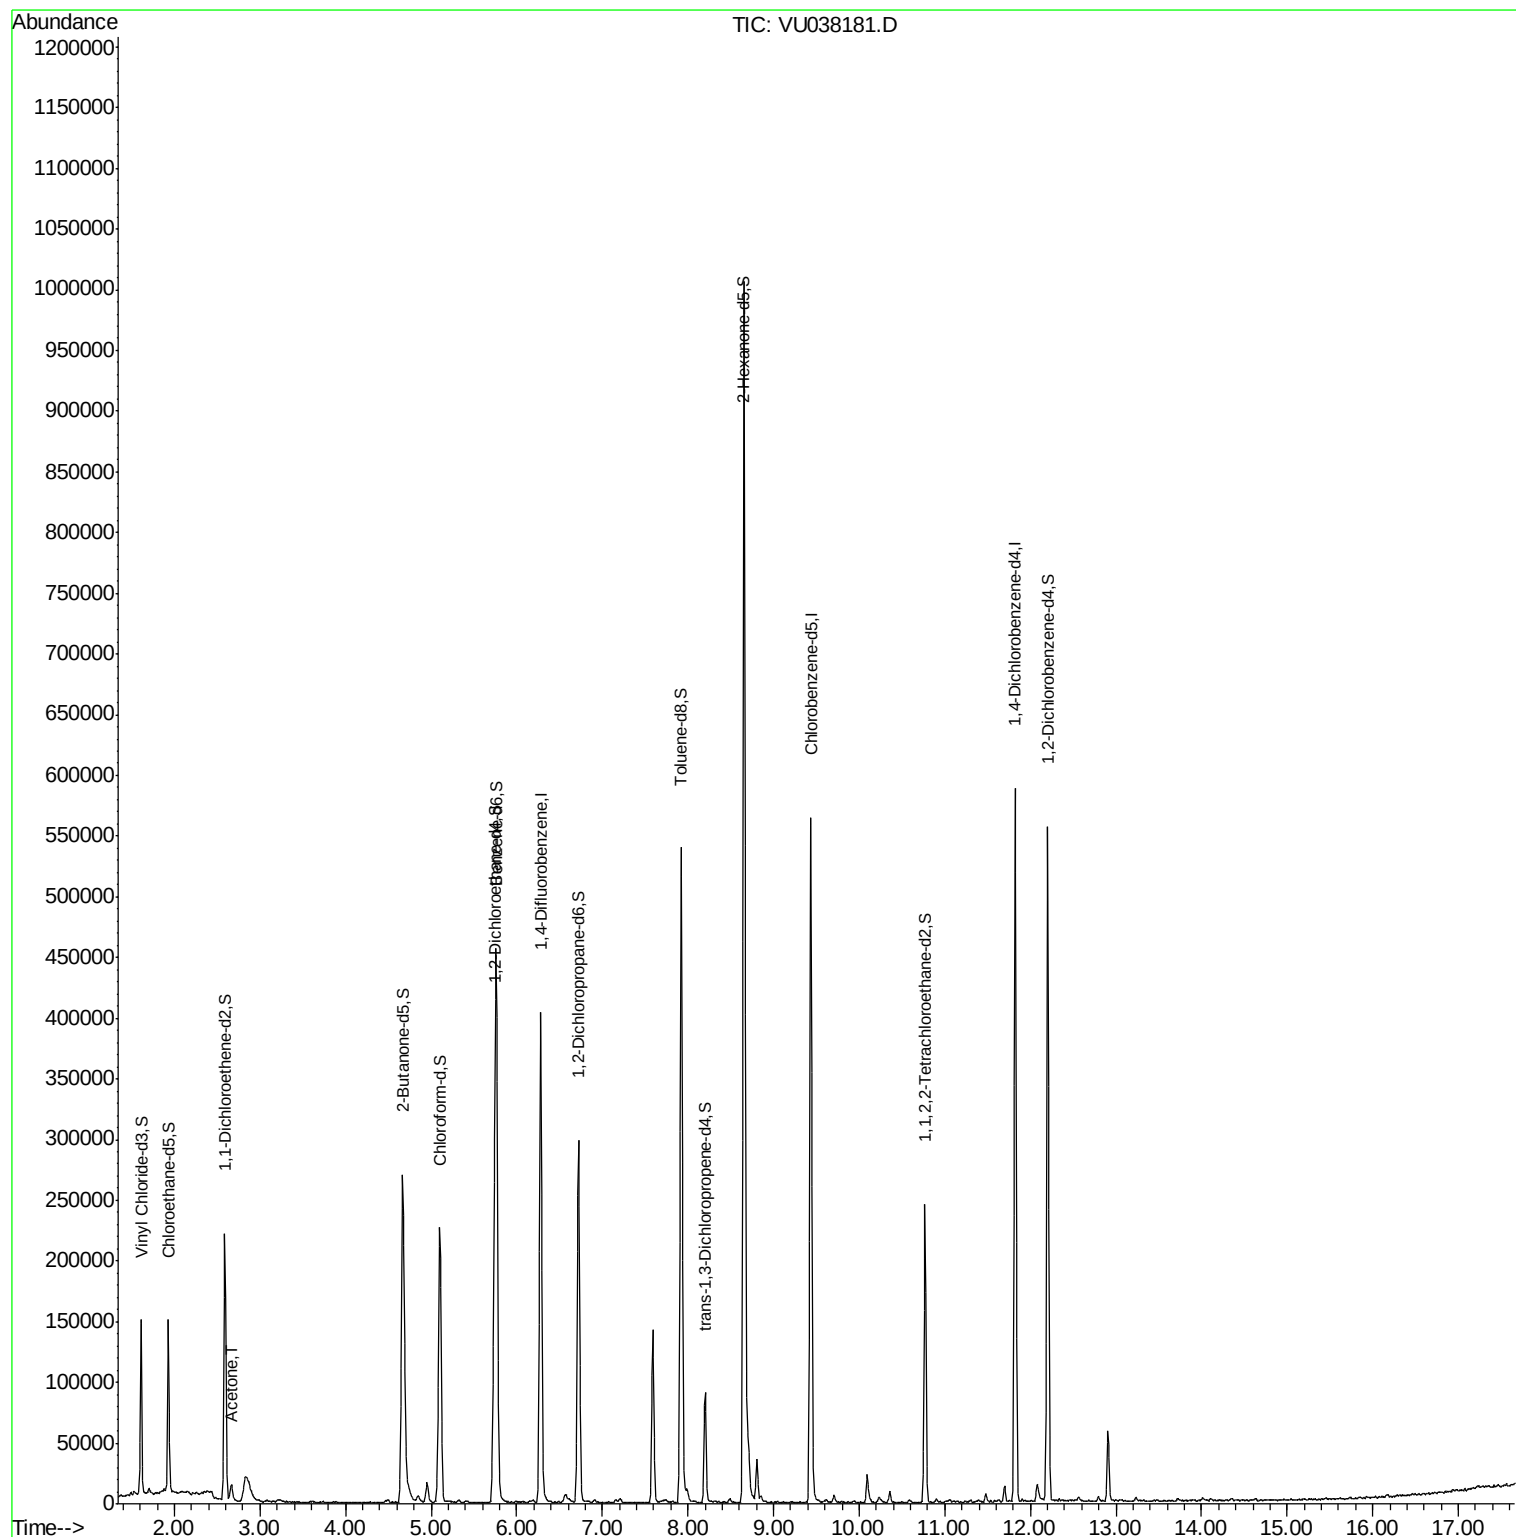

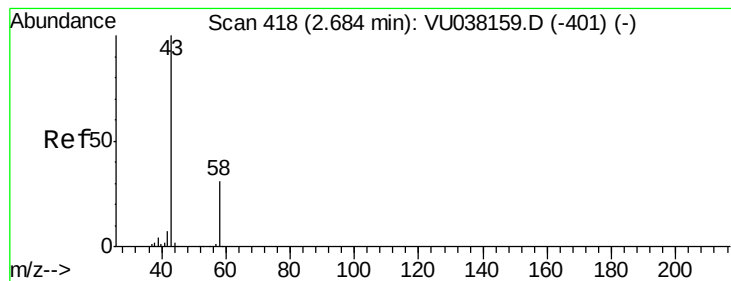

#13
 Acetone
 Concen: 4.114 ug/L
 RT: 2.66 min Scan# 412
 Delta R.T. -0.02 min
 Lab File: VU038181.D
 Acq: 14 May 2020 19:47

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE2

Tot Ion: 43 Resp: 18436
 Ion Ratio Lower Upper
 43 100
 58 31.4 0.0 63.6

