


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051420\
 Data File : VU038158.D
 Acq On : 14 May 2020 10:10
 Operator : JC/MD
 Sample : BFB23
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB23

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri May 15 04:24:22 2020

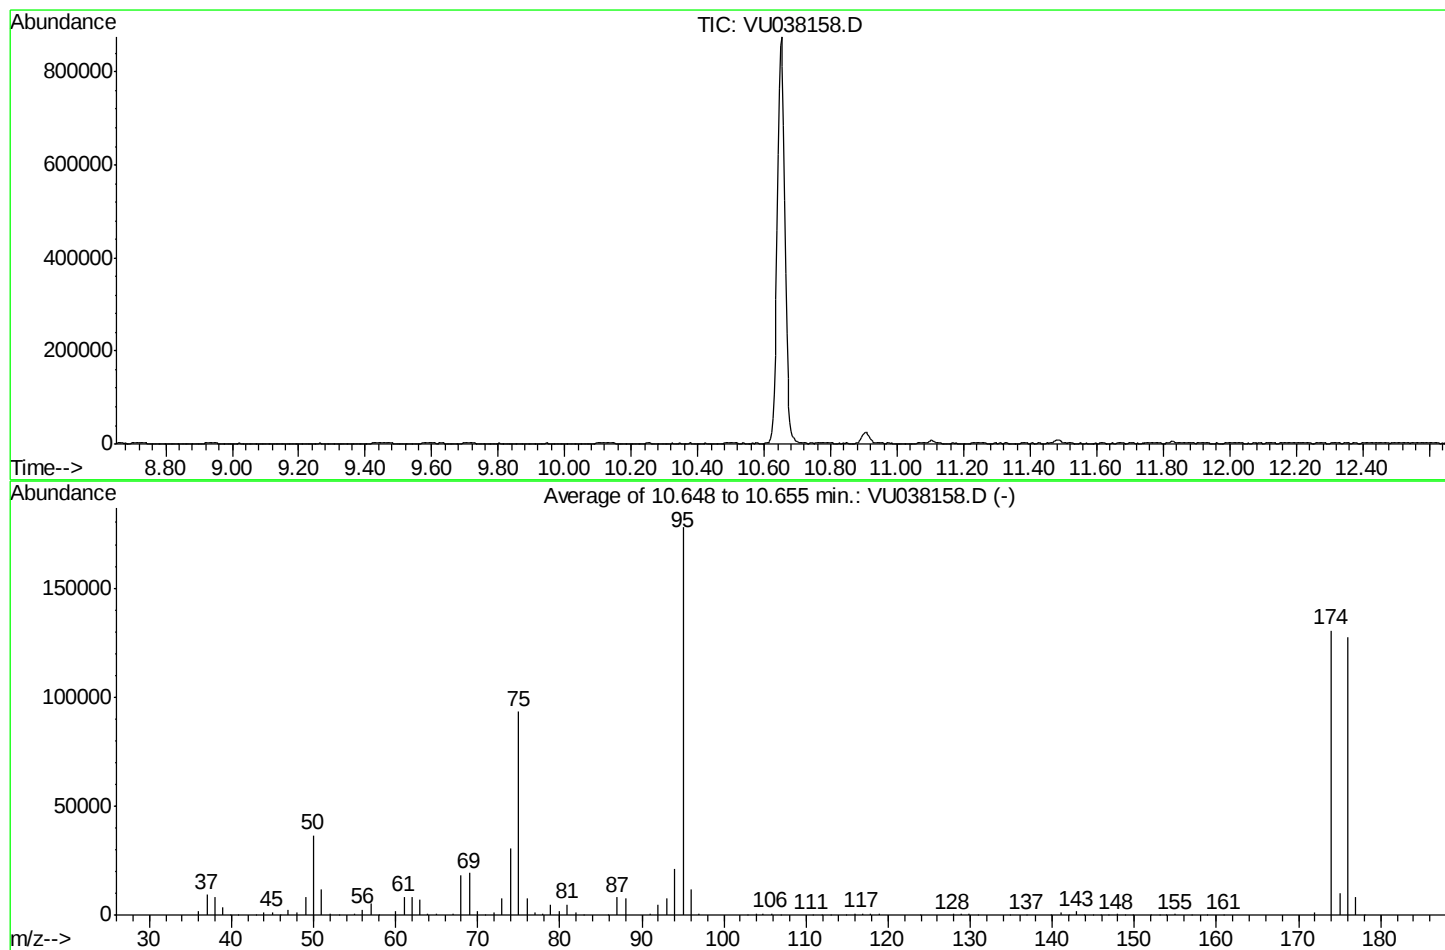

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	36512	PASS
75	95	30	80	52.5	93338	PASS
95	95	100	100	100.0	177834	PASS
96	95	5	9	6.6	11759	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.4	130616	PASS
175	174	5	9	7.7	10027	PASS
176	174	95	101	97.4	127280	PASS
177	176	5	9	6.3	8075	PASS

m/z	Abundance
36.00	1698.0
37.00	9602.0
38.00	8794.0
39.00	3940.0
39.90	485.0
40.80	105.0
42.90	135.0
43.90	2157.0
45.00	1415.0
46.00	264.0
46.90	2640.0
48.00	944.0
49.00	8418.0
50.00	38064.0
51.00	12258.0
52.10	480.0
55.00	511.0
56.00	2771.0
57.00	5248.0
58.00	186.0
60.00	1476.0
61.00	8469.0
62.00	8381.0
63.00	7029.0
63.90	882.0
65.00	742.0
66.90	655.0
68.00	19296.0
69.00	19864.0
70.00	1683.0
70.90	139.0
72.00	1165.0
73.00	8012.0
74.00	31160.0
75.00	95472.0
76.00	8130.0
76.90	1052.0
77.90	834.0
78.90	5214.0
80.00	1545.0
81.00	4866.0
81.90	1121.0
82.80	152.0
85.80	189.0
87.00	8105.0
88.00	7539.0
90.90	620.0
92.00	4663.0
93.00	7552.0
94.00	21424.0
95.00	180096.0
96.00	11962.0
97.00	348.0
103.90	673.0
104.80	400.0
105.80	791.0
106.90	249.0
110.80	172.0
111.90	126.0
113.00	138.0
115.90	721.0
116.90	890.0
117.90	576.0
118.90	751.0
127.90	468.0
128.90	365.0
129.90	401.0
130.90	234.0
134.90	161.0
136.90	307.0
139.80	111.0
141.00	1276.0
142.00	169.0
143.00	1726.0
143.90	146.0
145.00	196.0
145.90	223.0
146.90	116.0
147.90	451.0
148.80	112.0
153.00	157.0
153.80	129.0
154.90	342.0
156.90	273.0
160.90	164.0
172.00	951.0
174.00	129368.0
175.00	9797.0
176.00	126400.0
177.00	7747.0
178.00	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	1696.0
37.00	9605.0
38.00	8537.0
39.00	3764.0
39.90	487.0
42.90	129.0
44.00	2077.0
45.00	1503.0
46.00	212.0
47.00	2482.0
47.90	1077.0
49.00	8270.0
50.00	37512.0
51.00	12328.0
52.10	438.0
53.10	105.0
55.00	532.0
56.00	2752.0
57.00	5396.0
57.90	205.0
60.00	1671.0
61.00	8599.0
62.00	8703.0
63.00	7188.0
63.90	899.0
65.00	694.0
67.00	581.0
68.00	19016.0
69.00	20080.0
70.00	1543.0
70.90	115.0
72.00	1203.0
73.00	7959.0
74.00	31768.0
75.00	96400.0
76.00	8039.0
77.00	945.0
77.90	924.0
78.90	5202.0
80.00	1572.0
80.90	4944.0
81.90	1064.0
82.90	155.0
87.00	8381.0
88.00	7837.0
90.90	604.0
92.00	4790.0
93.00	7775.0
94.00	21848.0
95.00	183488.0
96.00	12094.0
97.00	396.0
103.90	748.0
104.80	338.0
105.80	786.0
106.90	267.0
110.80	228.0
111.90	136.0
113.00	111.0
114.90	140.0
115.90	744.0
116.90	930.0
117.90	570.0
118.90	786.0
123.90	124.0
127.90	560.0
128.90	393.0
129.90	446.0
130.90	269.0
134.90	217.0
136.90	275.0
139.80	145.0
141.00	1313.0
142.00	137.0
143.00	1709.0
143.90	168.0
145.00	196.0
146.00	186.0
147.90	487.0
148.80	148.0
149.80	109.0
151.90	156.0
153.00	119.0
153.90	118.0
155.00	328.0
156.90	292.0
160.90	164.0
172.00	947.0
174.00	134656.0
175.00	10382.0
176.00	131264.0
177.00	8406.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

178.00

171.0

Instrument :

MSVOA_U

ClientSampleId :

BFB23

m/z	Abundance
36.00	1563.0
37.00	8316.0
38.00	7777.0
39.00	3231.0
39.90	469.0
43.00	140.0
44.00	2014.0
45.00	1440.0
46.00	175.0
47.00	2281.0
48.00	1116.0
49.00	7322.0
50.00	33960.0
51.00	11182.0
52.00	424.0
55.00	514.0
56.00	2402.0
57.00	4774.0
57.90	191.0
60.00	1717.0
61.00	8205.0
62.00	8070.0
63.00	6451.0
63.90	793.0
65.00	532.0
67.00	487.0
68.00	17040.0
69.00	17912.0
70.00	1336.0
72.00	1030.0
73.00	7238.0
74.00	29544.0
75.00	88144.0
76.00	7511.0
77.00	820.0
77.90	785.0
78.90	4604.0
79.90	1415.0
80.90	4570.0
82.00	984.0
83.00	177.0
87.00	7502.0
88.00	7490.0
91.00	600.0
92.00	4532.0
93.00	7257.0
94.00	20560.0
95.00	169920.0
96.00	11221.0
97.00	360.0
102.80	117.0
103.90	700.0
104.90	223.0
105.80	623.0
106.90	212.0
110.80	194.0
112.90	107.0
114.90	151.0
115.90	647.0
116.90	859.0
117.90	527.0
119.00	778.0
123.90	141.0
127.90	608.0
128.90	293.0
129.90	455.0
130.90	253.0
134.90	235.0
136.90	221.0
139.80	170.0
141.00	1252.0
143.00	1474.0
143.90	161.0
145.00	160.0
145.90	168.0
147.90	440.0
148.80	149.0
151.90	180.0
153.90	105.0
155.00	303.0
156.90	294.0
158.80	111.0
160.90	174.0
172.00	829.0
174.00	127824.0
175.00	9903.0
176.00	124176.0
177.00	8072.0
178.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Scan 2880 (10.600 min): VU038158.D
BFB23

m/z	Abundance
39.90	257.0
44.00	1114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23