

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043722.D
 Acq On : 14 May 2021 00:48
 Operator : SY/MD
 Sample : M2316-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

Signal : TIC: VU043722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rBV	246039	275010	15.42%	2.104%
2	1.912	170	178	192	rVB	172492	222833	12.50%	1.705%
3	2.571	370	383	400	rBV	381623	629589	35.31%	4.816%
4	2.793	440	452	453	rBV6	1862	2648	0.15%	0.020%
5	2.944	495	499	500	rBV3	535	357	0.02%	0.003%
6	2.996	511	515	517	rBV	326	219	0.01%	0.002%
7	3.015	519	521	523	rVV3	403	234	0.01%	0.002%
8	3.051	523	532	545	rVV2	6162	11341	0.64%	0.087%
9	3.112	549	551	558	rVV3	320	351	0.02%	0.003%
10	3.144	558	561	563	rVV2	318	199	0.01%	0.002%
11	3.192	563	576	595	rVB2	11413	27532	1.54%	0.211%
12	3.314	611	614	618	rVV2	256	175	0.01%	0.001%
13	3.350	622	625	627	rBV2	517	373	0.02%	0.003%
14	3.362	627	629	634	rVB4	612	385	0.02%	0.003%
15	3.388	634	637	642	rVB3	329	287	0.02%	0.002%
16	3.424	642	648	650	rBV	412	347	0.02%	0.003%
17	3.658	719	721	729	rVB3	314	319	0.02%	0.002%
18	3.948	807	811	814	rBV2	415	304	0.02%	0.002%
19	4.131	863	868	871	rBV2	312	212	0.01%	0.002%
20	4.240	898	902	905	rBV	232	205	0.01%	0.002%
21	4.282	909	915	917	rBV2	263	256	0.01%	0.002%
22	4.407	948	954	960	rBV2	193	240	0.01%	0.002%
23	4.629	1008	1023	1058	rBV	197994	482574	27.06%	3.692%
24	4.854	1090	1093	1097	rBV2	325	268	0.02%	0.002%
25	4.983	1129	1133	1137	rVB3	299	271	0.02%	0.002%
26	5.073	1143	1161	1184	rBV	307808	673614	37.77%	5.153%
27	5.256	1214	1218	1221	rBV2	515	343	0.02%	0.003%
28	5.301	1221	1232	1239	rBV2	770	1683	0.09%	0.013%
29	5.391	1249	1260	1264	rBV2	773	1190	0.07%	0.009%
30	5.616	1327	1330	1334	rBV2	281	243	0.01%	0.002%
31	5.732	1343	1366	1390	rBV2	668085	1783241	100.00%	13.642%
32	5.877	1409	1411	1415	rVB2	408	240	0.01%	0.002%
33	5.964	1435	1438	1440	rBV2	268	179	0.01%	0.001%
34	5.980	1441	1443	1448	rVB4	452	279	0.02%	0.002%
35	6.050	1463	1465	1470	rVB3	536	366	0.02%	0.003%
36	6.115	1482	1485	1487	rBV2	409	279	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043722.D
 Acq On : 14 May 2021 00:48
 Operator : SY/MD
 Sample : M2316-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	6.256	1514	1529	1553	rBV	489643	920153	51.60%	7.039%
38	6.366	1559	1563	1565	rBV2	431	364	0.02%	0.003%
39	6.536	1608	1616	1625	rBV6	3848	6910	0.39%	0.053%
40	6.591	1629	1633	1636	rBV4	339	213	0.01%	0.002%
41	6.629	1644	1645	1651	rVB	297	195	0.01%	0.001%
42	6.700	1651	1667	1689	rBV	410907	800008	44.86%	6.120%
43	6.793	1693	1696	1698	rBV3	378	309	0.02%	0.002%
44	6.864	1713	1718	1723	rVB5	418	418	0.02%	0.003%
45	6.890	1723	1726	1729	rBV	326	195	0.01%	0.001%
46	7.005	1756	1762	1766	rBV3	258	232	0.01%	0.002%
47	7.054	1766	1777	1783	rVB2	804	1184	0.07%	0.009%
48	7.182	1812	1817	1825	rVB4	1020	1234	0.07%	0.009%
49	7.372	1869	1876	1879	rBV2	226	218	0.01%	0.002%
50	7.517	1916	1921	1925	rBV2	709	814	0.05%	0.006%
51	7.571	1925	1938	1957	rVV	215829	376560	21.12%	2.881%
52	7.690	1970	1975	1984	rVB5	807	1170	0.07%	0.009%
53	7.796	1999	2008	2011	rBV5	1717	2149	0.12%	0.016%
54	7.906	2025	2042	2056	rBV	795018	1368185	76.72%	10.466%
55	8.185	2117	2129	2146	rBV	149062	248749	13.95%	1.903%
56	8.472	2211	2218	2219	rBV	814	681	0.04%	0.005%
57	8.558	2237	2245	2249	rBV5	690	975	0.05%	0.007%
58	8.639	2255	2270	2303	rBV	557472	985880	55.29%	7.542%
59	8.816	2323	2325	2331	rVB2	426	280	0.02%	0.002%
60	8.886	2344	2347	2349	rBV2	420	256	0.01%	0.002%
61	8.918	2349	2357	2366	rVV3	2693	4292	0.24%	0.033%
62	9.012	2383	2386	2389	rBV2	252	218	0.01%	0.002%
63	9.423	2500	2514	2539	rBV	684038	1114437	62.50%	8.525%
64	9.574	2555	2561	2569	rBV2	851	1220	0.07%	0.009%
65	9.648	2580	2584	2588	rBV2	236	233	0.01%	0.002%
66	9.700	2592	2600	2609	rVB3	1326	2049	0.11%	0.016%
67	9.812	2631	2635	2637	rBV	247	206	0.01%	0.002%
68	10.002	2690	2694	2698	rVB2	229	201	0.01%	0.002%
69	10.037	2702	2705	2707	rBV2	246	180	0.01%	0.001%
70	10.111	2721	2728	2731	rBV5	682	787	0.04%	0.006%
71	10.494	2840	2847	2852	rVB3	502	706	0.04%	0.005%
72	10.677	2896	2904	2912	rVV3	3571	5437	0.30%	0.042%
73	10.764	2918	2931	2949	rBV	550271	894661	50.17%	6.844%
74	10.832	2949	2952	2954	rBV	413	238	0.01%	0.002%
75	10.873	2962	2965	2967	rBV2	529	362	0.02%	0.003%
76	11.008	3002	3007	3009	rBV2	332	337	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043722.D
 Acq On : 14 May 2021 00:48
 Operator : SY/MD
 Sample : M2316-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	11.095	3031	3034	3037	rBV3	384	332	0.02%	0.003%
78	11.124	3041	3043	3046	rVB3	533	244	0.01%	0.002%
79	11.205	3063	3068	3070	rBV2	242	223	0.01%	0.002%
80	11.307	3096	3100	3107	rBV3	398	433	0.02%	0.003%
81	11.375	3118	3121	3127	rBV2	456	444	0.02%	0.003%
82	11.465	3137	3149	3158	rBV6	3062	5144	0.29%	0.039%
83	11.590	3181	3188	3194	rBV2	471	624	0.03%	0.005%
84	11.700	3215	3222	3229	rBV4	1739	2245	0.13%	0.017%
85	11.751	3233	3238	3246	rBV3	1020	1317	0.07%	0.010%
86	11.819	3246	3259	3280	rBV	629953	995576	55.83%	7.616%
87	11.925	3289	3292	3294	rBV2	470	357	0.02%	0.003%
88	11.951	3296	3300	3303	rBV4	781	879	0.05%	0.007%
89	12.150	3357	3362	3363	rBV2	486	394	0.02%	0.003%
90	12.198	3363	3377	3397	rVV	743324	1184232	66.41%	9.059%
91	12.336	3416	3420	3428	rVB5	1067	1218	0.07%	0.009%
92	12.497	3467	3470	3474	rBV2	361	381	0.02%	0.003%
93	12.529	3478	3480	3484	rVV	290	207	0.01%	0.002%
94	13.227	3691	3697	3706	rVB4	1724	1986	0.11%	0.015%
95	13.291	3714	3717	3721	rVB2	408	313	0.02%	0.002%
96	13.478	3773	3775	3778	rBV2	365	268	0.02%	0.002%
97	13.536	3790	3793	3795	rBV2	406	279	0.02%	0.002%
98	13.851	3884	3891	3902	rVB6	2285	3648	0.20%	0.028%
99	14.092	3960	3966	3976	rBV	3923	6046	0.34%	0.046%
100	14.336	4034	4042	4054	rBV6	2690	4303	0.24%	0.033%




Sum of corrected areas: 13072175

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043722.D
Acq On : 14 May 2021 00:48
Operator : SY/MD
Sample : M2316-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

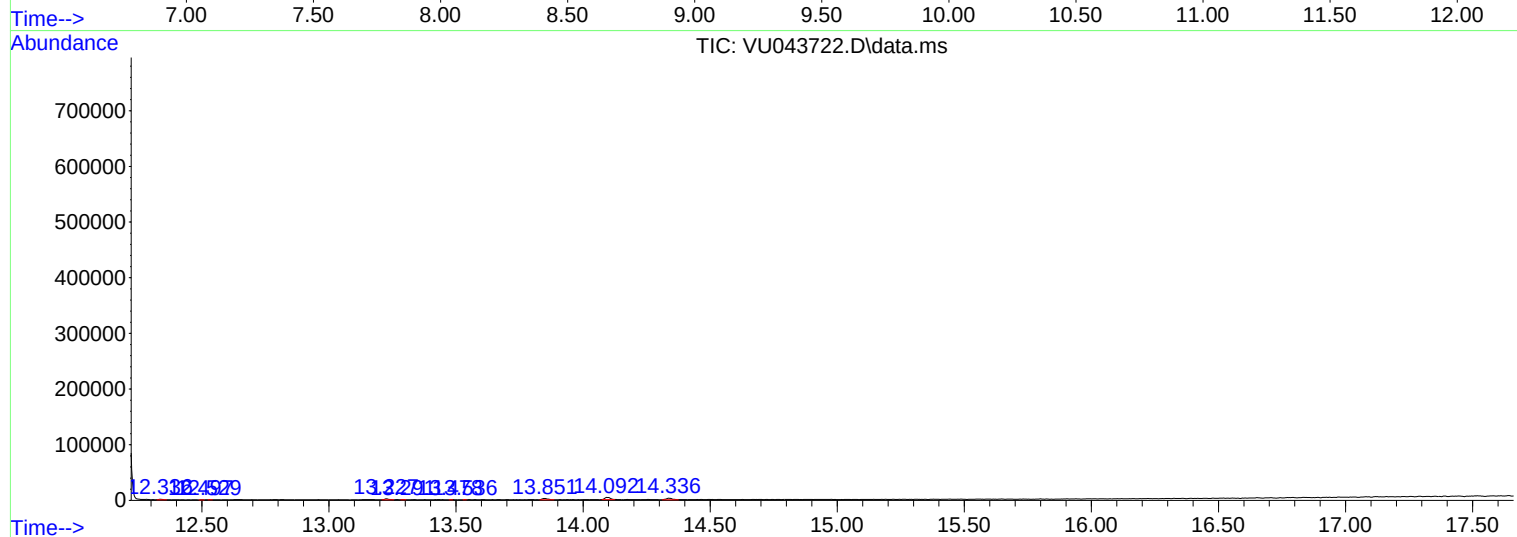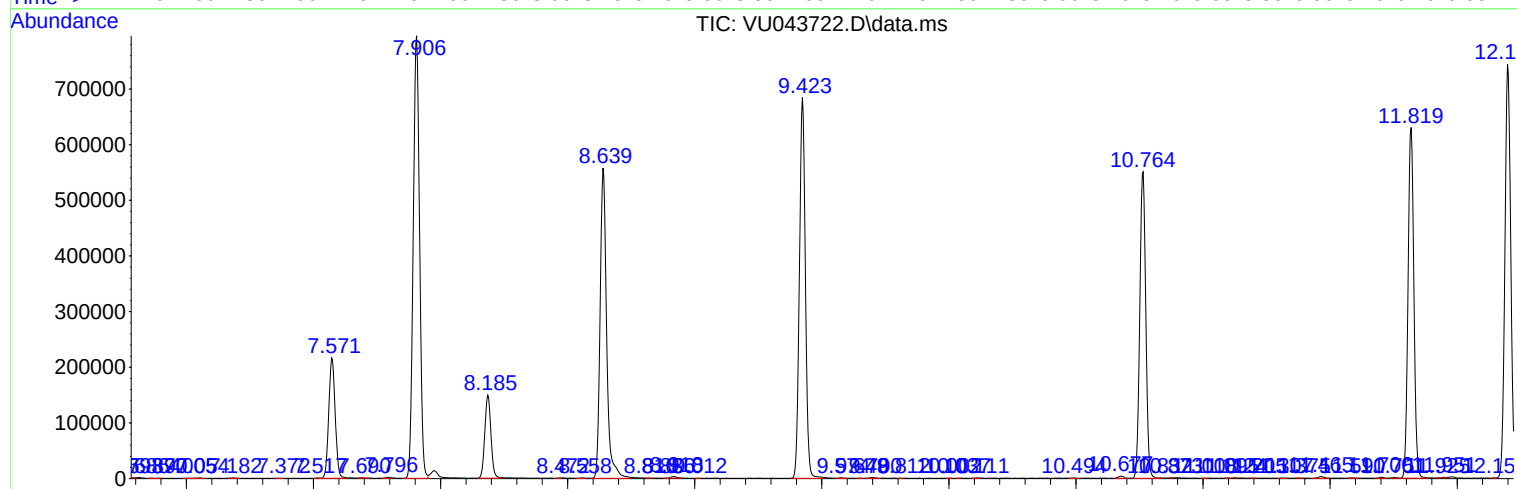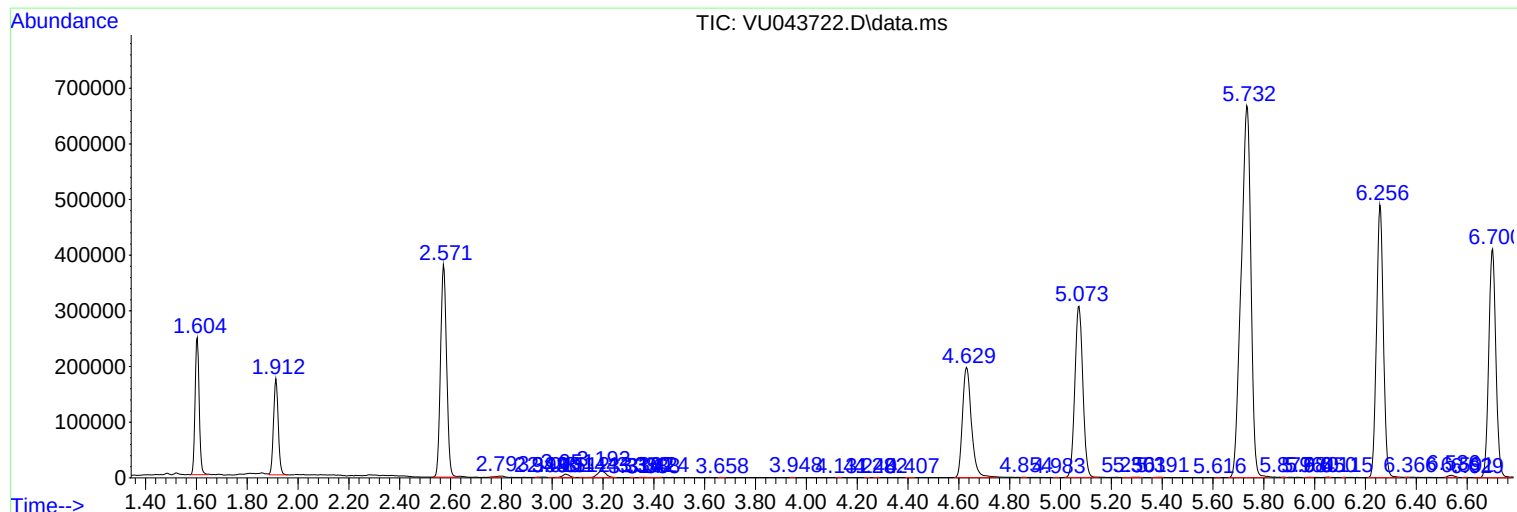

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043722.D
Acq On : 14 May 2021 00:48
Operator : SY/MD
Sample : M2316-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043722.D
Acq On : 14 May 2021 00:48
Operator : SY/MD
Sample : M2316-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------