

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043725.D
 Acq On : 14 May 2021 01:57
 Operator : SY/MD
 Sample : M2327-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

Signal : TIC: VU043725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rVB	260091	291965	15.40%	2.143%
2	1.913	169	178	195	rVB	181782	238866	12.60%	1.754%
3	2.572	370	383	399	rBV	405179	659398	34.79%	4.841%
4	2.691	417	420	423	rVB3	343	219	0.01%	0.002%
5	2.755	435	440	441	rBV3	873	713	0.04%	0.005%
6	2.842	463	467	469	rBV2	236	225	0.01%	0.002%
7	2.867	472	475	479	rBV3	231	189	0.01%	0.001%
8	2.922	488	492	494	rBV2	301	229	0.01%	0.002%
9	2.941	494	498	501	rBV3	342	317	0.02%	0.002%
10	2.999	514	516	522	rBV2	225	247	0.01%	0.002%
11	3.051	522	532	547	rVB4	6378	11827	0.62%	0.087%
12	3.192	562	576	593	rVB	12434	28943	1.53%	0.212%
13	3.282	598	604	609	rBV2	258	251	0.01%	0.002%
14	3.465	655	661	666	rBV3	325	378	0.02%	0.003%
15	3.578	692	696	699	rVB	281	204	0.01%	0.001%
16	3.613	704	707	711	rVB2	286	185	0.01%	0.001%
17	3.671	722	725	730	rVB2	244	187	0.01%	0.001%
18	3.758	746	752	757	rBV	226	289	0.02%	0.002%
19	3.838	770	777	779	rBV	242	218	0.01%	0.002%
20	3.896	792	795	798	rBV2	292	264	0.01%	0.002%
21	3.970	813	818	823	rVB3	279	320	0.02%	0.002%
22	4.006	823	829	831	rBV	184	190	0.01%	0.001%
23	4.626	1006	1022	1062	rVV	212298	511133	26.97%	3.752%
24	4.774	1066	1068	1072	rVB	456	297	0.02%	0.002%
25	5.070	1143	1160	1187	rVB	329733	718763	37.92%	5.277%
26	5.182	1194	1195	1198	rVV3	377	183	0.01%	0.001%
27	5.221	1205	1207	1212	rVB2	442	329	0.02%	0.002%
28	5.285	1220	1227	1228	rBV2	771	729	0.04%	0.005%
29	5.375	1247	1255	1257	rBV3	605	655	0.03%	0.005%
30	5.427	1268	1271	1275	rBV3	219	216	0.01%	0.002%
31	5.732	1342	1366	1395	rBV2	713360	1895301	100.00%	13.914%
32	5.916	1421	1423	1428	rVB3	394	230	0.01%	0.002%
33	6.115	1482	1485	1487	rBV	249	188	0.01%	0.001%
34	6.256	1514	1529	1558	rBV	483748	909494	47.99%	6.677%
35	6.536	1607	1616	1626	rVB5	3461	6664	0.35%	0.049%
36	6.597	1631	1635	1638	rBV2	255	251	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043725.D
 Acq On : 14 May 2021 01:57
 Operator : SY/MD
 Sample : M2327-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	6.697	1651	1666	1686	rBV	438358	851487	44.93%	6.251%
38	6.806	1696	1700	1703	rBV4	934	877	0.05%	0.006%
39	6.887	1722	1725	1732	rVB5	363	400	0.02%	0.003%
40	7.047	1768	1775	1783	rVB3	927	1401	0.07%	0.010%
41	7.157	1802	1809	1811	rBV3	235	241	0.01%	0.002%
42	7.189	1813	1819	1822	rVV4	471	611	0.03%	0.004%
43	7.356	1867	1871	1874	rBV2	206	187	0.01%	0.001%
44	7.507	1915	1918	1921	rBV2	253	185	0.01%	0.001%
45	7.571	1921	1938	1960	rBV	226166	394284	20.80%	2.895%
46	7.719	1981	1984	1987	rVB4	322	231	0.01%	0.002%
47	7.797	2001	2008	2014	rVB3	1033	1505	0.08%	0.011%
48	7.906	2023	2042	2056	rBV	855199	1462178	77.15%	10.734%
49	8.076	2093	2095	2099	rVB2	583	340	0.02%	0.002%
50	8.186	2117	2129	2148	rBV	157525	263905	13.92%	1.937%
51	8.346	2175	2179	2181	rBV	282	194	0.01%	0.001%
52	8.433	2201	2206	2208	rBV2	193	200	0.01%	0.001%
53	8.472	2212	2218	2220	rBV3	447	508	0.03%	0.004%
54	8.559	2243	2245	2247	rVB	433	185	0.01%	0.001%
55	8.639	2256	2270	2303	rBV	584547	1045096	55.14%	7.672%
56	8.919	2349	2357	2358	rBV3	1777	1839	0.10%	0.014%
57	9.002	2379	2383	2391	rBV	268	285	0.02%	0.002%
58	9.041	2391	2395	2398	rBV	242	182	0.01%	0.001%
59	9.343	2487	2489	2493	rVB	267	188	0.01%	0.001%
60	9.423	2497	2514	2544	rBV	674953	1105425	58.32%	8.115%
61	9.581	2556	2563	2568	rBV	641	678	0.04%	0.005%
62	9.694	2592	2598	2599	rBV2	1339	1102	0.06%	0.008%
63	9.800	2627	2631	2633	rBV2	322	253	0.01%	0.002%
64	9.816	2633	2636	2640	rVB3	289	241	0.01%	0.002%
65	10.067	2708	2714	2718	rBV2	240	288	0.02%	0.002%
66	10.105	2722	2726	2731	rBV2	445	471	0.02%	0.003%
67	10.292	2779	2784	2788	rBV2	232	224	0.01%	0.002%
68	10.359	2801	2805	2810	rBV2	263	343	0.02%	0.003%
69	10.385	2810	2813	2819	rBV	534	683	0.04%	0.005%
70	10.439	2827	2830	2833	rBV2	290	184	0.01%	0.001%
71	10.677	2895	2904	2912	rBV2	4179	6096	0.32%	0.045%
72	10.761	2917	2930	2950	rBV	598479	959657	50.63%	7.045%
73	10.841	2952	2955	2958	rVB3	504	306	0.02%	0.002%
74	10.870	2958	2964	2966	rBV3	580	599	0.03%	0.004%
75	11.057	3015	3022	3025	rBV3	258	392	0.02%	0.003%
76	11.086	3029	3031	3035	rBV3	331	245	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043725.D
 Acq On : 14 May 2021 01:57
 Operator : SY/MD
 Sample : M2327-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	11.124	3038	3043	3044	rBV3	745	610	0.03%	0.004%
78	11.160	3050	3054	3055	rBV	385	213	0.01%	0.002%
79	11.462	3141	3148	3163	rVB4	2655	5093	0.27%	0.037%
80	11.700	3215	3222	3232	rVB6	1562	2270	0.12%	0.017%
81	11.745	3233	3236	3238	rBV2	388	281	0.01%	0.002%
82	11.819	3246	3259	3279	rBV	608296	968933	51.12%	7.113%
83	11.947	3295	3299	3302	rBV4	875	723	0.04%	0.005%
84	12.044	3322	3329	3331	rBV3	380	426	0.02%	0.003%
85	12.115	3345	3351	3356	rBV4	552	616	0.03%	0.005%
86	12.198	3359	3377	3400	rVV	777110	1249138	65.91%	9.170%
87	12.275	3400	3401	3409	rVB4	878	715	0.04%	0.005%
88	12.337	3415	3420	3428	rVB6	1149	1423	0.08%	0.010%
89	12.401	3437	3440	3445	rVB	400	273	0.01%	0.002%
90	12.517	3473	3476	3479	rBV2	479	322	0.02%	0.002%
91	12.632	3508	3512	3515	rBV4	407	411	0.02%	0.003%
92	12.893	3590	3593	3596	rVB	507	290	0.02%	0.002%
93	13.076	3648	3650	3655	rBV3	339	201	0.01%	0.001%
94	13.147	3670	3672	3680	rVB2	337	280	0.01%	0.002%
95	13.619	3816	3819	3823	rBV	250	245	0.01%	0.002%
96	13.790	3869	3872	3875	rBV	362	224	0.01%	0.002%
97	13.851	3884	3891	3899	rVB5	841	1345	0.07%	0.010%
98	14.015	3939	3942	3945	rBV3	353	258	0.01%	0.002%
99	14.095	3960	3967	3973	rBV4	1549	2172	0.11%	0.016%
100	14.340	4036	4043	4046	rBV3	1259	1339	0.07%	0.010%




Sum of corrected areas: 13621554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043725.D
Acq On : 14 May 2021 01:57
Operator : SY/MD
Sample : M2327-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

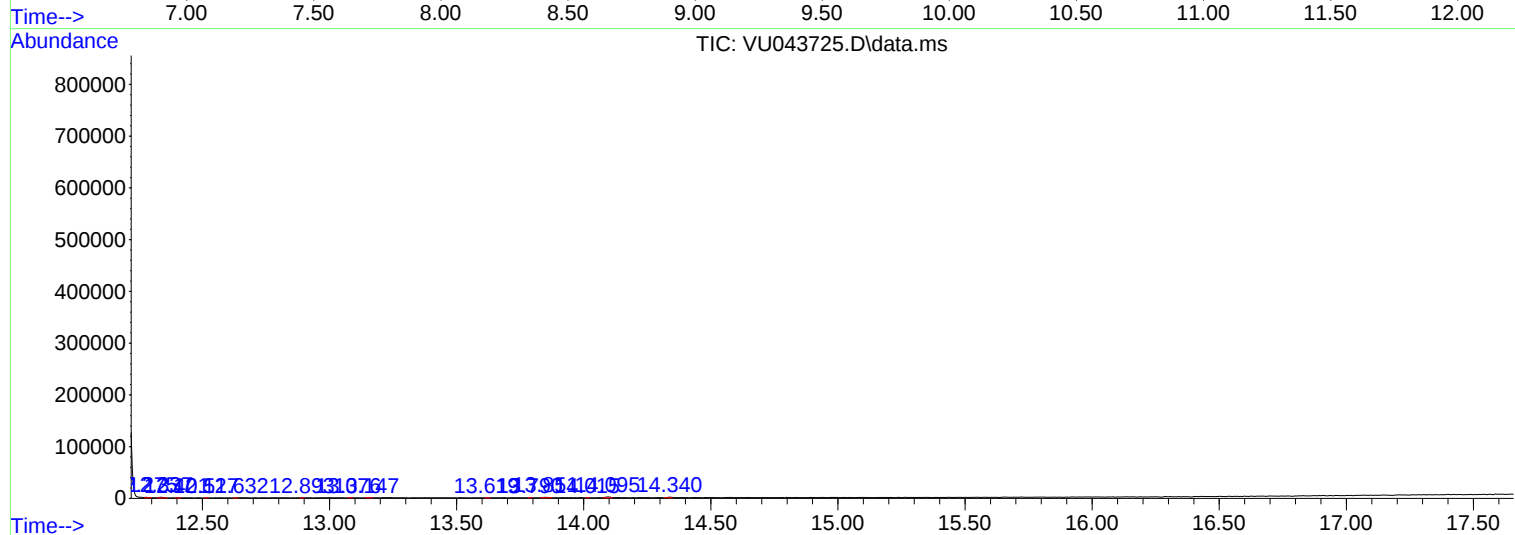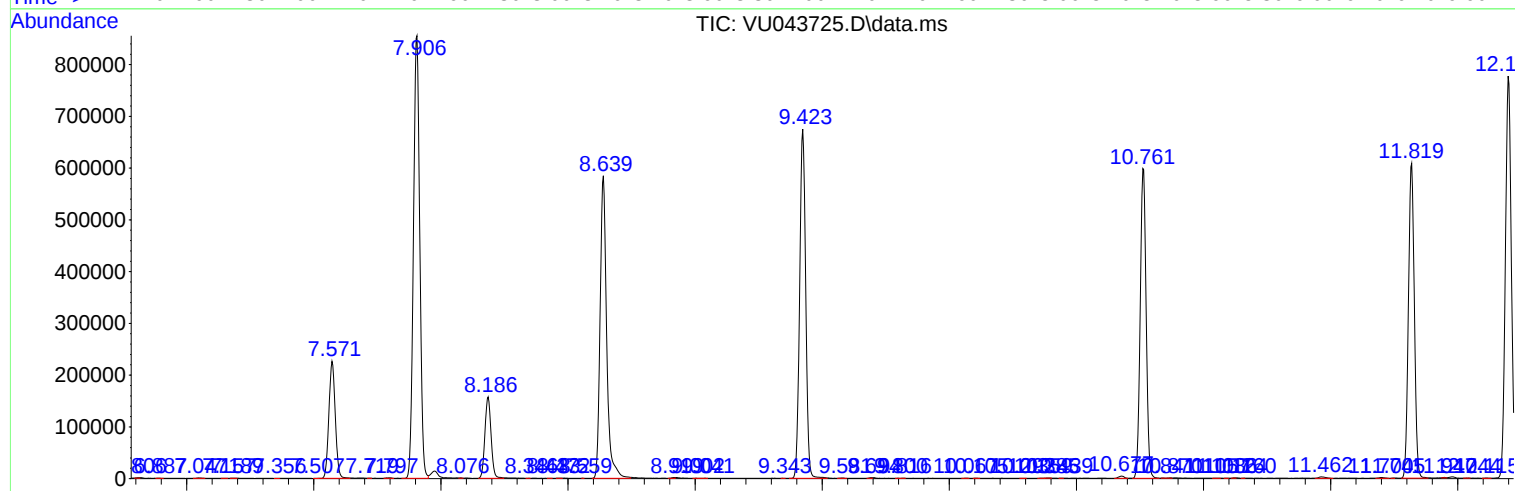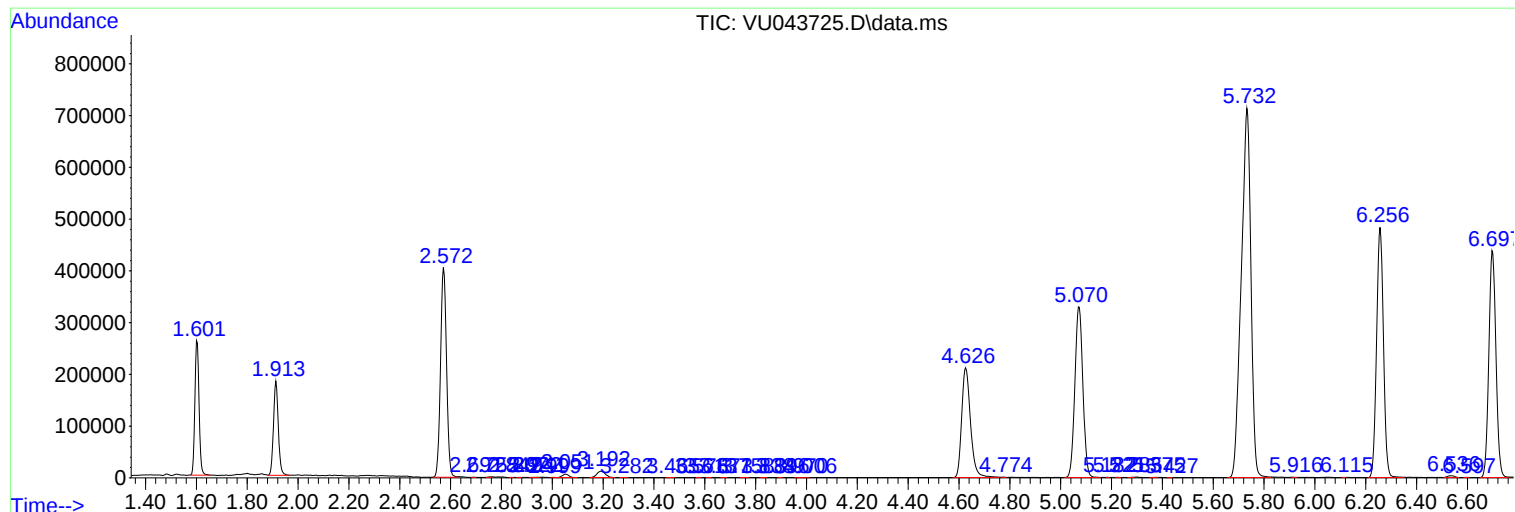

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043725.D
Acq On : 14 May 2021 01:57
Operator : SY/MD
Sample : M2327-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043725.D
Acq On : 14 May 2021 01:57
Operator : SY/MD
Sample : M2327-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
