

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043728.D
 Acq On : 14 May 2021 03:06
 Operator : SY/MD
 Sample : M2320-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

Signal : TIC: VU043728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rBV	253580	275721	15.08%	2.080%
2	1.909	169	177	194	rVB	167803	228275	12.49%	1.722%
3	2.571	370	383	401	rBV	384162	633216	34.63%	4.776%
4	2.951	497	501	507	rBV4	501	623	0.03%	0.005%
5	3.054	521	533	546	rBV	10816	20257	1.11%	0.153%
6	3.189	564	575	576	rBV3	2979	3653	0.20%	0.028%
7	3.324	614	617	623	rBV4	279	344	0.02%	0.003%
8	3.349	623	625	629	rVV	428	247	0.01%	0.002%
9	3.636	709	714	718	rVB2	270	259	0.01%	0.002%
10	3.655	718	720	724	rBV2	252	196	0.01%	0.001%
11	3.790	758	762	766	rBV2	256	221	0.01%	0.002%
12	4.137	864	870	872	rBV	179	181	0.01%	0.001%
13	4.430	958	961	973	rVB2	241	365	0.02%	0.003%
14	4.530	984	992	998	rVB3	294	524	0.03%	0.004%
15	4.626	1007	1022	1046	rBV	206332	488476	26.72%	3.685%
16	4.867	1094	1097	1100	rBV3	220	163	0.01%	0.001%
17	4.941	1117	1120	1123	rVB	377	231	0.01%	0.002%
18	5.073	1143	1161	1182	rBV	316288	691503	37.82%	5.216%
19	5.227	1204	1209	1212	rVB3	498	458	0.03%	0.003%
20	5.259	1217	1219	1222	rVV	296	166	0.01%	0.001%
21	5.295	1222	1230	1241	rVB3	1297	2679	0.15%	0.020%
22	5.385	1249	1258	1267	rBV2	527	996	0.05%	0.008%
23	5.504	1291	1295	1300	rBV2	294	243	0.01%	0.002%
24	5.620	1327	1331	1335	rBV2	215	161	0.01%	0.001%
25	5.732	1343	1366	1393	rBV2	684875	1828286	100.00%	13.791%
26	5.899	1415	1418	1422	rVB3	258	181	0.01%	0.001%
27	5.980	1440	1443	1446	rVB	332	177	0.01%	0.001%
28	6.044	1459	1463	1474	rVB5	773	990	0.05%	0.007%
29	6.108	1479	1483	1485	rBV2	345	299	0.02%	0.002%
30	6.256	1513	1529	1554	rBV	476981	899350	49.19%	6.784%
31	6.385	1566	1569	1570	rBV2	348	180	0.01%	0.001%
32	6.533	1607	1615	1628	rVB3	3839	7009	0.38%	0.053%
33	6.600	1632	1636	1642	rBV3	223	299	0.02%	0.002%
34	6.697	1651	1666	1692	rBV	424606	820684	44.89%	6.190%
35	6.800	1695	1698	1699	rVV2	833	551	0.03%	0.004%
36	6.812	1699	1702	1711	rVV3	1316	1656	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043728.D
 Acq On : 14 May 2021 03:06
 Operator : SY/MD
 Sample : M2320-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	6.848	1711	1713	1717	rVB2	518	348	0.02%	0.003%
38	6.964	1741	1749	1750	rBV2	217	234	0.01%	0.002%
39	7.047	1772	1775	1780	rVB	914	738	0.04%	0.006%
40	7.166	1808	1812	1813	rBV2	385	208	0.01%	0.002%
41	7.179	1813	1816	1817	rBV2	350	199	0.01%	0.002%
42	7.475	1901	1908	1912	rBV2	208	261	0.01%	0.002%
43	7.571	1923	1938	1955	rBV	212442	377846	20.67%	2.850%
44	7.687	1971	1974	1975	rBV2	553	340	0.02%	0.003%
45	7.735	1986	1989	1993	rVB2	278	239	0.01%	0.002%
46	7.790	2003	2006	2009	rBV	225	166	0.01%	0.001%
47	7.825	2014	2017	2022	rVB2	373	281	0.02%	0.002%
48	7.906	2026	2042	2056	rBV	822874	1404522	76.82%	10.594%
49	7.976	2057	2064	2075	rVB	12439	21464	1.17%	0.162%
50	8.185	2114	2129	2145	rBV	152009	251179	13.74%	1.895%
51	8.375	2184	2188	2191	rBV3	201	179	0.01%	0.001%
52	8.430	2202	2205	2209	rVB3	353	329	0.02%	0.002%
53	8.471	2209	2218	2220	rBV2	625	669	0.04%	0.005%
54	8.552	2239	2243	2246	rBV2	305	214	0.01%	0.002%
55	8.639	2257	2270	2303	rBV	582511	1031997	56.45%	7.784%
56	8.787	2314	2316	2318	rVB	402	166	0.01%	0.001%
57	8.870	2339	2342	2346	rBV3	346	280	0.02%	0.002%
58	8.896	2346	2350	2353	rVV3	312	236	0.01%	0.002%
59	8.925	2357	2359	2363	rVB	405	234	0.01%	0.002%
60	8.960	2366	2370	2374	rVB3	252	218	0.01%	0.002%
61	8.989	2374	2379	2380	rBV2	264	201	0.01%	0.002%
62	9.423	2495	2514	2550	rBV	676079	1111521	60.80%	8.384%
63	9.610	2568	2572	2576	rBV2	340	256	0.01%	0.002%
64	9.697	2594	2599	2601	rBV3	839	881	0.05%	0.007%
65	9.742	2609	2613	2615	rBV3	227	179	0.01%	0.001%
66	9.844	2641	2645	2649	rVB2	228	181	0.01%	0.001%
67	9.934	2668	2673	2678	rBV2	135	172	0.01%	0.001%
68	10.108	2719	2727	2730	rBV2	491	497	0.03%	0.004%
69	10.179	2743	2749	2753	rVB2	196	241	0.01%	0.002%
70	10.397	2812	2817	2823	rBV2	309	364	0.02%	0.003%
71	10.449	2830	2833	2837	rBV2	171	188	0.01%	0.001%
72	10.520	2850	2855	2860	rVB2	198	217	0.01%	0.002%
73	10.626	2884	2888	2891	rBV2	314	270	0.01%	0.002%
74	10.674	2895	2903	2913	rBV3	3845	5577	0.31%	0.042%
75	10.764	2917	2931	2949	rBV	586423	943180	51.59%	7.114%
76	10.877	2959	2966	2970	rBV4	830	1076	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043728.D
 Acq On : 14 May 2021 03:06
 Operator : SY/MD
 Sample : M2320-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	10.896	2970	2972	2979	rVV3	799	757	0.04%	0.006%
78	10.925	2979	2981	2988	rVV2	456	372	0.02%	0.003%
79	11.095	3030	3034	3037	rBV2	370	371	0.02%	0.003%
80	11.124	3037	3043	3048	rVV4	628	912	0.05%	0.007%
81	11.153	3048	3052	3061	rVB3	636	703	0.04%	0.005%
82	11.211	3066	3070	3073	rVB3	492	301	0.02%	0.002%
83	11.230	3073	3076	3081	rBV	187	186	0.01%	0.001%
84	11.458	3140	3147	3148	rBV3	1987	1713	0.09%	0.013%
85	11.584	3181	3186	3191	rBV2	370	448	0.02%	0.003%
86	11.703	3217	3223	3232	rVB5	1500	2112	0.12%	0.016%
87	11.758	3237	3240	3241	rBV2	321	163	0.01%	0.001%
88	11.819	3245	3259	3276	rBV	619498	969908	53.05%	7.316%
89	11.947	3294	3299	3302	rBV4	993	903	0.05%	0.007%
90	12.044	3326	3329	3331	rBV2	322	230	0.01%	0.002%
91	12.066	3334	3336	3340	rVB3	396	240	0.01%	0.002%
92	12.118	3350	3352	3357	rVB	340	236	0.01%	0.002%
93	12.198	3361	3377	3396	rBV	752218	1208259	66.09%	9.114%
94	12.343	3417	3422	3429	rVB4	958	1229	0.07%	0.009%
95	12.375	3430	3432	3435	rBV2	287	176	0.01%	0.001%
96	12.410	3441	3443	3446	rBV2	381	207	0.01%	0.002%
97	13.844	3887	3889	3890	rBV	506	254	0.01%	0.002%
98	14.031	3944	3947	3950	rBV2	332	214	0.01%	0.002%
99	15.462	4389	4392	4395	rBV3	608	442	0.02%	0.003%
100	15.934	4536	4539	4541	rBV3	778	515	0.03%	0.004%




Sum of corrected areas: 13257219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043728.D
Acq On : 14 May 2021 03:06
Operator : SY/MD
Sample : M2320-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

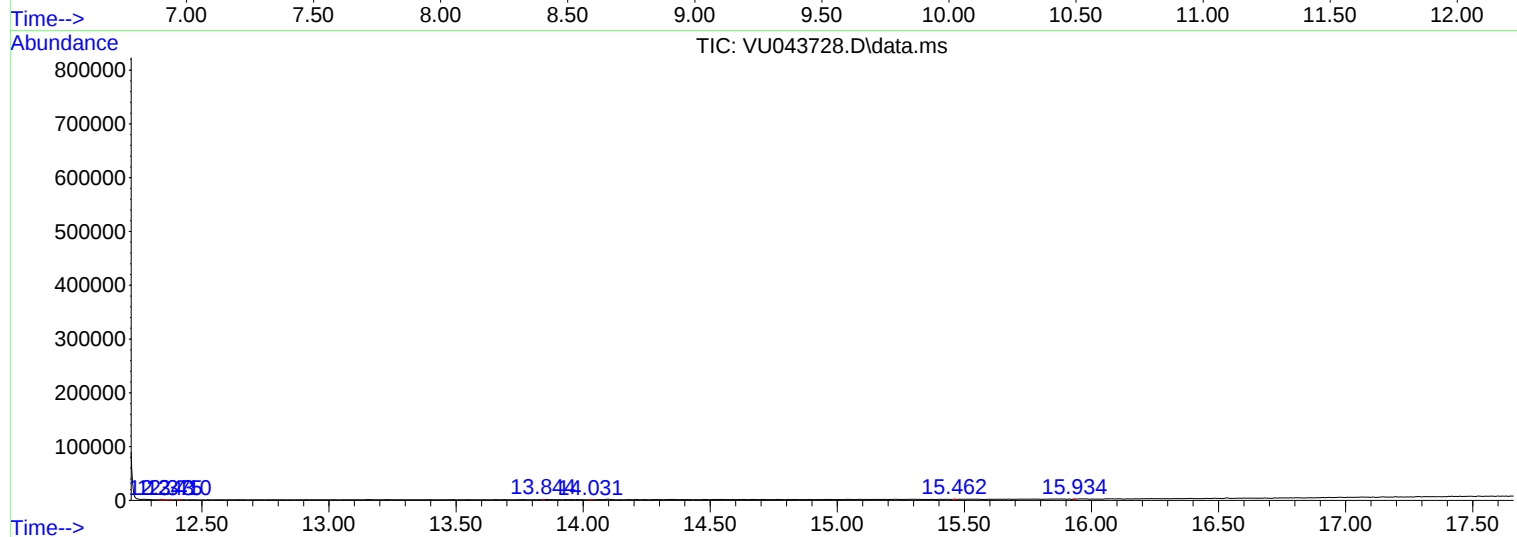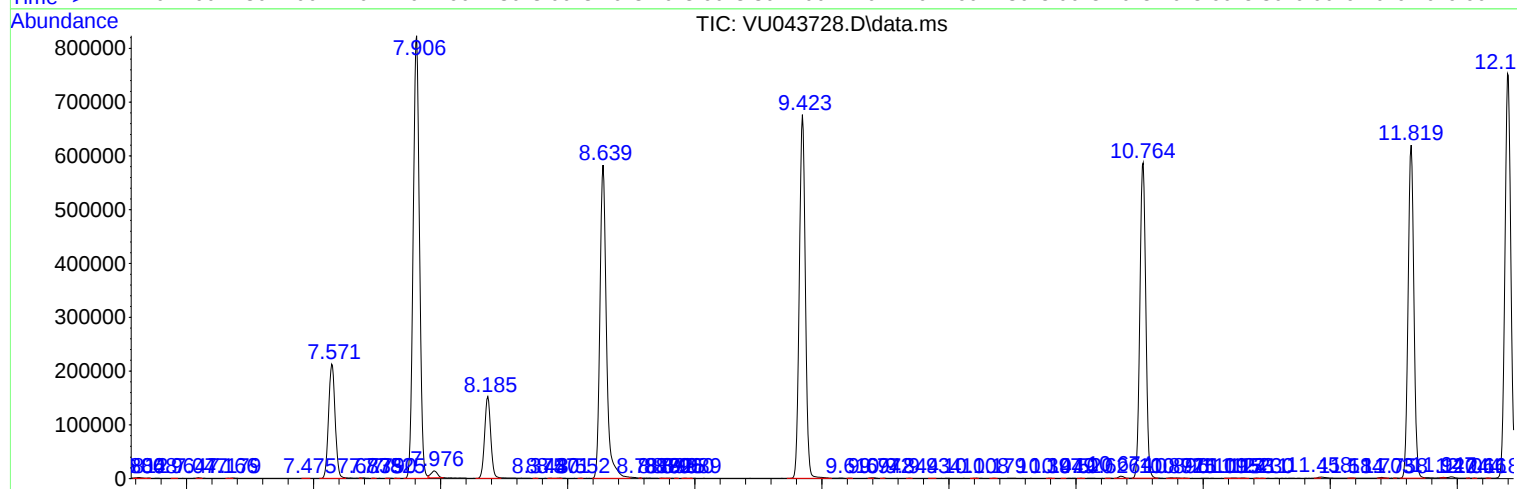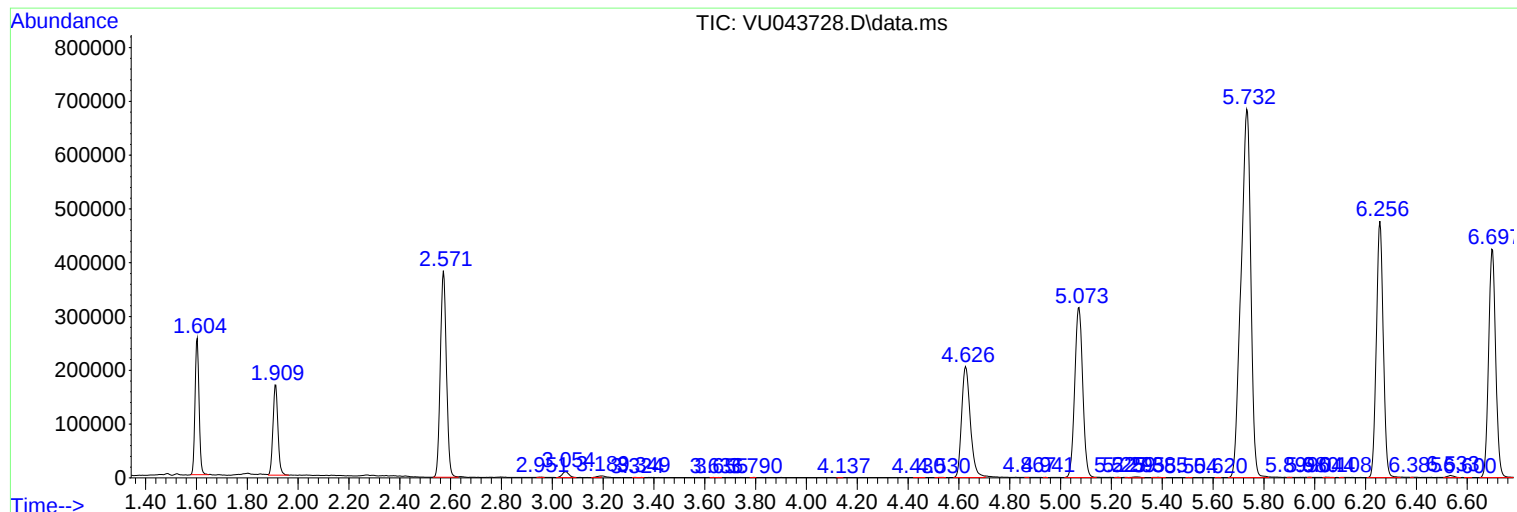

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043728.D
Acq On : 14 May 2021 03:06
Operator : SY/MD
Sample : M2320-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043728.D
Acq On : 14 May 2021 03:06
Operator : SY/MD
Sample : M2320-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
