

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043734.D
 Acq On : 14 May 2021 05:24
 Operator : SY/MD
 Sample : M2395-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M

Title : VOC Analysis

Signal : TIC: VU043734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	93	rBV	236200	266160	15.00%	2.040%
2	1.912	170	178	193	rVB	166021	217561	12.26%	1.667%
3	2.572	370	383	398	rVV	372658	608338	34.28%	4.662%
4	2.681	412	417	425	rVB4	531	581	0.03%	0.004%
5	2.803	446	455	462	rBV2	813	1338	0.08%	0.010%
6	2.983	509	511	515	rVB3	570	394	0.02%	0.003%
7	3.022	519	523	525	rBV2	286	258	0.01%	0.002%
8	3.054	525	533	539	rBV4	1274	1889	0.11%	0.014%
9	3.134	555	558	563	rVB2	368	302	0.02%	0.002%
10	3.189	570	575	577	rBV2	571	632	0.04%	0.005%
11	3.327	614	618	622	rBV2	367	292	0.02%	0.002%
12	3.385	632	636	639	rBV2	288	248	0.01%	0.002%
13	3.565	689	692	695	rVV2	216	178	0.01%	0.001%
14	3.594	699	701	705	rVV	267	206	0.01%	0.002%
15	3.620	705	709	713	rVV	233	237	0.01%	0.002%
16	3.642	713	716	719	rVV2	274	226	0.01%	0.002%
17	3.787	756	761	764	rBV	220	178	0.01%	0.001%
18	3.816	764	770	774	rVV3	211	230	0.01%	0.002%
19	4.224	893	897	901	rBV	217	181	0.01%	0.001%
20	4.272	907	912	918	rVB2	154	214	0.01%	0.002%
21	4.523	985	990	992	rBV2	268	191	0.01%	0.001%
22	4.626	1007	1022	1056	rBV	195318	467511	26.34%	3.583%
23	4.999	1132	1138	1142	rBV2	272	335	0.02%	0.003%
24	5.073	1142	1161	1178	rBV	308655	673415	37.94%	5.161%
25	5.308	1221	1234	1236	rBV2	1492	2348	0.13%	0.018%
26	5.382	1250	1257	1259	rBV3	693	911	0.05%	0.007%
27	5.465	1277	1283	1287	rBV	270	238	0.01%	0.002%
28	5.501	1287	1294	1296	rBV2	167	184	0.01%	0.001%
29	5.732	1344	1366	1390	rBV2	664863	1774786	100.00%	13.602%
30	5.883	1410	1413	1416	rBV	384	276	0.02%	0.002%
31	5.954	1433	1435	1439	rBV	280	175	0.01%	0.001%
32	6.256	1514	1529	1551	rBV	472263	894652	50.41%	6.857%
33	6.420	1578	1580	1587	rVB3	360	359	0.02%	0.003%
34	6.452	1587	1590	1595	rBV3	320	256	0.01%	0.002%
35	6.497	1601	1604	1608	rBV2	258	185	0.01%	0.001%
36	6.533	1608	1615	1625	rBV5	2642	4474	0.25%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043734.D
 Acq On : 14 May 2021 05:24
 Operator : SY/MD
 Sample : M2395-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	6.697	1652	1666	1694	rVV	410716	799182	45.03%	6.125%
38	6.813	1694	1702	1712	rVV6	1280	2353	0.13%	0.018%
39	6.944	1740	1743	1748	rBV2	326	256	0.01%	0.002%
40	7.031	1765	1770	1772	rBV2	301	242	0.01%	0.002%
41	7.050	1772	1776	1782	rVB3	495	605	0.03%	0.005%
42	7.182	1805	1817	1818	rBV3	731	718	0.04%	0.006%
43	7.263	1839	1842	1847	rVB2	285	200	0.01%	0.002%
44	7.520	1918	1922	1923	rBV	392	294	0.02%	0.002%
45	7.571	1925	1938	1960	rBV	209665	361786	20.38%	2.773%
46	7.690	1972	1975	1978	rBV5	490	245	0.01%	0.002%
47	7.793	2004	2007	2013	rVB4	554	466	0.03%	0.004%
48	7.832	2016	2019	2023	rVB2	220	211	0.01%	0.002%
49	7.906	2025	2042	2056	rBV	792682	1359976	76.63%	10.423%
50	7.973	2059	2063	2079	rVB	12574	19737	1.11%	0.151%
51	8.185	2116	2129	2147	rBV	146706	245619	13.84%	1.882%
52	8.372	2185	2187	2191	rVB2	412	284	0.02%	0.002%
53	8.394	2191	2194	2197	rBV2	293	220	0.01%	0.002%
54	8.517	2228	2232	2234	rBV3	331	223	0.01%	0.002%
55	8.558	2234	2245	2257	rBV	120864	201883	11.38%	1.547%
56	8.639	2257	2270	2299	rBV	552936	984354	55.46%	7.544%
57	8.890	2346	2348	2351	rVB2	350	183	0.01%	0.001%
58	9.176	2432	2437	2439	rBV	236	188	0.01%	0.001%
59	9.227	2450	2453	2455	rVV2	303	204	0.01%	0.002%
60	9.250	2457	2460	2464	rVV	351	260	0.01%	0.002%
61	9.423	2500	2514	2550	rVV	671707	1094588	61.67%	8.389%
62	9.568	2556	2559	2561	rBV	402	279	0.02%	0.002%
63	9.610	2570	2572	2579	rVB4	696	512	0.03%	0.004%
64	9.693	2593	2598	2607	rBV5	1229	1993	0.11%	0.015%
65	9.780	2621	2625	2628	rBV3	257	176	0.01%	0.001%
66	9.832	2637	2641	2643	rBV2	301	222	0.01%	0.002%
67	10.105	2722	2726	2731	rBV3	419	383	0.02%	0.003%
68	10.179	2744	2749	2754	rBV2	181	242	0.01%	0.002%
69	10.266	2771	2776	2779	rBV3	325	321	0.02%	0.002%
70	10.324	2790	2794	2798	rBV2	240	203	0.01%	0.002%
71	10.439	2827	2830	2836	rVB	232	180	0.01%	0.001%
72	10.677	2897	2904	2912	rBV5	2774	4122	0.23%	0.032%
73	10.761	2917	2930	2952	rBV	573311	911133	51.34%	6.983%
74	10.864	2957	2962	2963	rBV2	564	400	0.02%	0.003%
75	10.877	2964	2966	2967	rBV2	405	179	0.01%	0.001%
76	11.002	3002	3005	3007	rBV	408	267	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043734.D
 Acq On : 14 May 2021 05:24
 Operator : SY/MD
 Sample : M2395-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	11.037	3010	3016	3022	rVB5	1889	2518	0.14%	0.019%
78	11.095	3030	3034	3037	rVB3	324	249	0.01%	0.002%
79	11.115	3037	3040	3042	rBV2	511	404	0.02%	0.003%
80	11.153	3050	3052	3057	rVB3	462	318	0.02%	0.002%
81	11.320	3100	3104	3108	rBV	334	265	0.01%	0.002%
82	11.465	3142	3149	3159	rVB8	1985	3559	0.20%	0.027%
83	11.706	3215	3224	3229	rBV6	1290	1706	0.10%	0.013%
84	11.819	3246	3259	3277	rBV	609161	948581	53.45%	7.270%
85	11.944	3296	3298	3302	rBV3	561	474	0.03%	0.004%
86	11.976	3305	3308	3315	rVB4	1881	2138	0.12%	0.016%
87	12.063	3332	3335	3336	rBV	414	225	0.01%	0.002%
88	12.115	3348	3351	3354	rBV	284	231	0.01%	0.002%
89	12.131	3354	3356	3359	rVB2	513	213	0.01%	0.002%
90	12.198	3363	3377	3397	rBV	724436	1167780	65.80%	8.950%
91	12.330	3416	3418	3427	rVB3	779	934	0.05%	0.007%
92	12.446	3444	3454	3456	rBV2	371	579	0.03%	0.004%
93	12.494	3464	3469	3471	rBV2	409	403	0.02%	0.003%
94	12.639	3511	3514	3520	rVB4	544	566	0.03%	0.004%
95	12.960	3611	3614	3620	rVB3	391	308	0.02%	0.002%
96	13.176	3679	3681	3686	rBV	360	246	0.01%	0.002%
97	13.288	3714	3716	3719	rBV	356	181	0.01%	0.001%
98	13.568	3798	3803	3806	rBV3	313	356	0.02%	0.003%
99	13.706	3841	3846	3849	rBV3	395	416	0.02%	0.003%
100	14.594	4120	4122	4124	rBV2	451	289	0.02%	0.002%




Sum of corrected areas: 13047767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043734.D
Acq On : 14 May 2021 05:24
Operator : SY/MD
Sample : M2395-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

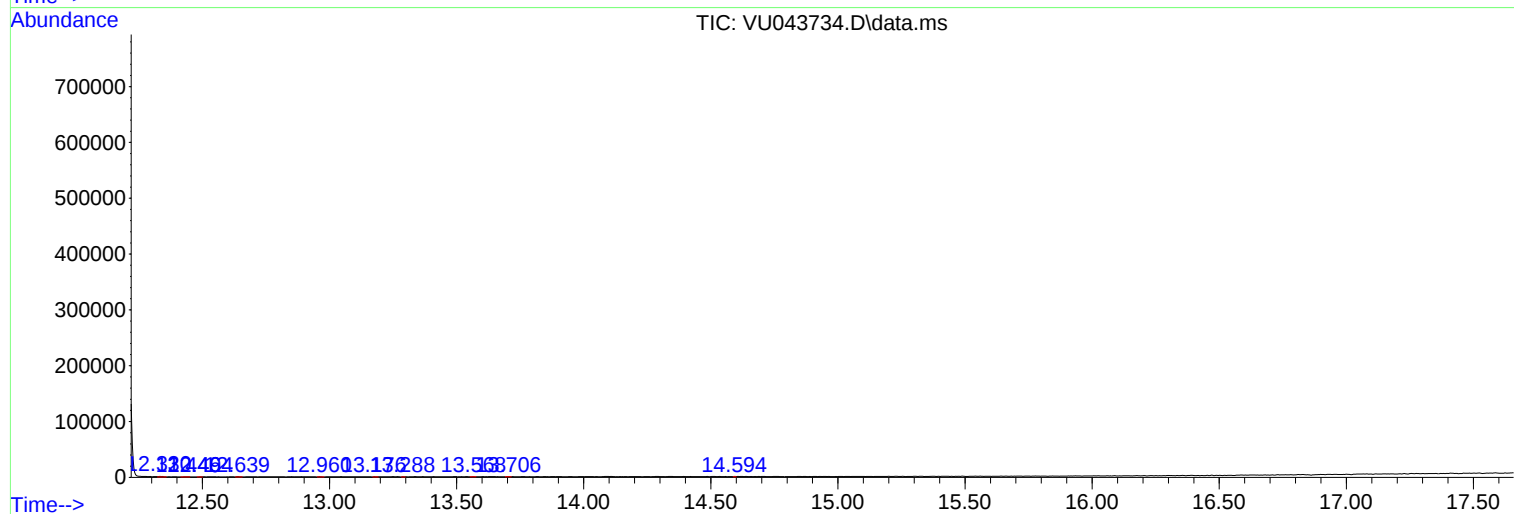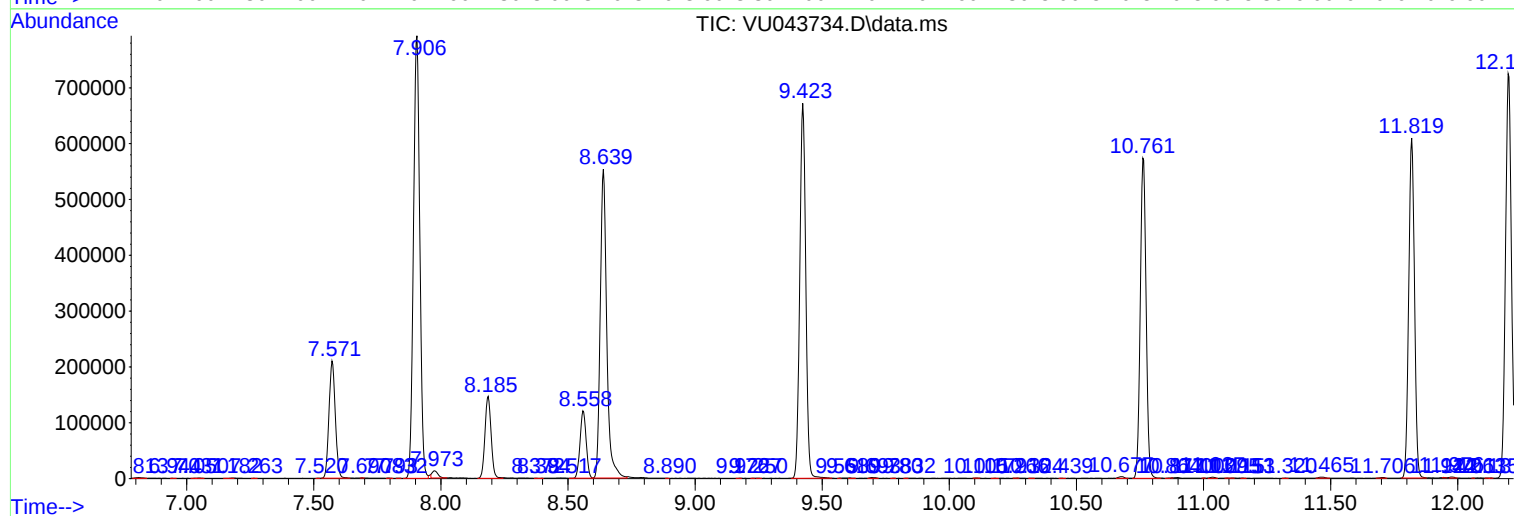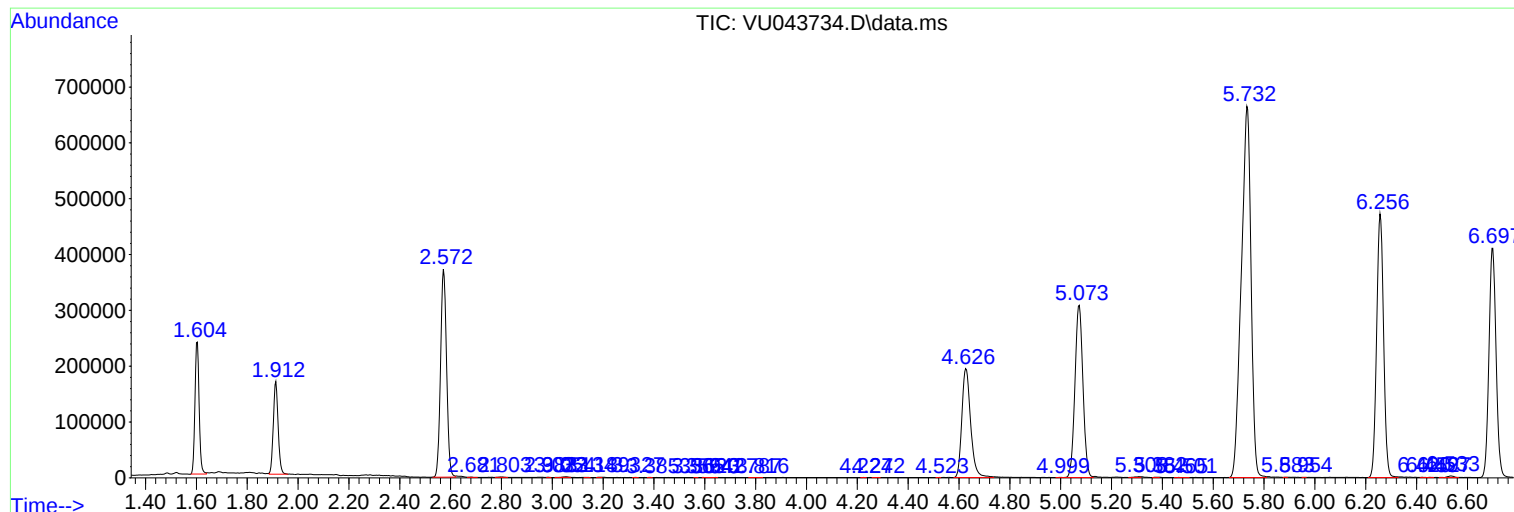

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043734.D
Acq On : 14 May 2021 05:24
Operator : SY/MD
Sample : M2395-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043734.D
Acq On : 14 May 2021 05:24
Operator : SY/MD
Sample : M2395-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
