

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043735.D
 Acq On : 14 May 2021 05:47
 Operator : SY/MD
 Sample : M2395-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

Signal : TIC: VU043735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	245132	274356	14.92%	2.012%
2	1.912	169	178	194	rVB	168859	227490	12.37%	1.668%
3	2.572	370	383	399	rBV	383056	626674	34.08%	4.596%
4	2.761	439	442	445	rVV2	223	165	0.01%	0.001%
5	2.797	448	453	462	rVB4	817	1265	0.07%	0.009%
6	2.883	478	480	483	rVB2	314	190	0.01%	0.001%
7	2.903	483	486	488	rBV2	304	224	0.01%	0.002%
8	2.954	496	502	506	rBV3	686	813	0.04%	0.006%
9	3.051	526	532	540	rVB5	1586	2434	0.13%	0.018%
10	3.102	545	548	550	rBV	242	153	0.01%	0.001%
11	3.189	570	575	577	rBV2	627	641	0.03%	0.005%
12	3.250	592	594	597	rVB2	287	159	0.01%	0.001%
13	3.282	601	604	607	rBV2	271	186	0.01%	0.001%
14	3.301	607	610	613	rVB2	221	142	0.01%	0.001%
15	3.318	613	615	618	rBV2	288	218	0.01%	0.002%
16	3.449	652	656	660	rBV2	181	189	0.01%	0.001%
17	3.491	665	669	672	rBV3	271	238	0.01%	0.002%
18	3.639	712	715	718	rVB2	184	145	0.01%	0.001%
19	3.922	800	803	808	rBV	230	168	0.01%	0.001%
20	4.057	842	845	853	rVB2	402	341	0.02%	0.003%
21	4.375	938	944	946	rBV	220	207	0.01%	0.002%
22	4.443	963	965	969	rBV2	263	182	0.01%	0.001%
23	4.520	986	989	992	rBV	336	242	0.01%	0.002%
24	4.626	1006	1022	1051	rBV	199744	474441	25.80%	3.479%
25	4.832	1084	1086	1089	rVB2	389	209	0.01%	0.002%
26	5.006	1137	1140	1142	rBV2	229	163	0.01%	0.001%
27	5.070	1142	1160	1187	rVV	319039	699547	38.04%	5.130%
28	5.221	1203	1207	1208	rBV2	273	210	0.01%	0.002%
29	5.247	1213	1215	1218	rVB2	254	166	0.01%	0.001%
30	5.295	1221	1230	1231	rBV	1154	1144	0.06%	0.008%
31	5.379	1248	1256	1264	rBV3	720	1247	0.07%	0.009%
32	5.465	1280	1283	1289	rVV2	162	158	0.01%	0.001%
33	5.732	1342	1366	1396	rBV2	689988	1839027	100.00%	13.487%
34	6.044	1459	1463	1466	rBV4	695	546	0.03%	0.004%
35	6.112	1480	1484	1485	rBV3	191	146	0.01%	0.001%
36	6.256	1514	1529	1551	rBV	518373	967189	52.59%	7.093%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043735.D
 Acq On : 14 May 2021 05:47
 Operator : SY/MD
 Sample : M2395-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	6.501	1600	1605	1607	rBV3	317	294	0.02%	0.002%
38	6.533	1607	1615	1623	rVV3	3149	5363	0.29%	0.039%
39	6.607	1634	1638	1643	rVB3	426	421	0.02%	0.003%
40	6.697	1643	1666	1689	rBV	422162	827092	44.97%	6.066%
41	6.816	1700	1703	1710	rVB4	1023	987	0.05%	0.007%
42	6.845	1710	1712	1716	rVB3	573	287	0.02%	0.002%
43	6.960	1744	1748	1751	rBV2	212	222	0.01%	0.002%
44	6.977	1751	1753	1758	rVB	228	159	0.01%	0.001%
45	7.050	1768	1776	1783	rVB4	651	957	0.05%	0.007%
46	7.182	1815	1817	1819	rBV	253	165	0.01%	0.001%
47	7.192	1819	1820	1825	rVB2	836	448	0.02%	0.003%
48	7.571	1924	1938	1957	rBV	216136	375327	20.41%	2.753%
49	7.694	1974	1976	1980	rVB2	588	352	0.02%	0.003%
50	7.729	1985	1987	1990	rVB3	313	193	0.01%	0.001%
51	7.796	2003	2008	2013	rBV2	576	581	0.03%	0.004%
52	7.906	2027	2042	2056	rBV	834473	1417625	77.09%	10.397%
53	8.140	2113	2115	2117	rBV2	211	141	0.01%	0.001%
54	8.185	2117	2129	2159	rVB	150077	254060	13.81%	1.863%
55	8.295	2159	2163	2166	rBV3	465	446	0.02%	0.003%
56	8.337	2172	2176	2178	rBV3	211	174	0.01%	0.001%
57	8.353	2178	2181	2183	rVV3	398	236	0.01%	0.002%
58	8.391	2190	2193	2197	rVB2	290	213	0.01%	0.002%
59	8.411	2197	2199	2203	rBV2	185	171	0.01%	0.001%
60	8.478	2216	2220	2225	rBV3	674	705	0.04%	0.005%
61	8.558	2233	2245	2257	rBV	123004	205526	11.18%	1.507%
62	8.639	2257	2270	2309	rVV	570992	1027333	55.86%	7.534%
63	8.796	2316	2319	2324	rVB5	1010	826	0.04%	0.006%
64	8.893	2346	2349	2352	rVB3	309	168	0.01%	0.001%
65	9.259	2460	2463	2467	rVB2	243	194	0.01%	0.001%
66	9.423	2500	2514	2535	rBV	724380	1180789	64.21%	8.660%
67	9.578	2555	2562	2564	rBV3	348	472	0.03%	0.003%
68	9.700	2593	2600	2610	rVB2	1520	2227	0.12%	0.016%
69	9.919	2665	2668	2672	rBV2	267	226	0.01%	0.002%
70	10.285	2779	2782	2783	rBV	244	163	0.01%	0.001%
71	10.349	2799	2802	2805	rVV	268	177	0.01%	0.001%
72	10.427	2820	2826	2829	rBV2	276	300	0.02%	0.002%
73	10.494	2843	2847	2850	rBV2	237	200	0.01%	0.001%
74	10.610	2878	2883	2886	rBV	354	255	0.01%	0.002%
75	10.677	2896	2904	2915	rVB2	3210	4407	0.24%	0.032%
76	10.764	2915	2931	2952	rBV	597109	955125	51.94%	7.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043735.D
 Acq On : 14 May 2021 05:47
 Operator : SY/MD
 Sample : M2395-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	10.870	2960	2964	2968	rBV2	713	809	0.04%	0.006%
78	11.034	3010	3015	3020	rBV4	1044	1008	0.05%	0.007%
79	11.057	3020	3022	3026	rVB2	305	187	0.01%	0.001%
80	11.095	3031	3034	3036	rBV	257	185	0.01%	0.001%
81	11.301	3095	3098	3104	rVB2	317	231	0.01%	0.002%
82	11.365	3115	3118	3123	rBV2	182	155	0.01%	0.001%
83	11.468	3142	3150	3159	rVB3	2095	3340	0.18%	0.024%
84	11.526	3166	3168	3172	rBV2	186	156	0.01%	0.001%
85	11.587	3182	3187	3193	rVB3	448	551	0.03%	0.004%
86	11.652	3203	3207	3212	rBV2	258	254	0.01%	0.002%
87	11.703	3217	3223	3230	rVB5	1251	1549	0.08%	0.011%
88	11.819	3246	3259	3274	rBV	643807	1018474	55.38%	7.469%
89	11.941	3295	3297	3303	rVV5	709	717	0.04%	0.005%
90	11.980	3303	3309	3316	rVB3	2027	2332	0.13%	0.017%
91	12.070	3334	3337	3342	rVB4	635	627	0.03%	0.005%
92	12.108	3347	3349	3351	rBV2	252	146	0.01%	0.001%
93	12.198	3363	3377	3397	rVV	754047	1216602	66.15%	8.922%
94	12.330	3415	3418	3419	rBV	552	339	0.02%	0.002%
95	12.536	3480	3482	3485	rBV2	254	142	0.01%	0.001%
96	13.012	3628	3630	3632	rBV	277	171	0.01%	0.001%
97	13.147	3669	3672	3673	rBV	383	201	0.01%	0.001%
98	14.063	3954	3957	3962	rBV2	385	301	0.02%	0.002%
99	14.095	3962	3967	3970	rBV4	514	627	0.03%	0.005%
100	14.504	4091	4094	4096	rBV2	372	270	0.01%	0.002%


Sum of corrected areas: 13635396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043735.D
Acq On : 14 May 2021 05:47
Operator : SY/MD
Sample : M2395-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

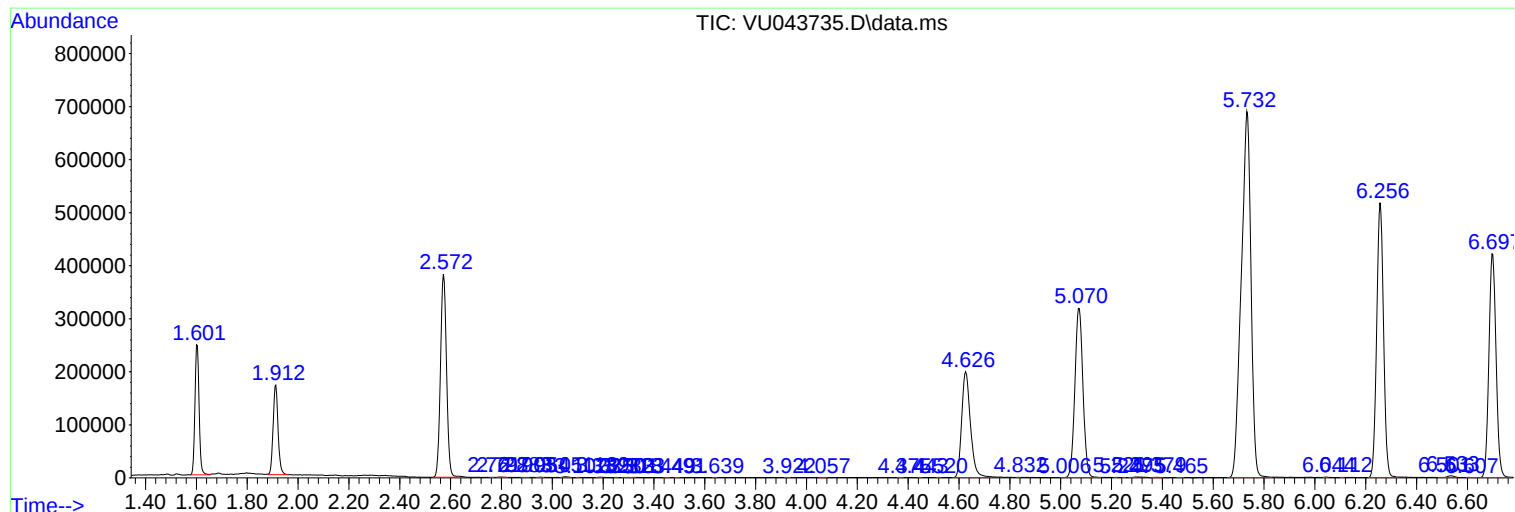

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043735.D
Acq On : 14 May 2021 05:47
Operator : SY/MD
Sample : M2395-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043735.D
Acq On : 14 May 2021 05:47
Operator : SY/MD
Sample : M2395-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
