

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043736.D
 Acq On : 14 May 2021 06:10
 Operator : SY/MD
 Sample : M2395-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M

Title : VOC Analysis

Signal : TIC: VU043736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rVB	235487	263488	14.92%	1.992%
2	1.912	170	178	195	rVB	168154	221227	12.53%	1.672%
3	2.571	370	383	399	rBV	369951	607809	34.43%	4.595%
4	2.797	447	453	463	rBV3	1245	2110	0.12%	0.016%
5	3.025	520	524	525	rBV	328	207	0.01%	0.002%
6	3.054	525	533	540	rVB3	1204	2063	0.12%	0.016%
7	3.141	555	560	562	rBV2	317	260	0.01%	0.002%
8	3.176	568	571	574	rVB2	404	209	0.01%	0.002%
9	3.192	574	576	584	rBV2	468	520	0.03%	0.004%
10	3.250	590	594	598	rVB3	254	234	0.01%	0.002%
11	3.301	604	610	615	rBV2	381	372	0.02%	0.003%
12	3.350	621	625	631	rVB	298	357	0.02%	0.003%
13	3.404	638	642	645	rBV3	254	218	0.01%	0.002%
14	3.446	652	655	661	rBV2	346	246	0.01%	0.002%
15	3.787	756	761	773	rBV2	283	547	0.03%	0.004%
16	3.867	780	786	788	rBV2	201	225	0.01%	0.002%
17	4.034	833	838	841	rBV2	163	179	0.01%	0.001%
18	4.105	856	860	865	rVB2	185	168	0.01%	0.001%
19	4.179	876	883	885	rBV	260	223	0.01%	0.002%
20	4.456	964	969	972	rBV	200	163	0.01%	0.001%
21	4.629	1003	1023	1067	rBV	183337	452066	25.61%	3.417%
22	5.073	1143	1161	1186	rBV	308936	675548	38.26%	5.107%
23	5.211	1202	1204	1206	rVB2	378	173	0.01%	0.001%
24	5.231	1206	1210	1215	rVB4	487	514	0.03%	0.004%
25	5.279	1222	1225	1226	rBV	494	253	0.01%	0.002%
26	5.295	1226	1230	1234	rBV3	818	801	0.05%	0.006%
27	5.366	1248	1252	1253	rBV2	278	181	0.01%	0.001%
28	5.382	1253	1257	1263	rVB3	387	521	0.03%	0.004%
29	5.732	1343	1366	1401	rBV2	653956	1765481	100.00%	13.346%
30	5.867	1406	1408	1410	rVV2	722	438	0.02%	0.003%
31	5.899	1413	1418	1423	rVV3	375	451	0.03%	0.003%
32	5.941	1427	1431	1436	rBV	332	275	0.02%	0.002%
33	6.047	1454	1464	1468	rBV4	692	883	0.05%	0.007%
34	6.189	1506	1508	1511	rBV	327	206	0.01%	0.002%
35	6.256	1514	1529	1553	rBV	469381	885818	50.17%	6.696%
36	6.414	1576	1578	1582	rBV	318	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043736.D
 Acq On : 14 May 2021 06:10
 Operator : SY/MD
 Sample : M2395-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	6.533	1608	1615	1625	rVB5	2818	4973	0.28%	0.038%
38	6.700	1651	1667	1690	rBV	403513	792093	44.87%	5.988%
39	6.809	1695	1701	1709	rVB6	1281	2058	0.12%	0.016%
40	6.883	1721	1724	1727	rBV2	270	170	0.01%	0.001%
41	7.031	1763	1770	1771	rBV	361	245	0.01%	0.002%
42	7.179	1813	1816	1817	rBV	347	200	0.01%	0.002%
43	7.189	1817	1819	1825	rVB2	727	543	0.03%	0.004%
44	7.465	1901	1905	1908	rBV2	227	197	0.01%	0.001%
45	7.571	1924	1938	1957	rBV	205540	359402	20.36%	2.717%
46	7.719	1982	1984	1988	rVB3	427	212	0.01%	0.002%
47	7.800	2001	2009	2018	rBV4	2595	4234	0.24%	0.032%
48	7.906	2027	2042	2056	rBV	789619	1347912	76.35%	10.189%
49	8.185	2115	2129	2154	rBV	144563	243699	13.80%	1.842%
50	8.349	2178	2180	2186	rVB3	390	272	0.02%	0.002%
51	8.404	2194	2197	2201	rVB	239	165	0.01%	0.001%
52	8.478	2214	2220	2226	rBV2	593	728	0.04%	0.006%
53	8.558	2231	2245	2258	rBV	277727	469302	26.58%	3.548%
54	8.639	2258	2270	2300	rVV	547119	973218	55.12%	7.357%
55	8.963	2367	2371	2372	rBV2	332	184	0.01%	0.001%
56	9.185	2436	2440	2441	rBV	335	204	0.01%	0.002%
57	9.423	2499	2514	2548	rBV	656025	1078650	61.10%	8.154%
58	9.578	2559	2562	2565	rVV3	514	408	0.02%	0.003%
59	9.597	2566	2568	2577	rVB3	926	1086	0.06%	0.008%
60	9.700	2592	2600	2610	rBV4	1720	2825	0.16%	0.021%
61	9.790	2625	2628	2631	rBV2	261	176	0.01%	0.001%
62	9.816	2631	2636	2638	rBV	167	163	0.01%	0.001%
63	9.935	2669	2673	2675	rBV2	292	202	0.01%	0.002%
64	9.970	2681	2684	2689	rVB2	212	176	0.01%	0.001%
65	10.018	2696	2699	2702	rBV2	274	186	0.01%	0.001%
66	10.108	2721	2727	2729	rBV3	452	405	0.02%	0.003%
67	10.166	2742	2745	2750	rBV2	185	210	0.01%	0.002%
68	10.420	2820	2824	2829	rVB2	290	246	0.01%	0.002%
69	10.555	2863	2866	2871	rVB	245	188	0.01%	0.001%
70	10.603	2875	2881	2885	rBV2	289	338	0.02%	0.003%
71	10.626	2885	2888	2894	rVB2	213	197	0.01%	0.001%
72	10.677	2894	2904	2915	rBV5	3192	4603	0.26%	0.035%
73	10.764	2916	2931	2955	rBV	561059	900770	51.02%	6.809%
74	10.848	2955	2957	2960	rVB2	334	168	0.01%	0.001%
75	10.870	2960	2964	2965	rBV	955	539	0.03%	0.004%
76	10.902	2970	2974	2982	rVV5	1146	1188	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043736.D
 Acq On : 14 May 2021 06:10
 Operator : SY/MD
 Sample : M2395-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW6E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	10.999	3001	3004	3010	rVB3	509	508	0.03%	0.004%
78	11.053	3017	3021	3029	rVB4	508	631	0.04%	0.005%
79	11.121	3038	3042	3047	rVB5	770	694	0.04%	0.005%
80	11.385	3116	3124	3130	rVB3	370	545	0.03%	0.004%
81	11.420	3130	3135	3140	rBV3	468	428	0.02%	0.003%
82	11.462	3142	3148	3163	rVB6	2615	4068	0.23%	0.031%
83	11.581	3181	3185	3187	rBV2	587	482	0.03%	0.004%
84	11.700	3217	3222	3233	rBV4	1263	1749	0.10%	0.013%
85	11.748	3233	3237	3246	rBV2	646	1142	0.06%	0.009%
86	11.819	3246	3259	3281	rVV	597318	945604	53.56%	7.148%
87	12.069	3325	3337	3351	rBV3	7792	14486	0.82%	0.110%
88	12.201	3360	3378	3399	rBV	728013	1177198	66.68%	8.899%
89	12.336	3418	3420	3425	rVB3	1240	785	0.04%	0.006%
90	12.385	3431	3435	3438	rBV2	338	293	0.02%	0.002%
91	12.449	3452	3455	3459	rVB3	361	272	0.02%	0.002%
92	12.475	3459	3463	3466	rBV2	301	253	0.01%	0.002%
93	12.494	3466	3469	3472	rBV	319	277	0.02%	0.002%
94	12.606	3502	3504	3507	rBV2	268	174	0.01%	0.001%
95	12.735	3541	3544	3546	rBV	267	185	0.01%	0.001%
96	13.156	3671	3675	3681	rBV4	448	494	0.03%	0.004%
97	13.291	3714	3717	3722	rBV2	317	317	0.02%	0.002%
98	14.012	3939	3941	3944	rBV	384	230	0.01%	0.002%
99	14.227	4004	4008	4012	rBV3	559	532	0.03%	0.004%
100	15.201	4309	4311	4312	rBV2	438	196	0.01%	0.001%


Sum of corrected areas: 13228937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043736.D
Acq On : 14 May 2021 06:10
Operator : SY/MD
Sample : M2395-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

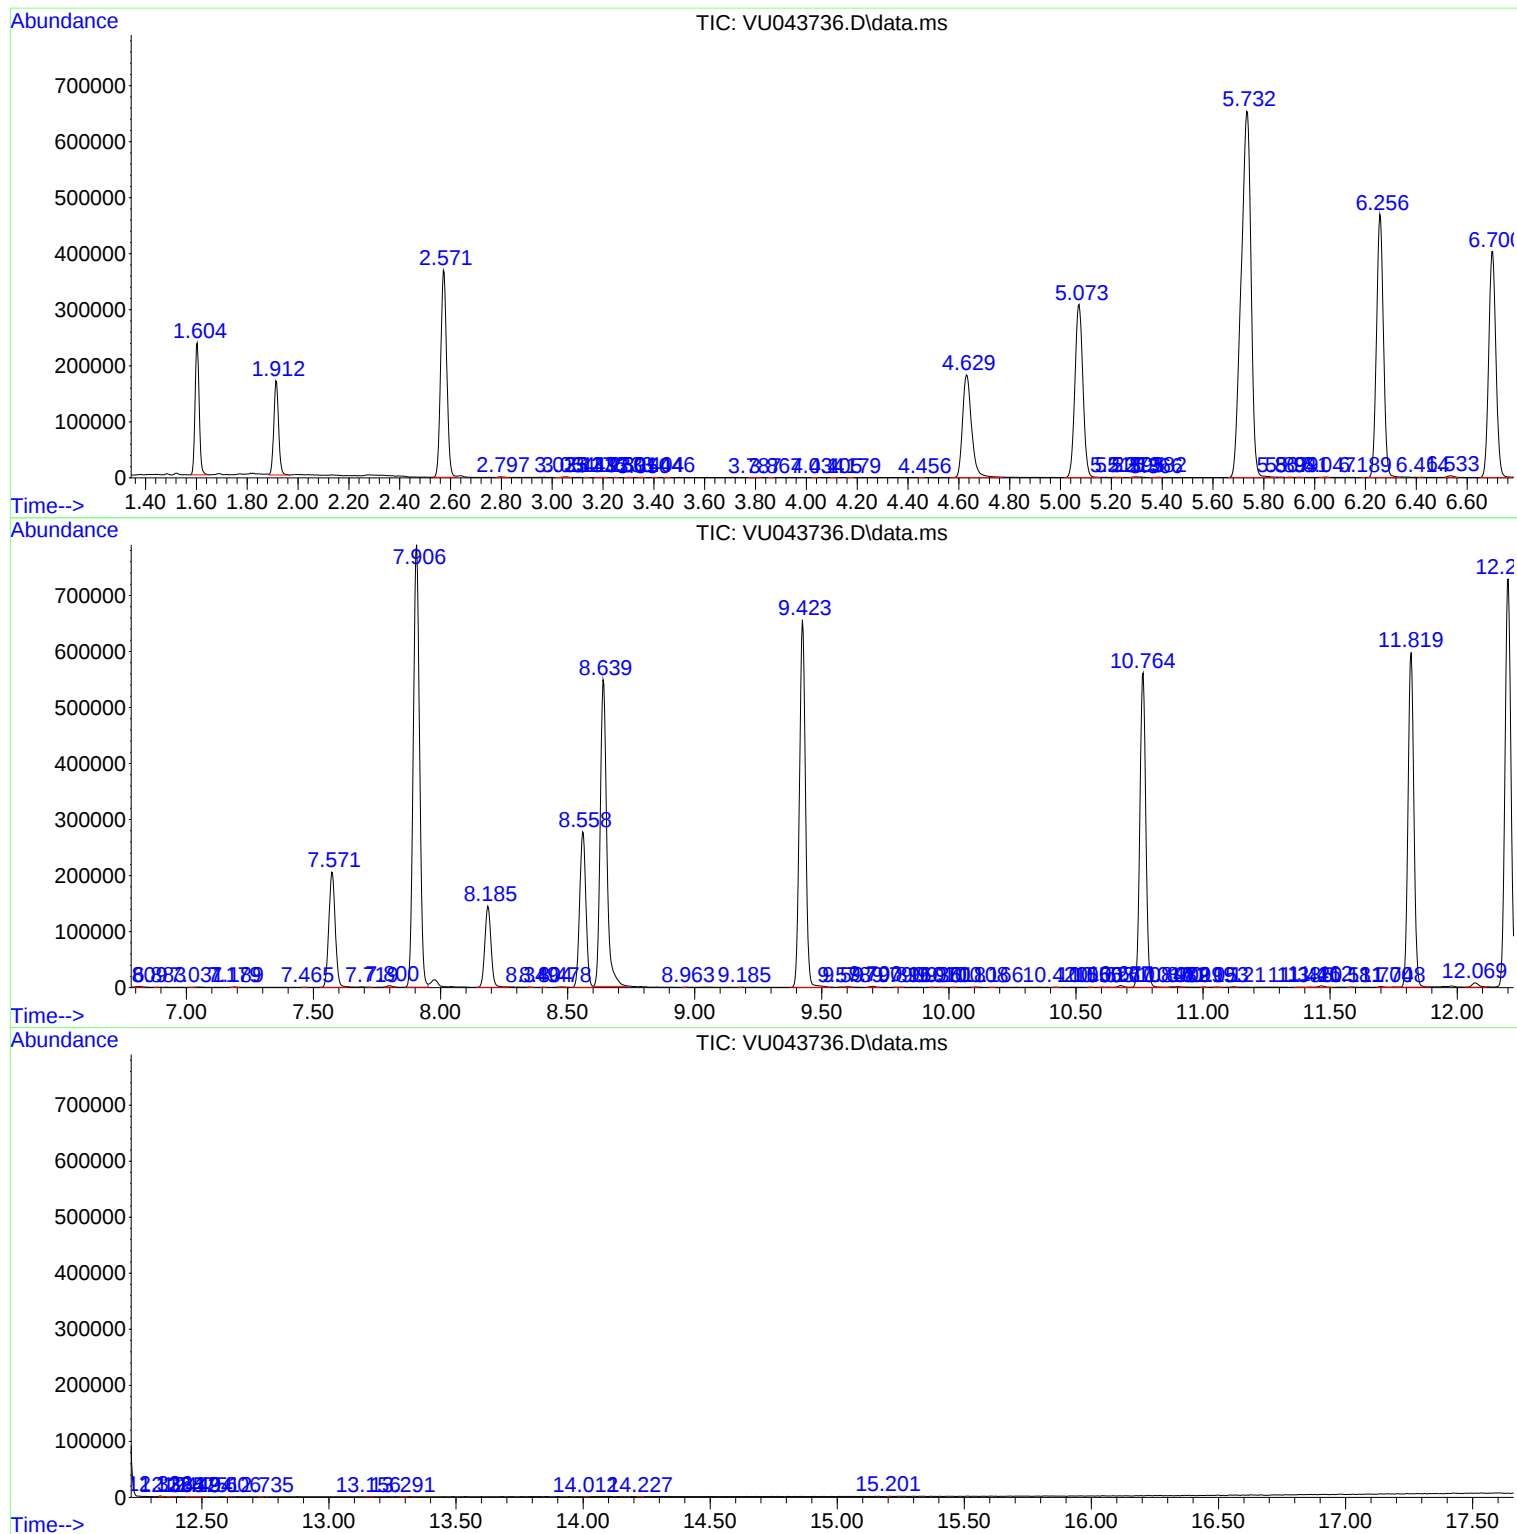

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043736.D
Acq On : 14 May 2021 06:10
Operator : SY/MD
Sample : M2395-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043736.D
Acq On : 14 May 2021 06:10
Operator : SY/MD
Sample : M2395-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW6E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
