

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043741.D
 Acq On : 14 May 2021 09:24
 Operator : SY/MD
 Sample : VU0514WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

Signal : TIC: VU043741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	98	rVB	270827	298385	15.36%	2.051%
2	1.912	170	178	193	rVB	179909	240848	12.39%	1.655%
3	2.571	371	383	401	rBV	422219	694633	35.75%	4.774%
4	2.710	424	426	429	rBV	185	85	0.00%	0.001%
5	2.735	432	434	441	rBV2	351	374	0.02%	0.003%
6	3.054	525	533	547	rVB6	2902	5453	0.28%	0.037%
7	3.189	567	575	581	rBV2	681	1217	0.06%	0.008%
8	3.237	588	590	593	rVB2	285	116	0.01%	0.001%
9	3.350	623	625	626	rBV	199	111	0.01%	0.001%
10	3.414	643	645	648	rBV2	149	91	0.00%	0.001%
11	3.449	654	656	660	rVB2	211	88	0.00%	0.001%
12	3.481	664	666	672	rVV2	249	163	0.01%	0.001%
13	3.514	673	676	681	rVB2	144	133	0.01%	0.001%
14	3.568	689	693	696	rBV2	152	119	0.01%	0.001%
15	3.588	696	699	702	rVV2	139	87	0.00%	0.001%
16	3.604	702	704	709	rVV2	186	112	0.01%	0.001%
17	3.645	713	717	720	rBV2	216	163	0.01%	0.001%
18	3.665	720	723	726	rBV2	147	90	0.00%	0.001%
19	3.816	768	770	773	rBV	122	76	0.00%	0.001%
20	3.906	796	798	801	rVB2	146	78	0.00%	0.001%
21	3.925	801	804	805	rBV	157	99	0.01%	0.001%
22	4.018	830	833	840	rVV2	197	249	0.01%	0.002%
23	4.124	864	866	870	rBV2	53	39	0.00%	0.000%
24	4.153	870	875	878	rBV	204	177	0.01%	0.001%
25	4.198	885	889	895	rBV2	143	162	0.01%	0.001%
26	4.234	895	900	903	rVB2	208	164	0.01%	0.001%
27	4.250	903	905	908	rBV	112	64	0.00%	0.000%
28	4.423	957	959	961	rBV	84	49	0.00%	0.000%
29	4.469	969	973	976	rBV2	166	142	0.01%	0.001%
30	4.520	987	989	993	rVB2	284	177	0.01%	0.001%
31	4.626	1005	1022	1050	rBV	202928	484300	24.92%	3.328%
32	4.993	1133	1136	1139	rBV2	209	139	0.01%	0.001%
33	5.073	1144	1161	1180	rBV	343184	743721	38.27%	5.111%
34	5.218	1203	1206	1207	rBV	453	252	0.01%	0.002%
35	5.259	1217	1219	1221	rBV2	194	128	0.01%	0.001%
36	5.292	1222	1229	1231	rBV4	1110	1157	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043741.D
 Acq On : 14 May 2021 09:24
 Operator : SY/MD
 Sample : VU0514WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

37	5.382	1250	1257	1264	rBV3	690	956	0.05%	0.007%
38	5.465	1280	1283	1286	rBV2	126	98	0.01%	0.001%
39	5.481	1286	1288	1290	rVV	69	39	0.00%	0.000%
40	5.494	1290	1292	1296	rVV2	115	85	0.00%	0.001%
41	5.526	1296	1302	1306	rVV	225	258	0.01%	0.002%
42	5.549	1306	1309	1313	rVB2	232	150	0.01%	0.001%
43	5.658	1340	1343	1344	rBV	174	94	0.00%	0.001%
44	5.735	1344	1367	1395	rVV2	733551	1943188	100.00%	13.355%
45	6.108	1480	1483	1486	rBV2	425	349	0.02%	0.002%
46	6.163	1498	1500	1506	rBV2	371	361	0.02%	0.002%
47	6.256	1514	1529	1552	rBV	584520	1096012	56.40%	7.533%
48	6.536	1606	1616	1629	rVB2	4580	8330	0.43%	0.057%
49	6.645	1644	1650	1652	rBV2	165	167	0.01%	0.001%
50	6.700	1652	1667	1692	rVV	448403	872998	44.93%	6.000%
51	6.854	1711	1715	1716	rBV	254	147	0.01%	0.001%
52	6.867	1716	1719	1721	rVB2	259	150	0.01%	0.001%
53	6.880	1721	1723	1724	rBV2	129	54	0.00%	0.000%
54	6.915	1731	1734	1736	rBV2	271	161	0.01%	0.001%
55	6.951	1742	1745	1746	rBV2	276	143	0.01%	0.001%
56	7.015	1763	1765	1768	rBV	148	94	0.00%	0.001%
57	7.044	1768	1774	1784	rVV3	723	1160	0.06%	0.008%
58	7.153	1803	1808	1810	rBV2	161	151	0.01%	0.001%
59	7.192	1812	1820	1826	rVB3	543	899	0.05%	0.006%
60	7.340	1863	1866	1870	rBV2	252	170	0.01%	0.001%
61	7.436	1893	1896	1899	rBV3	293	189	0.01%	0.001%
62	7.574	1925	1939	1962	rBV	238635	416386	21.43%	2.862%
63	7.777	1998	2002	2003	rBV2	147	94	0.00%	0.001%
64	7.906	2024	2042	2056	rBV	892551	1514599	77.94%	10.409%
65	8.131	2107	2112	2114	rBV2	322	301	0.02%	0.002%
66	8.185	2117	2129	2149	rBV	167693	280140	14.42%	1.925%
67	8.365	2180	2185	2187	rBV2	252	268	0.01%	0.002%
68	8.446	2208	2210	2212	rBV2	239	123	0.01%	0.001%
69	8.468	2214	2217	2220	rBV3	229	186	0.01%	0.001%
70	8.510	2228	2230	2232	rBV	182	98	0.01%	0.001%
71	8.562	2242	2246	2249	rBV4	287	180	0.01%	0.001%
72	8.639	2256	2270	2303	rBV	571397	1020648	52.52%	7.015%
73	8.848	2333	2335	2343	rVB2	388	375	0.02%	0.003%
74	8.877	2343	2344	2347	rBV	217	115	0.01%	0.001%
75	8.896	2347	2350	2353	rBV2	257	191	0.01%	0.001%
76	8.925	2356	2359	2361	rBV	251	194	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043741.D
 Acq On : 14 May 2021 09:24
 Operator : SY/MD
 Sample : VU0514WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis

77	9.115	2415	2418	2423	rBV3	198	198	0.01%	0.001%
78	9.153	2427	2430	2435	rBV2	234	253	0.01%	0.002%
79	9.240	2454	2457	2460	rBV	177	141	0.01%	0.001%
80	9.423	2500	2514	2557	rBV	823358	1356140	69.79%	9.320%
81	9.700	2592	2600	2608	rBV2	1157	1668	0.09%	0.011%
82	9.951	2676	2678	2683	rVB2	210	106	0.01%	0.001%
83	10.160	2740	2743	2746	rBV2	144	99	0.01%	0.001%
84	10.208	2753	2758	2760	rBV2	185	194	0.01%	0.001%
85	10.401	2814	2818	2822	rBV	257	309	0.02%	0.002%
86	10.452	2831	2834	2837	rBV	220	159	0.01%	0.001%
87	10.677	2896	2904	2913	rVB3	5519	7966	0.41%	0.055%
88	10.764	2918	2931	2948	rBV	623409	987530	50.82%	6.787%
89	11.095	3029	3034	3035	rBV2	725	481	0.02%	0.003%
90	11.118	3038	3041	3042	rBV2	835	548	0.03%	0.004%
91	11.211	3065	3070	3074	rBV4	461	521	0.03%	0.004%
92	11.365	3114	3118	3121	rBV3	318	271	0.01%	0.002%
93	11.465	3142	3149	3160	rVB3	3247	5056	0.26%	0.035%
94	11.706	3218	3224	3230	rVB5	2145	2469	0.13%	0.017%
95	11.748	3233	3237	3246	rBV2	1213	1396	0.07%	0.010%
96	11.819	3246	3259	3281	rBV	784012	1220365	62.80%	8.387%
97	12.028	3321	3324	3325	rBV	224	122	0.01%	0.001%
98	12.201	3359	3378	3396	rBV	829520	1325832	68.23%	9.112%
99	12.340	3415	3421	3427	rVB4	1614	1890	0.10%	0.013%
100	13.851	3886	3891	3899	rVB5	1809	2751	0.14%	0.019%




Sum of corrected areas: 14550207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043741.D
Acq On : 14 May 2021 09:24
Operator : SY/MD
Sample : VU0514WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

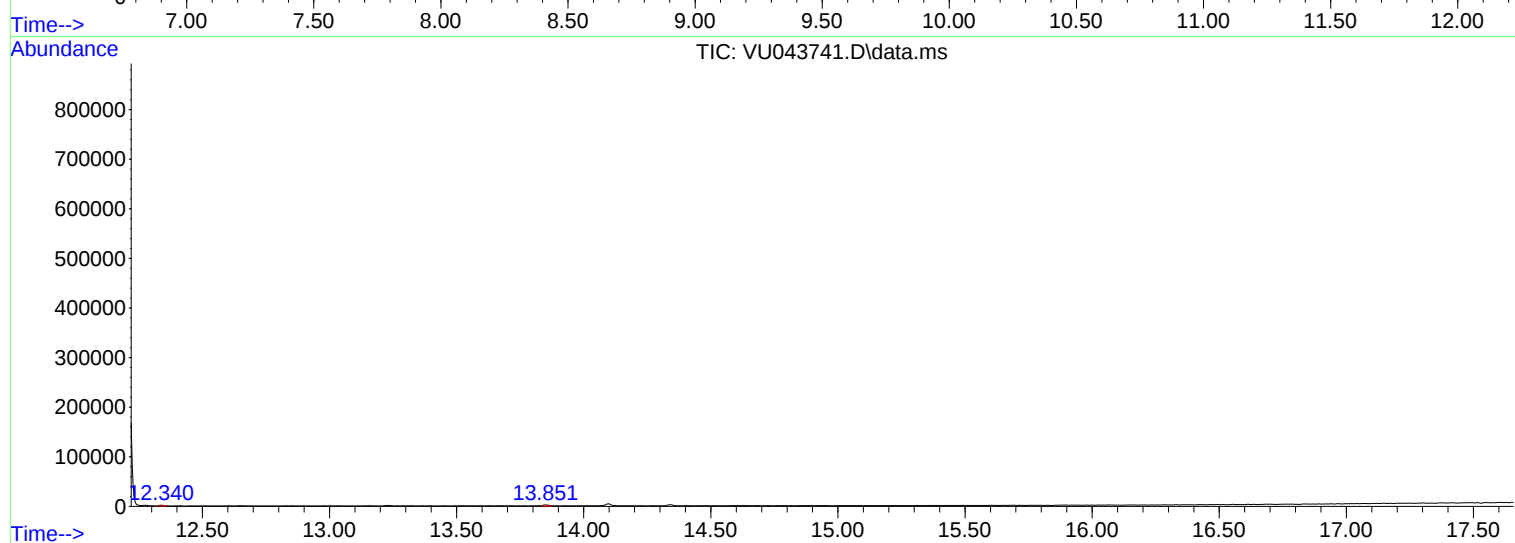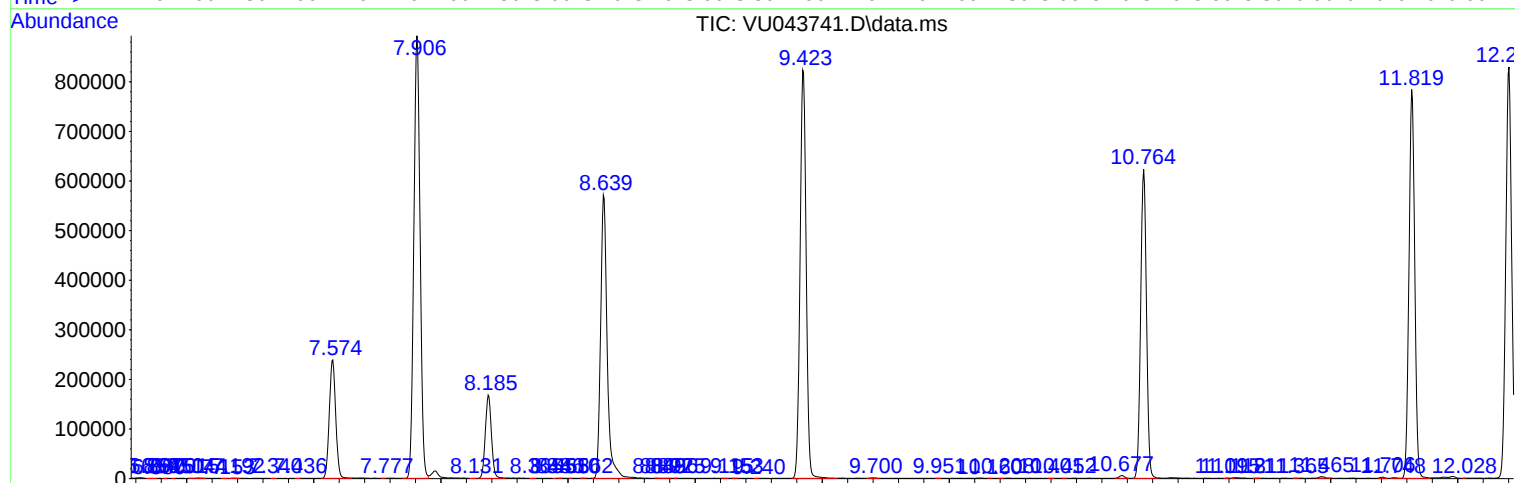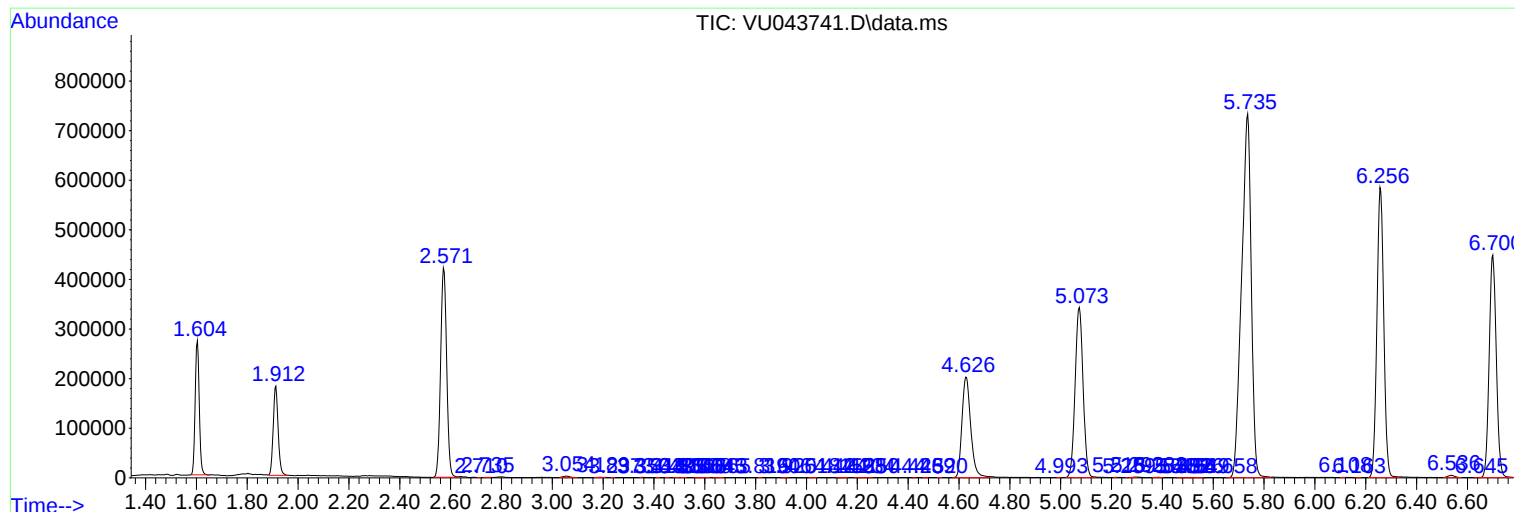

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043741.D
Acq On : 14 May 2021 09:24
Operator : SY/MD
Sample : VU0514WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
Data File : VU043741.D
Acq On : 14 May 2021 09:24
Operator : SY/MD
Sample : VU0514WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
