

m/z	Abundance
35.90	516.0
37.00	2810.0
38.00	2578.0
38.90	1162.0
39.80	268.0
43.90	832.0
44.90	629.0
46.90	899.0
47.90	396.0
48.90	2779.0
50.00	11228.0
51.00	3801.0
51.90	159.0
55.00	150.0
55.90	987.0
57.00	1703.0
59.90	685.0
61.00	3189.0
61.90	3050.0
63.00	2494.0
64.00	513.0
65.00	659.0
66.90	210.0
67.90	6469.0
69.00	6618.0
69.90	557.0
71.80	294.0
72.90	2827.0
73.90	10514.0
75.00	32696.0
76.00	3001.0
76.90	557.0
77.80	330.0
78.90	2003.0
79.90	641.0
80.80	2177.0
81.80	569.0
86.90	3031.0
87.90	2818.0
90.80	193.0
91.90	1796.0
92.90	3091.0
94.00	7126.0
95.00	68408.0
95.90	4396.0
96.90	112.0
103.80	260.0
105.90	291.0
115.70	204.0
116.80	448.0
117.80	188.0
118.80	442.0
127.90	229.0
128.80	141.0
129.90	200.0
130.80	111.0
136.90	141.0
140.80	510.0
142.90	779.0
144.80	361.0
145.80	106.0
147.80	125.0
154.80	189.0
156.70	100.0
170.80	102.0
171.90	1041.0
172.90	569.0
173.90	58680.0
174.90	4336.0
175.90	56272.0
176.90	3784.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
39.70	249.0
43.90	489.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
35.90	503.0
37.00	2747.0
38.00	2532.0
38.90	1087.0
39.80	306.0
43.90	844.0
44.90	570.0
46.90	876.0
47.90	386.0
48.90	2681.0
49.90	11288.0
51.00	3545.0
51.90	110.0
54.90	125.0
55.90	921.0
57.00	1604.0
59.90	710.0
61.00	3098.0
61.90	2919.0
63.00	2301.0
64.00	357.0
65.00	524.0
66.90	158.0
67.90	6101.0
69.00	5961.0
70.00	522.0
71.90	336.0
73.00	2533.0
73.90	9731.0
75.00	30272.0
76.00	2581.0
76.90	524.0
77.90	278.0
78.80	1874.0
79.80	593.0
80.90	1850.0
81.80	481.0
86.00	145.0
86.90	2947.0
87.90	2508.0
90.80	244.0
91.90	1822.0
92.90	2848.0
94.00	6477.0
95.00	63792.0
96.00	4421.0
103.80	233.0
105.80	229.0
115.90	189.0
116.90	392.0
117.90	143.0
118.80	319.0
127.80	148.0
128.70	120.0
129.60	202.0
140.80	410.0
142.90	796.0
144.80	406.0
147.80	191.0
154.80	148.0
170.90	111.0
171.80	784.0
173.90	51376.0
174.90	3832.0
175.90	49184.0
176.90	3410.0

Instrument :
MSVOA_U
ClientSampleId :
BFB165

m/z	Abundance
35.90	527.0
37.00	2903.0
38.00	2677.0
38.90	1147.0
39.80	286.0
43.90	848.0
44.90	643.0
46.90	943.0
47.90	415.0
48.90	2893.0
50.00	11838.0
51.00	3899.0
51.90	126.0
55.00	136.0
55.90	1032.0
57.00	1739.0
59.90	743.0
61.00	3229.0
61.90	3116.0
63.00	2534.0
64.00	455.0
65.00	600.0
66.90	191.0
67.90	6546.0
69.00	6570.0
69.90	547.0
71.90	352.0
73.00	2829.0
73.90	10602.0
75.00	33216.0
76.00	2931.0
76.90	596.0
77.90	304.0
78.90	2013.0
79.80	639.0
80.90	2102.0
81.80	555.0
85.90	116.0
86.90	3141.0
87.90	2876.0
90.80	249.0
91.90	1947.0
92.90	3089.0
94.00	7112.0
95.00	69272.0
96.00	4637.0
96.90	114.0
103.80	250.0
105.90	280.0
115.80	194.0
116.80	461.0
117.90	186.0
118.80	416.0
127.90	189.0
128.70	121.0
129.90	186.0
136.90	130.0
140.80	479.0
142.90	780.0
144.80	414.0
145.70	110.0
147.80	155.0
154.80	170.0
170.90	133.0
171.80	933.0
173.90	57504.0
174.90	4206.0
175.90	55224.0
176.90	3773.0


Instrument :
MSVOA_U
ClientSampleId :
BFB165

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051421\
 Data File : VU043712.D
 Acq On : 13 May 2021 19:46
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB165

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis
 Last Update : Fri May 14 04:42:41 2021

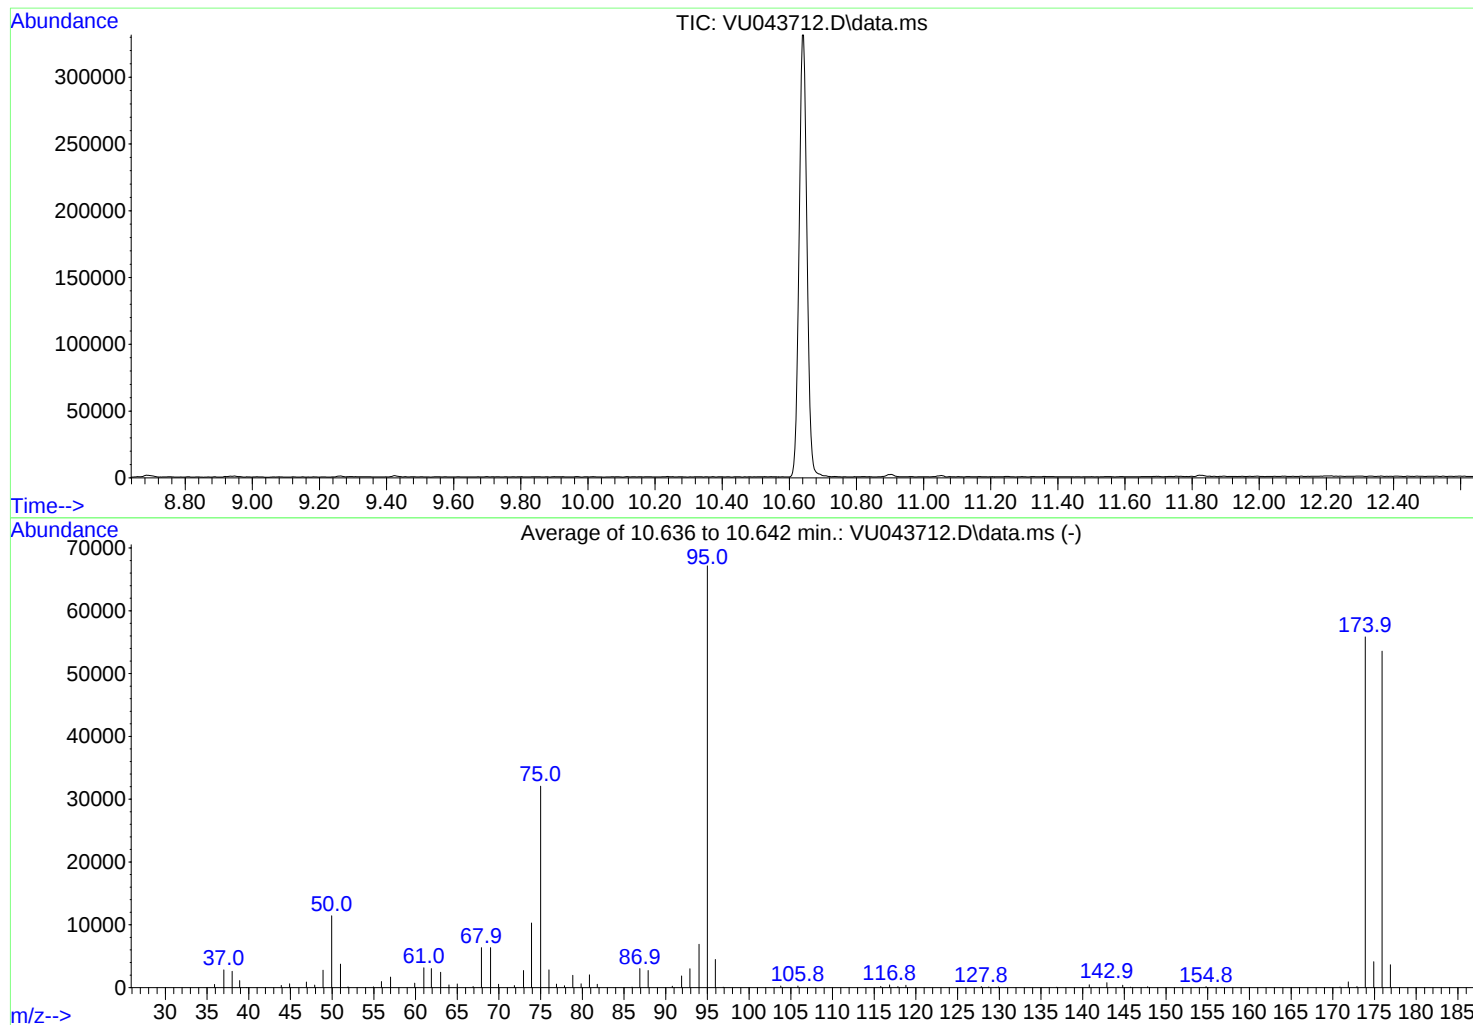

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	11451	PASS
75	95	30	80	47.7	32061	PASS
95	95	100	100	100.0	67157	PASS
96	95	5	9	6.7	4485	PASS
173	174	0.00	2	0.3	190	PASS
174	95	50	120	83.2	55853	PASS
175	174	5	9	7.4	4125	PASS
176	174	95	101	95.9	53560	PASS
177	176	5	9	6.8	3656	PASS