

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032032.D
 Acq On : 15 May 2019 15:21
 Operator : JC/SP
 Sample : K2814-01ME
 Misc : 5.05g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4246ME

Quant Time: May 16 06:35:19 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 16 04:24:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	1197474	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	1183113	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	513183	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	346467	32.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.94%
7) Chloroethane-d5	1.64	69	186001	21.86	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	43.72%#
11) 1,1-Dichloroethene-d2	2.23	63	518810	27.54	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	55.08%#
21) 2-Butanone-d5	4.19	46	682318	92.73	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.73%
24) Chloroform-d	4.64	84	709531	40.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.68%
26) 1,2-Dichloroethane-d4	5.30	65	472818	42.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.36%
32) Benzene-d6	5.33	84	1509441	44.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.14%
36) 1,2-Dichloropropane-d6	6.32	67	512847	45.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.76%
41) Toluene-d8	7.56	98	1302413	42.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.88%
43) trans-1,3-Dichloropropene-	7.85	79	223246	44.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.56%
47) 2-Hexanone-d5	8.32	63	495758	108.18	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.18%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	788980	47.17	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.34%
64) 1,2-Dichlorobenzene-d4	11.86	152	502867	46.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.14%


Target Compounds					Ovalue
13) Acetone	2.34	43	44292	5.855 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032032.D
Acq On : 15 May 2019 15:21
Operator : JC/SP
Sample : K2814-01ME
Misc : 5.05g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4246ME

Quant Time: May 16 06:35:19 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 16 04:24:16 2019
Response via : Initial Calibration

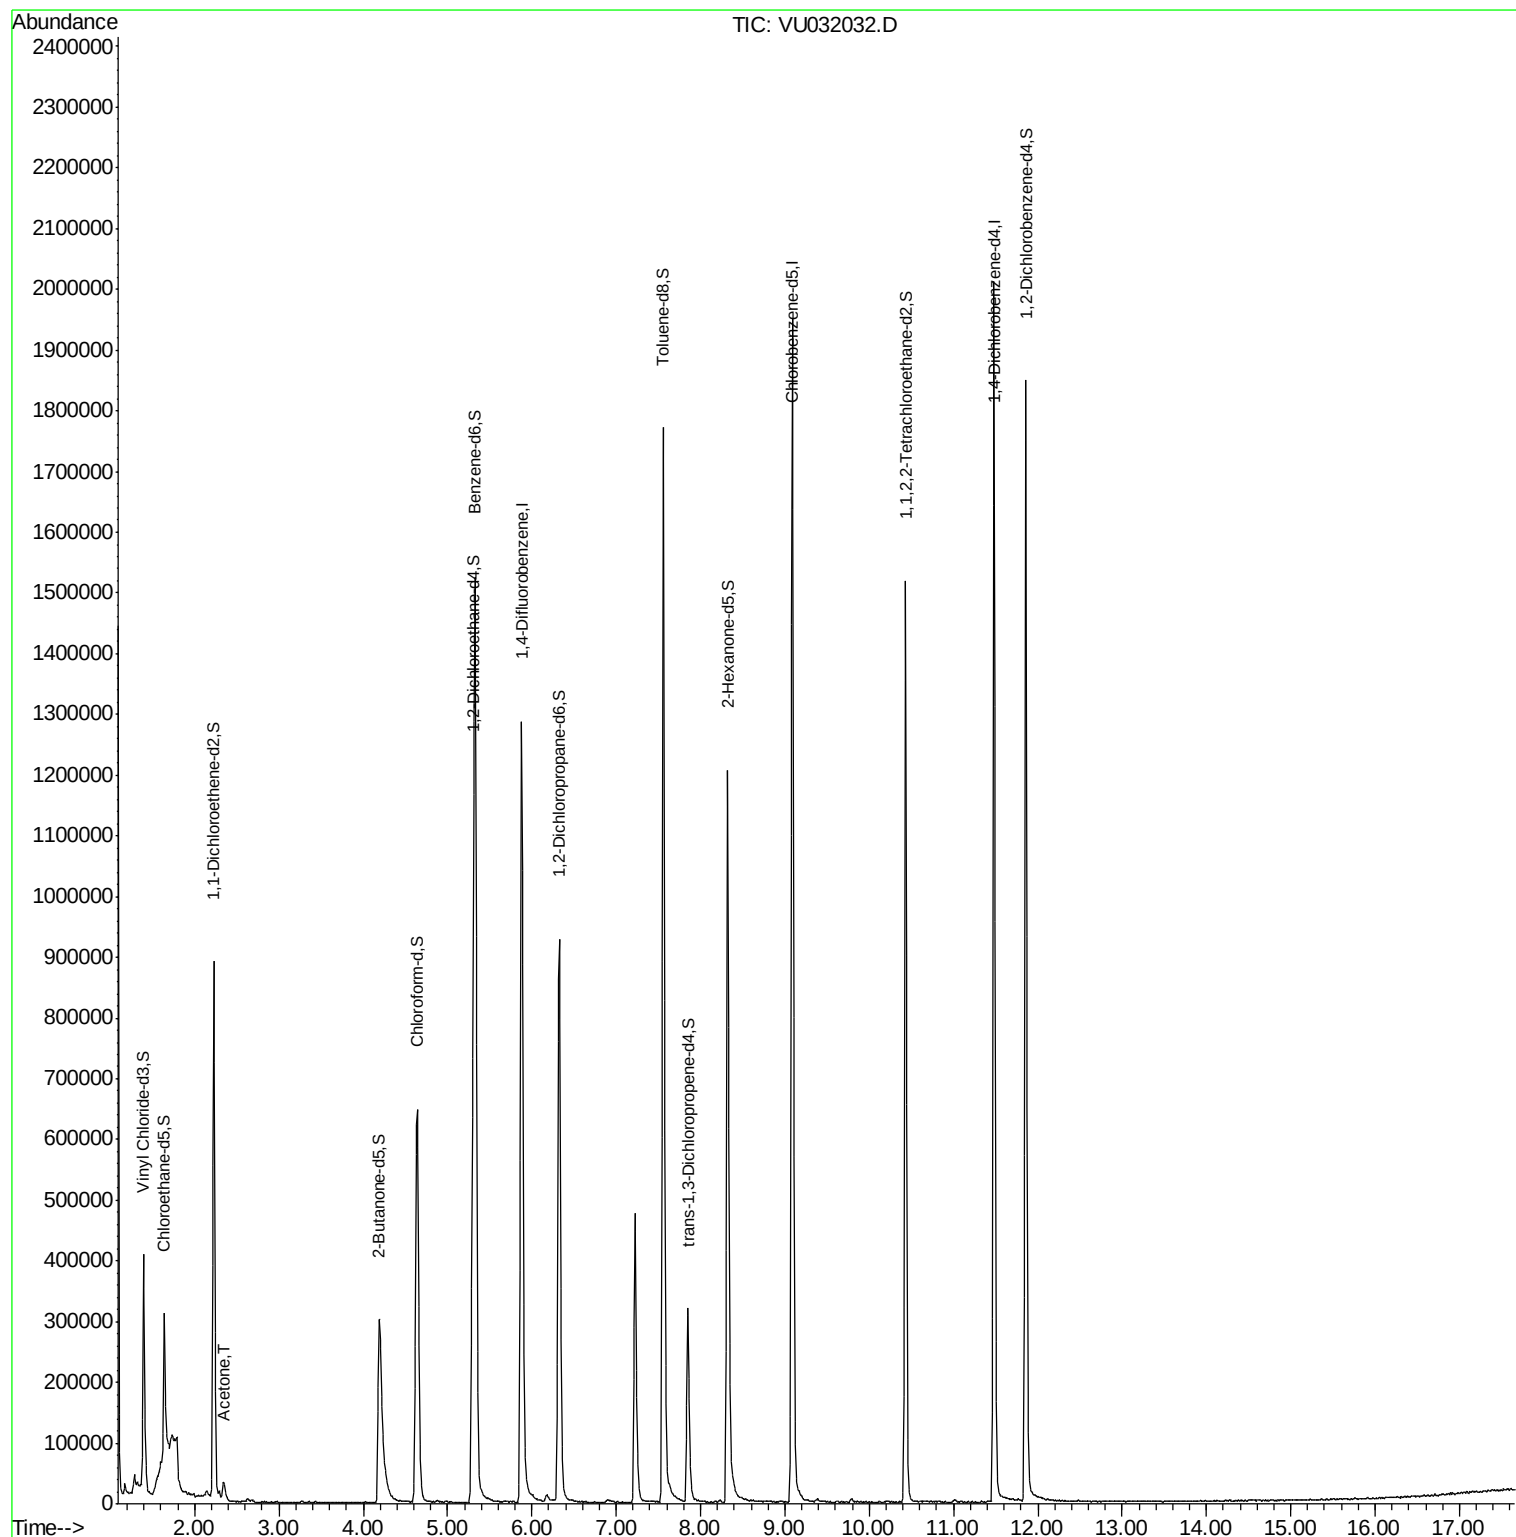

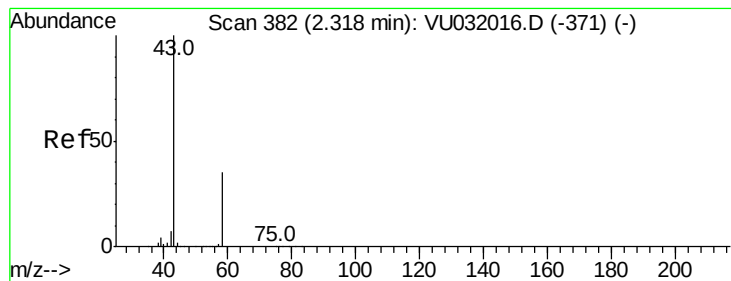

#13
 Acetone
 Concen: 5.855 ug/L
 RT: 2.34 min Scan# 390
 Delta R.T. 0.03 min
 Lab File: VU032032.D
 Acq: 15 May 2019 15:21

Instrument :
 MSVOA_U
 ClientSampleId :
 A4246ME

Tot Ion: 43 Resp: 44292
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 68.2

