

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032021.D
 Acq On : 15 May 2019 11:02
 Operator : JC/SP
 Sample : K2738-11DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB896DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	40	rVB3	18164	19343	0.47%	0.058%
2	1.286	56	61	70	rBV3	25876	31742	0.77%	0.095%
3	1.399	88	96	106	rBV	578176	608635	14.81%	1.827%
4	1.675	174	182	203	rVB	426819	577649	14.05%	1.734%
5	2.267	356	366	381	rBV	937358	1401126	34.09%	4.205%
6	2.444	416	421	430	rBV2	5364	8765	0.21%	0.026%
7	2.521	443	445	449	rVB	1546	1094	0.03%	0.003%
8	2.820	535	538	539	rBV2	1184	565	0.01%	0.002%
9	2.923	567	570	572	rBV3	1323	662	0.02%	0.002%
10	2.981	576	588	605	rBV	59787	113892	2.77%	0.342%
11	3.083	612	620	624	rBV6	1040	1253	0.03%	0.004%
12	3.106	624	627	632	rVB3	882	670	0.02%	0.002%
13	3.145	636	639	643	rBV2	1084	872	0.02%	0.003%
14	3.215	657	661	663	rBV3	1235	905	0.02%	0.003%
15	3.257	671	674	678	rBV2	977	887	0.02%	0.003%
16	3.341	697	700	703	rBV2	835	677	0.02%	0.002%
17	3.402	716	719	723	rVB4	1270	968	0.02%	0.003%
18	3.492	741	747	750	rBV3	845	941	0.02%	0.003%
19	3.572	769	772	778	rVB2	863	735	0.02%	0.002%
20	3.604	780	782	786	rVB2	917	619	0.02%	0.002%
21	3.752	825	828	833	rVB3	709	638	0.02%	0.002%
22	3.817	845	848	851	rBV3	668	523	0.01%	0.002%
23	3.855	857	860	865	rVB4	1030	894	0.02%	0.003%
24	3.884	865	869	871	rBV2	695	537	0.01%	0.002%
25	3.923	878	881	885	rVV2	836	549	0.01%	0.002%
26	4.170	945	958	994	rBV	352319	1021933	24.86%	3.067%
27	4.563	1078	1080	1083	rVB3	1612	858	0.02%	0.003%
28	4.643	1087	1105	1126	rBV	666312	1573607	38.28%	4.722%
29	4.816	1156	1159	1161	rBV3	1132	700	0.02%	0.002%
30	4.939	1194	1197	1201	rBV5	896	867	0.02%	0.003%
31	4.987	1208	1212	1216	rVV4	1953	1742	0.04%	0.005%
32	5.006	1216	1218	1221	rVB3	1375	836	0.02%	0.003%
33	5.058	1231	1234	1239	rVB4	1796	1246	0.03%	0.004%
34	5.083	1239	1242	1246	rBV4	993	730	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032021.D
 Acq On : 15 May 2019 11:02
 Operator : JC/SP
 Sample : K2738-11DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 DB896DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	5.116	1249	1252	1257	rVB5	1180	904	0.02%	0.003%
36	5.215	1280	1283	1288	rVB4	1655	1487	0.04%	0.004%
37	5.241	1288	1291	1294	rBV3	948	636	0.02%	0.002%
38	5.334	1296	1320	1345	rBV2	1387346	4110254	100.00%	12.335%
39	5.813	1465	1469	1473	rVB5	1486	1234	0.03%	0.004%
40	5.881	1473	1490	1519	rBV	1198776	2452339	59.66%	7.359%
41	6.183	1570	1584	1614	rBV	869535	1770272	43.07%	5.313%
42	6.324	1616	1628	1660	rVB	906417	1855449	45.14%	5.568%
43	6.675	1735	1737	1743	rVB5	1847	1498	0.04%	0.004%
44	6.710	1746	1748	1753	rVB5	1070	706	0.02%	0.002%
45	6.775	1764	1768	1772	rBV5	1144	1164	0.03%	0.003%
46	6.839	1785	1788	1792	rVB3	1036	546	0.01%	0.002%
47	6.874	1796	1799	1800	rBV2	1429	739	0.02%	0.002%
48	6.987	1831	1834	1837	rBV3	1187	783	0.02%	0.002%
49	7.006	1837	1840	1842	rVB3	841	568	0.01%	0.002%
50	7.067	1856	1859	1864	rBV3	1121	1033	0.03%	0.003%
51	7.103	1867	1870	1873	rVV2	770	521	0.01%	0.002%
52	7.225	1896	1908	1933	rBV	478433	897898	21.85%	2.695%
53	7.469	1980	1984	1986	rBV4	1420	1060	0.03%	0.003%
54	7.562	2000	2013	2053	rBV	1721160	3229030	78.56%	9.690%
55	7.845	2091	2101	2126	rBV	327204	583034	14.18%	1.750%
56	8.061	2165	2168	2170	rBV	899	587	0.01%	0.002%
57	8.109	2181	2183	2189	rBV5	968	839	0.02%	0.003%
58	8.173	2194	2203	2207	rBV6	3619	4993	0.12%	0.015%
59	8.225	2207	2219	2235	rBV2	285585	513596	12.50%	1.541%
60	8.308	2235	2245	2284	rVV	1024191	1935618	47.09%	5.809%
61	8.739	2375	2379	2382	rBV5	1293	1115	0.03%	0.003%
62	8.765	2385	2387	2391	rVB4	1191	681	0.02%	0.002%
63	8.845	2407	2412	2417	rVB8	1262	1290	0.03%	0.004%
64	8.868	2417	2419	2422	rVB2	1128	595	0.01%	0.002%
65	8.987	2454	2456	2459	rVB2	1114	700	0.02%	0.002%
66	9.032	2465	2470	2474	rBV4	1014	1116	0.03%	0.003%
67	9.086	2474	2487	2535	rVV	1771427	3119557	75.90%	9.362%
68	9.373	2572	2576	2577	rBV3	992	750	0.02%	0.002%
69	9.437	2594	2596	2601	rVB3	1300	662	0.02%	0.002%
70	9.459	2601	2603	2605	rBV3	970	546	0.01%	0.002%
71	9.636	2654	2658	2659	rBV3	1215	865	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032021.D
 Acq On : 15 May 2019 11:02
 Operator : JC/SP
 Sample : K2738-11DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB896DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	9.688	2670	2674	2676	rBV4	872	842	0.02%	0.003%
73	9.720	2680	2684	2687	rBV2	1337	1007	0.02%	0.003%
74	9.829	2714	2718	2721	rBV2	1048	1091	0.03%	0.003%
75	9.845	2721	2723	2726	rVB2	1258	786	0.02%	0.002%
76	9.871	2726	2731	2732	rBV2	1290	928	0.02%	0.003%
77	9.935	2748	2751	2757	rBV4	1382	1237	0.03%	0.004%
78	9.980	2763	2765	2768	rVB2	956	537	0.01%	0.002%
79	10.029	2774	2780	2781	rBV2	743	799	0.02%	0.002%
80	10.106	2801	2804	2806	rBV3	1096	764	0.02%	0.002%
81	10.212	2835	2837	2840	rVB3	1059	620	0.02%	0.002%
82	10.373	2883	2887	2890	rBV2	745	707	0.02%	0.002%
83	10.427	2891	2904	2940	rBV	1244722	2053576	49.96%	6.163%
84	10.578	2941	2951	2975	rBV6	31818	90075	2.19%	0.270%
85	11.080	3103	3107	3112	rVB5	3772	3663	0.09%	0.011%
86	11.392	3201	3204	3205	rBV2	1470	806	0.02%	0.002%
87	11.479	3219	3231	3255	rBV	1547652	2554216	62.14%	7.665%
88	11.762	3310	3319	3332	rBV6	10121	18939	0.46%	0.057%
89	11.855	3335	3348	3381	rBV	1650459	2703408	65.77%	8.113%
90	12.109	3425	3427	3431	rBV3	1632	1423	0.03%	0.004%
91	12.231	3461	3465	3469	rBV6	2198	1946	0.05%	0.006%
92	12.450	3530	3533	3536	rBV4	1539	1404	0.03%	0.004%
93	12.594	3572	3578	3579	rBV4	1910	1748	0.04%	0.005%
94	12.839	3651	3654	3662	rBV7	1469	1921	0.05%	0.006%
95	12.964	3690	3693	3694	rBV3	1132	685	0.02%	0.002%
96	13.260	3782	3785	3786	rBV2	1123	732	0.02%	0.002%
97	13.366	3813	3818	3821	rBV4	1506	1423	0.03%	0.004%
98	14.205	4076	4079	4085	rBV5	1758	1661	0.04%	0.005%
99	14.806	4264	4266	4271	rVB3	1943	1298	0.03%	0.004%
100	15.192	4383	4386	4389	rBV3	1837	1573	0.04%	0.005%


Sum of corrected areas: 33322140

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032021.D
Acq On : 15 May 2019 11:02
Operator : JC/SP
Sample : K2738-11DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB896DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

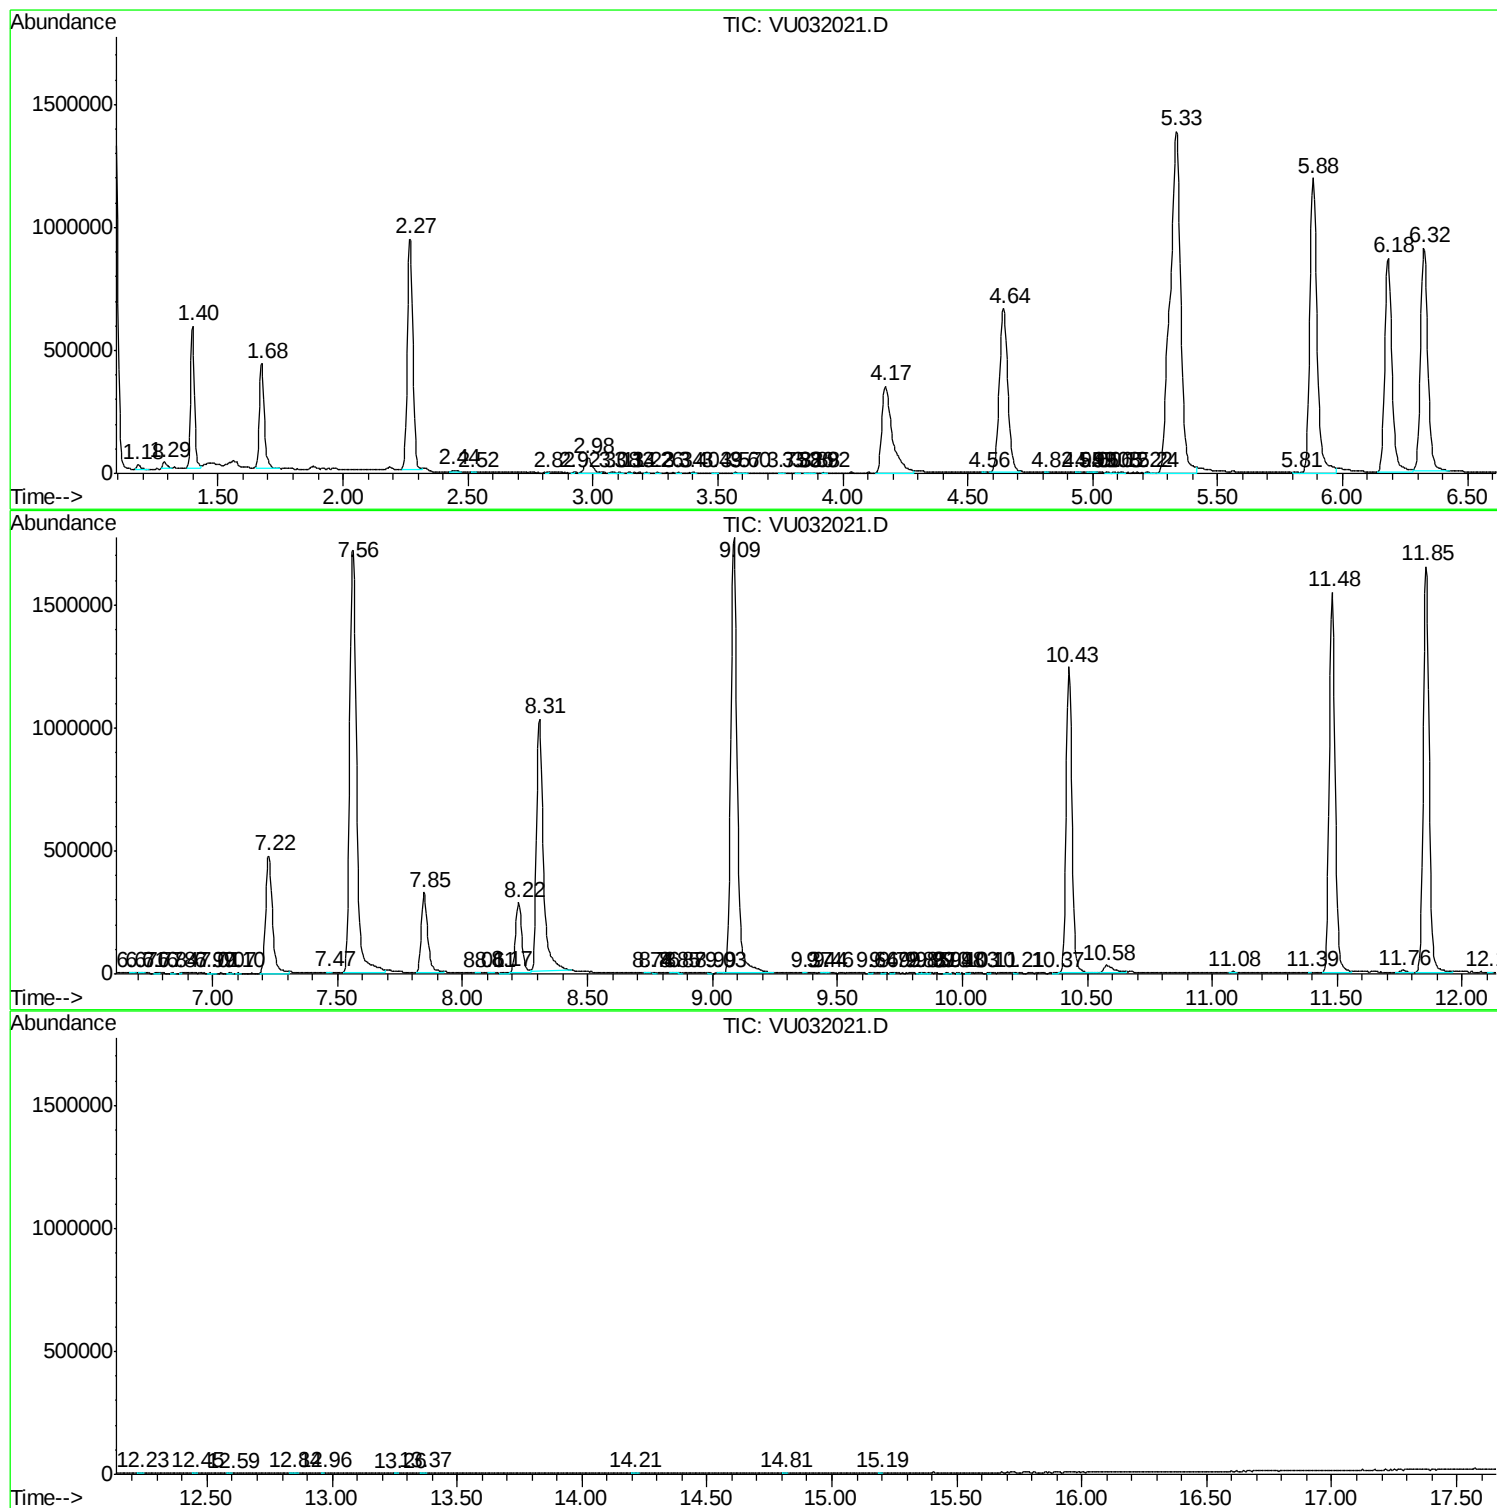

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032021.D
Acq On : 15 May 2019 11:02
Operator : JC/SP
Sample : K2738-11DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB896DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032021.D
Acq On : 15 May 2019 11:02
Operator : JC/SP
Sample : K2738-11DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB896DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc