

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032028.D
 Acq On : 15 May 2019 13:47
 Operator : JC/SP
 Sample : K2738-07DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB890DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	39	rVB2	18248	17145	0.42%	0.051%
2	1.396	88	95	107	rBV	559613	589463	14.28%	1.747%
3	1.672	173	181	197	rVB	426693	559389	13.55%	1.658%
4	2.267	355	366	380	rBV	915949	1381497	33.46%	4.094%
5	2.605	466	471	473	rBV4	800	754	0.02%	0.002%
6	2.646	481	484	487	rVB2	1173	752	0.02%	0.002%
7	2.759	517	519	525	rVB5	1038	727	0.02%	0.002%
8	2.913	563	567	572	rBV2	606	694	0.02%	0.002%
9	2.939	573	575	578	rVV4	890	586	0.01%	0.002%
10	2.984	580	589	600	rVB7	7373	13670	0.33%	0.041%
11	3.103	622	626	628	rBV3	792	618	0.01%	0.002%
12	3.158	640	643	646	rVB2	1090	579	0.01%	0.002%
13	3.196	653	655	659	rVV2	933	665	0.02%	0.002%
14	3.232	661	666	669	rBV3	1129	867	0.02%	0.003%
15	3.379	708	712	715	rBV4	1116	934	0.02%	0.003%
16	3.505	746	751	754	rBV4	944	861	0.02%	0.003%
17	3.566	766	770	773	rBV3	815	725	0.02%	0.002%
18	3.585	773	776	779	rVV2	870	686	0.02%	0.002%
19	3.630	787	790	793	rVV4	1042	766	0.02%	0.002%
20	3.740	821	824	829	rVB3	679	587	0.01%	0.002%
21	3.772	829	834	838	rBV3	1087	1105	0.03%	0.003%
22	3.826	844	851	857	rVB5	832	1115	0.03%	0.003%
23	3.888	865	870	876	rVB3	852	1079	0.03%	0.003%
24	3.920	876	880	883	rBV2	727	568	0.01%	0.002%
25	4.048	917	920	924	rVB2	777	555	0.01%	0.002%
26	4.074	924	928	931	rBV3	1324	1460	0.04%	0.004%
27	4.170	946	958	1001	rBV	379688	1045090	25.31%	3.097%
28	4.511	1061	1064	1066	rBV3	901	616	0.01%	0.002%
29	4.547	1073	1075	1080	rBV4	1332	1195	0.03%	0.004%
30	4.643	1088	1105	1132	rBV	656362	1568547	37.99%	4.648%
31	4.839	1163	1166	1168	rBV3	1376	969	0.02%	0.003%
32	4.971	1205	1207	1210	rBV2	1405	915	0.02%	0.003%
33	4.997	1210	1215	1221	rVB6	1878	1961	0.05%	0.006%
34	5.042	1226	1229	1233	rVB3	834	667	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032028.D
 Acq On : 15 May 2019 13:47
 Operator : JC/SP
 Sample : K2738-07DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 DB890DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	5.087	1240	1243	1245	rBV2	817	519	0.01%	0.002%
36	5.170	1268	1269	1273	rVB2	1313	716	0.02%	0.002%
37	5.196	1273	1277	1278	rBV3	1141	798	0.02%	0.002%
38	5.244	1287	1292	1293	rBV3	828	758	0.02%	0.002%
39	5.334	1294	1320	1360	rBV2	1392489	4129223	100.00%	12.235%
40	5.746	1445	1448	1450	rBV4	1379	1012	0.02%	0.003%
41	5.775	1455	1457	1459	rBV3	1101	647	0.02%	0.002%
42	5.881	1477	1490	1521	rBV	1212679	2483374	60.14%	7.358%
43	6.183	1570	1584	1612	rBV2	288981	612841	14.84%	1.816%
44	6.325	1615	1628	1651	rVV2	904936	1828165	44.27%	5.417%
45	6.730	1751	1754	1757	rVV3	951	723	0.02%	0.002%
46	6.891	1798	1804	1805	rBV3	1507	1440	0.03%	0.004%
47	6.984	1831	1833	1838	rVB3	1248	935	0.02%	0.003%
48	7.071	1856	1860	1863	rBV3	940	698	0.02%	0.002%
49	7.167	1886	1890	1892	rBV3	1001	577	0.01%	0.002%
50	7.225	1895	1908	1932	rBV	474924	880635	21.33%	2.609%
51	7.559	1998	2012	2068	rBV	1775235	3267697	79.14%	9.683%
52	7.846	2090	2101	2125	rBV	324544	578281	14.00%	1.714%
53	8.170	2199	2202	2205	rBV5	1082	1013	0.02%	0.003%
54	8.222	2205	2218	2235	rVV	1194534	2099908	50.85%	6.222%
55	8.305	2235	2244	2292	rVB	1151307	2160300	52.32%	6.401%
56	8.714	2368	2371	2376	rBV3	876	861	0.02%	0.003%
57	8.736	2376	2378	2382	rVB4	1225	686	0.02%	0.002%
58	8.775	2386	2390	2393	rVB3	1599	1243	0.03%	0.004%
59	8.794	2393	2396	2397	rBV3	808	527	0.01%	0.002%
60	8.842	2409	2411	2416	rVB4	1279	677	0.02%	0.002%
61	8.900	2425	2429	2432	rBV5	1368	1196	0.03%	0.004%
62	8.923	2432	2436	2442	rVB6	1177	1589	0.04%	0.005%
63	9.087	2474	2487	2530	rBV	1819805	3161016	76.55%	9.366%
64	9.302	2551	2554	2557	rVB3	1216	695	0.02%	0.002%
65	9.334	2562	2564	2569	rVB3	1116	659	0.02%	0.002%
66	9.392	2580	2582	2585	rVB3	1491	797	0.02%	0.002%
67	9.434	2591	2595	2596	rBV	774	545	0.01%	0.002%
68	9.489	2609	2612	2617	rVB3	899	661	0.02%	0.002%
69	9.566	2634	2636	2639	rBV	1663	1188	0.03%	0.004%
70	9.656	2659	2664	2666	rBV3	1554	1388	0.03%	0.004%
71	9.730	2681	2687	2690	rBV4	681	678	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032028.D
 Acq On : 15 May 2019 13:47
 Operator : JC/SP
 Sample : K2738-07DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB890DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	9.852	2717	2725	2727	rBV6	1140	1429	0.03%	0.004%
73	9.942	2751	2753	2759	rVB4	904	752	0.02%	0.002%
74	9.974	2759	2763	2767	rVB3	1294	1302	0.03%	0.004%
75	10.000	2767	2771	2774	rBV4	866	576	0.01%	0.002%
76	10.038	2780	2783	2788	rBV3	1030	896	0.02%	0.003%
77	10.170	2819	2824	2829	rBV5	1946	1829	0.04%	0.005%
78	10.296	2860	2863	2865	rBV2	922	687	0.02%	0.002%
79	10.308	2865	2867	2871	rVB2	1190	710	0.02%	0.002%
80	10.353	2876	2881	2885	rBV2	1229	1268	0.03%	0.004%
81	10.427	2890	2904	2934	rBV	1267738	2066085	50.04%	6.122%
82	10.595	2947	2956	2968	rBV9	3448	5732	0.14%	0.017%
83	10.746	3000	3003	3004	rBV3	1014	608	0.01%	0.002%
84	10.964	3069	3071	3073	rBV2	1147	703	0.02%	0.002%
85	11.132	3121	3123	3127	rVB3	1331	765	0.02%	0.002%
86	11.173	3133	3136	3141	rBV4	957	798	0.02%	0.002%
87	11.202	3143	3145	3150	rVV2	774	605	0.01%	0.002%
88	11.318	3178	3181	3183	rBV4	874	703	0.02%	0.002%
89	11.479	3218	3231	3257	rBV	1575218	2551922	61.80%	7.562%
90	11.762	3313	3319	3327	rVB5	7471	10606	0.26%	0.031%
91	11.855	3335	3348	3373	rBV	1597205	2669638	64.65%	7.910%
92	12.566	3566	3569	3570	rBV2	1163	555	0.01%	0.002%
93	12.697	3608	3610	3612	rBV3	929	548	0.01%	0.002%
94	12.807	3642	3644	3647	rBV2	1152	689	0.02%	0.002%
95	12.916	3672	3678	3680	rBV4	1239	1239	0.03%	0.004%
96	12.964	3690	3693	3694	rBV2	1660	885	0.02%	0.003%
97	13.459	3844	3847	3852	rBV5	976	805	0.02%	0.002%
98	14.533	4178	4181	4184	rBV	1546	1214	0.03%	0.004%
99	14.810	4264	4267	4271	rBV3	1157	1176	0.03%	0.003%
100	15.717	4547	4549	4551	rBV3	2225	1285	0.03%	0.004%


Sum of corrected areas: 33748483

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032028.D
Acq On : 15 May 2019 13:47
Operator : JC/SP
Sample : K2738-07DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB890DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

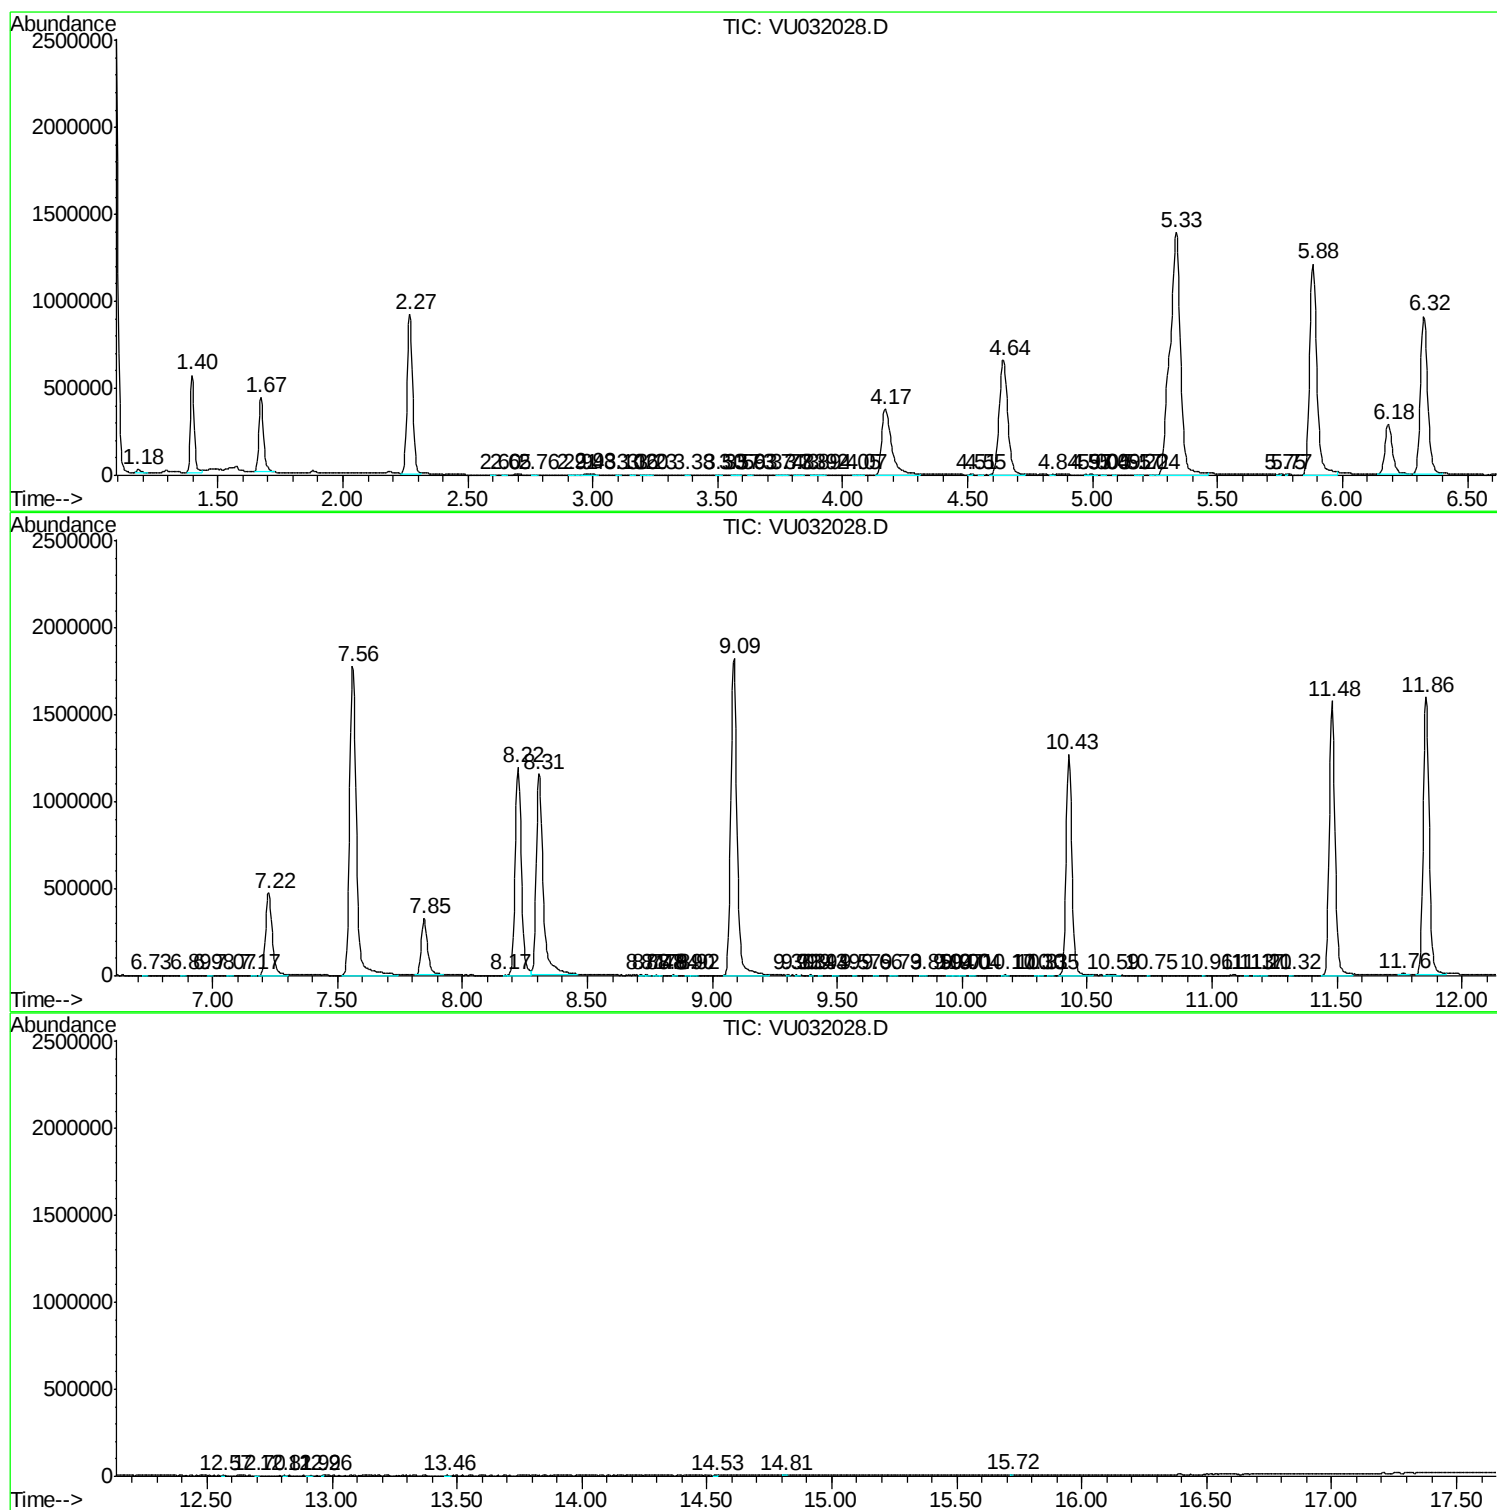

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032028.D
Acq On : 15 May 2019 13:47
Operator : JC/SP
Sample : K2738-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB890DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032028.D
Acq On : 15 May 2019 13:47
Operator : JC/SP
Sample : K2738-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB890DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc