

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032029.D
 Acq On : 15 May 2019 14:10
 Operator : JC/SP
 Sample : K2738-08DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB891DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	35	rVB3	17662	15334	0.38%	0.046%
2	1.396	88	95	107	rBV	566020	595083	14.68%	1.787%
3	1.672	173	181	199	rVB	426578	561379	13.85%	1.686%
4	2.267	355	366	381	rVB	907345	1358507	33.51%	4.079%
5	2.431	414	417	419	rBV3	1383	1055	0.03%	0.003%
6	2.543	449	452	453	rBV3	1289	695	0.02%	0.002%
7	2.698	492	500	511	rBV9	3705	7882	0.19%	0.024%
8	2.743	511	514	518	rVV3	1221	1161	0.03%	0.003%
9	2.769	520	522	525	rVV3	1293	885	0.02%	0.003%
10	2.817	534	537	541	rVV3	522	476	0.01%	0.001%
11	2.926	568	571	577	rVB3	728	706	0.02%	0.002%
12	2.984	580	589	600	rVB4	9024	16785	0.41%	0.050%
13	3.032	600	604	608	rBV4	630	493	0.01%	0.001%
14	3.071	612	616	619	rBV2	954	851	0.02%	0.003%
15	3.145	635	639	641	rVV3	553	500	0.01%	0.002%
16	3.212	656	660	663	rVB2	702	504	0.01%	0.002%
17	3.235	664	667	670	rVB3	784	574	0.01%	0.002%
18	3.347	697	702	708	rVB2	922	977	0.02%	0.003%
19	3.383	708	713	715	rBV4	1315	1084	0.03%	0.003%
20	3.399	716	718	724	rVV3	955	1002	0.02%	0.003%
21	3.486	742	745	747	rVV3	848	612	0.02%	0.002%
22	3.514	751	754	759	rVB4	807	717	0.02%	0.002%
23	3.582	772	775	780	rBV4	747	621	0.02%	0.002%
24	3.650	794	796	800	rVB3	873	501	0.01%	0.002%
25	3.675	800	804	807	rBV2	630	496	0.01%	0.001%
26	3.759	824	830	834	rBV2	904	784	0.02%	0.002%
27	3.804	838	844	846	rVB3	654	582	0.01%	0.002%
28	3.974	893	897	901	rBV3	617	658	0.02%	0.002%
29	4.170	944	958	995	rBV	376120	1033730	25.50%	3.104%
30	4.643	1087	1105	1130	rBV	654362	1554437	38.34%	4.667%
31	4.862	1171	1173	1176	rBV2	1069	694	0.02%	0.002%
32	5.228	1283	1287	1294	rBV6	1252	1332	0.03%	0.004%
33	5.334	1296	1320	1351	rBV2	1360169	4054489	100.00%	12.174%
34	5.694	1429	1432	1436	rVB5	1643	1065	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032029.D
 Acq On : 15 May 2019 14:10
 Operator : JC/SP
 Sample : K2738-08DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 DB891DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	5.720	1438	1440	1444	rVB4	1334	703	0.02%	0.002%
36	5.820	1469	1471	1476	rVB3	1126	732	0.02%	0.002%
37	5.881	1476	1490	1528	rBV	1210202	2505850	61.80%	7.524%
38	6.183	1572	1584	1613	rVB3	279364	578008	14.26%	1.735%
39	6.325	1615	1628	1660	rVV	894595	1809391	44.63%	5.433%
40	6.643	1725	1727	1732	rVB4	1464	1135	0.03%	0.003%
41	6.749	1757	1760	1766	rVB4	983	853	0.02%	0.003%
42	6.788	1769	1772	1774	rVB2	968	575	0.01%	0.002%
43	6.807	1774	1778	1780	rBV	850	613	0.02%	0.002%
44	6.829	1783	1785	1789	rVB4	1125	675	0.02%	0.002%
45	6.862	1792	1795	1800	rBV4	986	857	0.02%	0.003%
46	6.942	1818	1820	1825	rVB3	918	530	0.01%	0.002%
47	6.968	1825	1828	1831	rBV2	819	724	0.02%	0.002%
48	7.000	1835	1838	1844	rVB4	1572	1488	0.04%	0.004%
49	7.032	1844	1848	1850	rBV4	1168	924	0.02%	0.003%
50	7.112	1871	1873	1877	rVB2	881	574	0.01%	0.002%
51	7.225	1896	1908	1939	rBV	463970	870646	21.47%	2.614%
52	7.508	1994	1996	1999	rBV3	836	665	0.02%	0.002%
53	7.563	1999	2013	2035	rBV	1708057	3137833	77.39%	9.421%
54	7.845	2090	2101	2134	rBV	321273	573748	14.15%	1.723%
55	8.222	2202	2218	2235	rBV	1140762	2010635	49.59%	6.037%
56	8.308	2235	2245	2291	rVB	1112002	2150469	53.04%	6.457%
57	8.759	2383	2385	2390	rBV4	730	714	0.02%	0.002%
58	8.845	2409	2412	2417	rVB5	1758	1427	0.04%	0.004%
59	8.919	2432	2435	2439	rVB4	938	725	0.02%	0.002%
60	8.997	2457	2459	2464	rVB2	1232	588	0.01%	0.002%
61	9.087	2473	2487	2527	rBV	1801873	3159800	77.93%	9.487%
62	9.472	2604	2607	2609	rBV3	896	531	0.01%	0.002%
63	9.585	2639	2642	2646	rVB3	1136	892	0.02%	0.003%
64	9.611	2646	2650	2653	rBV4	794	847	0.02%	0.003%
65	9.746	2687	2692	2694	rBV3	1145	967	0.02%	0.003%
66	9.781	2699	2703	2706	rVV3	2107	1706	0.04%	0.005%
67	9.797	2706	2708	2711	rVB3	1388	755	0.02%	0.002%
68	9.820	2711	2715	2717	rBV3	721	587	0.01%	0.002%
69	9.849	2721	2724	2727	rBV2	864	647	0.02%	0.002%
70	9.887	2732	2736	2739	rVB3	1368	837	0.02%	0.003%
71	9.939	2746	2752	2754	rVB5	879	889	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032029.D
 Acq On : 15 May 2019 14:10
 Operator : JC/SP
 Sample : K2738-08DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB891DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	9.996	2768	2770	2773	rBV2	875	530	0.01%	0.002%
73	10.132	2808	2812	2813	rBV3	1014	731	0.02%	0.002%
74	10.222	2838	2840	2843	rBV2	961	704	0.02%	0.002%
75	10.289	2859	2861	2865	rBV3	600	496	0.01%	0.001%
76	10.350	2877	2880	2883	rVB4	888	578	0.01%	0.002%
77	10.369	2883	2886	2889	rBV3	843	651	0.02%	0.002%
78	10.427	2891	2904	2932	rBV	1266996	2059028	50.78%	6.182%
79	10.559	2941	2945	2948	rBV4	1105	850	0.02%	0.003%
80	10.588	2950	2954	2960	rVV7	2090	2587	0.06%	0.008%
81	10.646	2970	2972	2976	rVB4	1601	870	0.02%	0.003%
82	10.672	2976	2980	2981	rBV3	1023	670	0.02%	0.002%
83	10.868	3037	3041	3044	rBV4	1406	1188	0.03%	0.004%
84	10.993	3075	3080	3082	rBV2	1474	1293	0.03%	0.004%
85	11.164	3127	3133	3137	rBV5	1204	1559	0.04%	0.005%
86	11.222	3148	3151	3153	rVB	1014	609	0.02%	0.002%
87	11.238	3153	3156	3159	rBV2	883	597	0.01%	0.002%
88	11.308	3174	3178	3180	rBV3	1450	937	0.02%	0.003%
89	11.353	3190	3192	3199	rVB4	988	719	0.02%	0.002%
90	11.479	3218	3231	3262	rBV	1555347	2548827	62.86%	7.653%
91	11.765	3314	3320	3330	rVB8	5534	8400	0.21%	0.025%
92	11.855	3335	3348	3375	rBV	1541978	2630109	64.87%	7.897%
93	12.469	3536	3539	3544	rBV3	1370	1215	0.03%	0.004%
94	12.598	3575	3579	3581	rBV3	1301	1031	0.03%	0.003%
95	12.665	3598	3600	3604	rBV2	949	850	0.02%	0.003%
96	12.987	3697	3700	3703	rBV2	1470	1204	0.03%	0.004%
97	13.119	3737	3741	3742	rBV2	1634	1216	0.03%	0.004%
98	13.723	3927	3929	3933	rBV2	1068	661	0.02%	0.002%
99	13.755	3937	3939	3941	rBV2	1097	605	0.01%	0.002%
100	14.308	4109	4111	4114	rBV2	1016	605	0.01%	0.002%


Sum of corrected areas: 33305511

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032029.D
Acq On : 15 May 2019 14:10
Operator : JC/SP
Sample : K2738-08DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB891DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

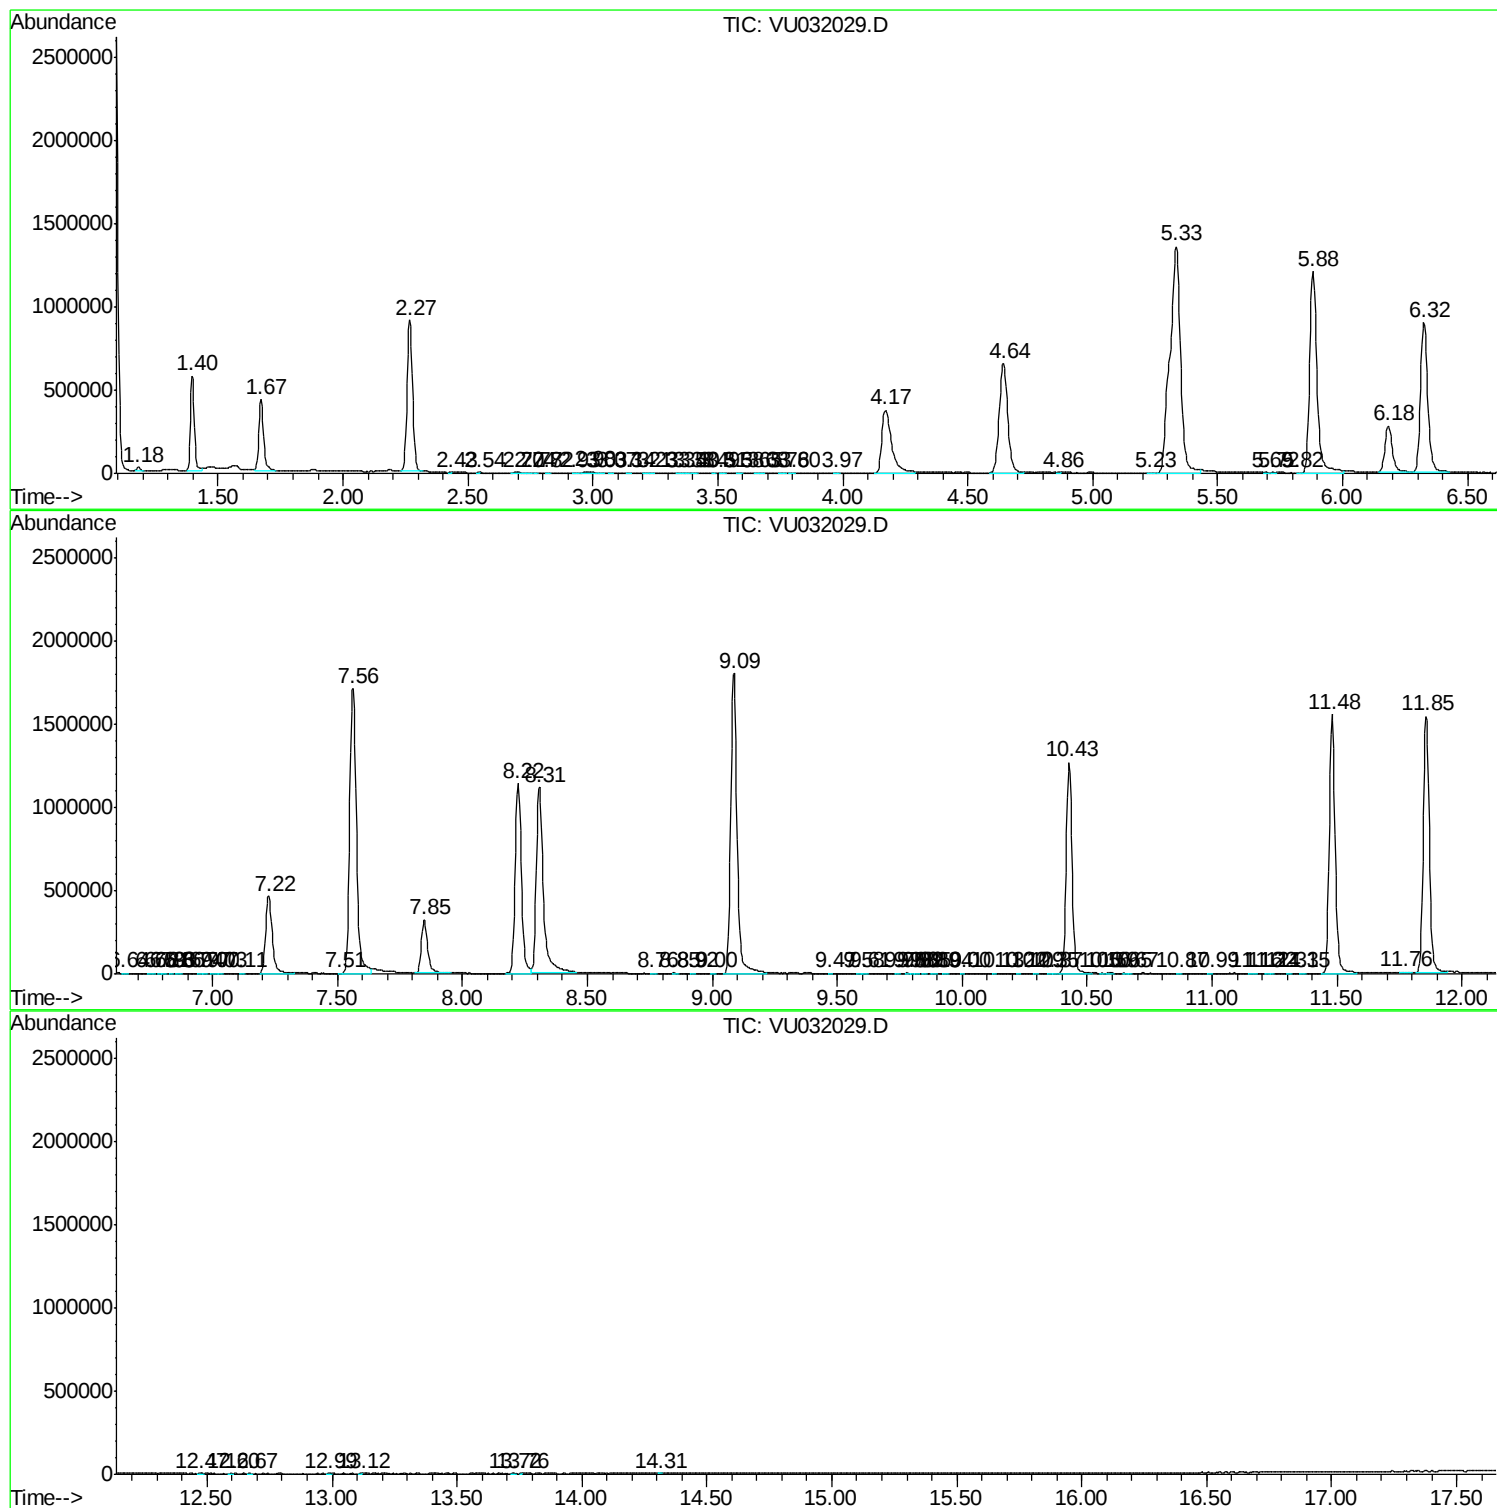

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032029.D
Acq On : 15 May 2019 14:10
Operator : JC/SP
Sample : K2738-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB891DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032029.D
Acq On : 15 May 2019 14:10
Operator : JC/SP
Sample : K2738-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB891DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc