

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032036.D
 Acq On : 15 May 2019 16:56
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB2	19018	16845	0.42%	0.056%
2	1.396	88	95	105	rBV	532162	555231	13.83%	1.835%
3	1.669	172	180	198	rVB	402073	534948	13.32%	1.768%
4	2.267	355	366	379	rVB	860056	1301946	32.42%	4.302%
5	2.441	416	420	421	rBV3	1036	875	0.02%	0.003%
6	2.521	441	445	449	rBV4	1183	771	0.02%	0.003%
7	2.566	455	459	462	rVB3	1332	964	0.02%	0.003%
8	2.588	462	466	467	rBV3	721	596	0.01%	0.002%
9	2.701	497	501	508	rVB4	3305	4203	0.10%	0.014%
10	2.749	512	516	518	rBV4	672	574	0.01%	0.002%
11	2.817	530	537	541	rBV4	1354	1759	0.04%	0.006%
12	2.913	562	567	569	rBV3	1199	1168	0.03%	0.004%
13	3.122	627	632	633	rBV4	817	687	0.02%	0.002%
14	3.296	682	686	692	rVB7	961	1227	0.03%	0.004%
15	3.325	692	695	699	rBV	860	656	0.02%	0.002%
16	3.351	699	703	705	rVB2	1067	724	0.02%	0.002%
17	3.376	705	711	714	rVB2	869	624	0.02%	0.002%
18	3.421	723	725	731	rVB2	886	792	0.02%	0.003%
19	3.463	735	738	745	rBV3	846	836	0.02%	0.003%
20	3.608	779	783	785	rBV2	782	622	0.02%	0.002%
21	3.826	847	851	853	rBV3	695	556	0.01%	0.002%
22	3.862	859	862	865	rVB2	1166	785	0.02%	0.003%
23	3.891	865	871	873	rBV4	702	557	0.01%	0.002%
24	3.907	873	876	878	rBV3	920	650	0.02%	0.002%
25	3.955	886	891	894	rBV4	911	725	0.02%	0.002%
26	4.093	929	934	935	rBV2	964	746	0.02%	0.002%
27	4.170	946	958	1008	rBV	377658	1043030	25.98%	3.447%
28	4.428	1036	1038	1043	rVB3	2377	1876	0.05%	0.006%
29	4.527	1066	1069	1072	rVB3	890	641	0.02%	0.002%
30	4.640	1087	1104	1126	rBV	642580	1533333	38.19%	5.067%
31	4.984	1208	1211	1213	rBV4	1292	861	0.02%	0.003%
32	5.032	1224	1226	1231	rVB3	929	683	0.02%	0.002%
33	5.212	1279	1282	1286	rVB2	1038	663	0.02%	0.002%
34	5.235	1286	1289	1294	rVB3	1205	998	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U051519\
 Data File : VU032036.D
 Acq On : 15 May 2019 16:56
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	5.334	1294	1320	1350	rBV2	1345745	4015462	100.00%	13.270%
36	5.881	1476	1490	1521	rBV	1211474	2459648	61.25%	8.128%
37	6.183	1574	1584	1597	rBV9	25306	58050	1.45%	0.192%
38	6.325	1614	1628	1652	rBV	896263	1805612	44.97%	5.967%
39	6.630	1719	1723	1726	rBV3	1101	959	0.02%	0.003%
40	6.682	1736	1739	1743	rVB4	875	612	0.02%	0.002%
41	6.730	1752	1754	1760	rVB4	1160	790	0.02%	0.003%
42	6.765	1761	1765	1770	rVB6	946	1003	0.02%	0.003%
43	6.820	1778	1782	1786	rVB4	804	833	0.02%	0.003%
44	6.852	1786	1792	1794	rBV2	836	635	0.02%	0.002%
45	6.891	1800	1804	1807	rBV4	979	1045	0.03%	0.003%
46	6.993	1833	1836	1841	rVB5	872	769	0.02%	0.003%
47	7.064	1856	1858	1862	rVB2	980	602	0.01%	0.002%
48	7.161	1884	1888	1890	rBV3	783	590	0.01%	0.002%
49	7.225	1895	1908	1938	rBV	452255	846604	21.08%	2.798%
50	7.415	1965	1967	1974	rVB7	2128	1901	0.05%	0.006%
51	7.559	1999	2012	2066	rBV	1680838	3134615	78.06%	10.359%
52	7.846	2091	2101	2132	rBV	314228	556195	13.85%	1.838%
53	8.067	2166	2170	2172	rBV3	919	635	0.02%	0.002%
54	8.225	2211	2219	2228	rBV9	9682	17021	0.42%	0.056%
55	8.309	2233	2245	2283	rBV	1094568	2099756	52.29%	6.939%
56	8.678	2357	2360	2362	rBV3	1210	1029	0.03%	0.003%
57	8.865	2414	2418	2420	rBV	1320	854	0.02%	0.003%
58	8.894	2424	2427	2429	rVV2	1078	720	0.02%	0.002%
59	9.083	2473	2486	2531	rBV	1782764	3140235	78.20%	10.377%
60	9.376	2573	2577	2578	rBV4	1227	867	0.02%	0.003%
61	9.386	2578	2580	2583	rVB3	1643	868	0.02%	0.003%
62	9.431	2591	2594	2602	rVV6	1442	1570	0.04%	0.005%
63	9.485	2609	2611	2617	rVB4	1778	1192	0.03%	0.004%
64	9.569	2635	2637	2641	rVB2	1503	917	0.02%	0.003%
65	9.591	2641	2644	2646	rBV3	1327	1062	0.03%	0.004%
66	9.730	2682	2687	2689	rBV2	945	829	0.02%	0.003%
67	9.897	2736	2739	2742	rBV2	855	569	0.01%	0.002%
68	9.913	2742	2744	2748	rVB3	1237	652	0.02%	0.002%
69	9.968	2758	2761	2766	rVB2	848	842	0.02%	0.003%
70	10.099	2799	2802	2808	rVB4	699	630	0.02%	0.002%
71	10.321	2867	2871	2874	rBV2	858	645	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032036.D
 Acq On : 15 May 2019 16:56
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	10.357	2878	2882	2888	rVB2	784	637	0.02%	0.002%
73	10.427	2889	2904	2930	rBV	1251543	2044721	50.92%	6.757%
74	10.617	2961	2963	2970	rVB6	946	874	0.02%	0.003%
75	11.141	3121	3126	3128	rBV2	714	671	0.02%	0.002%
76	11.189	3138	3141	3145	rVB2	1180	908	0.02%	0.003%
77	11.222	3145	3151	3152	rBV2	968	851	0.02%	0.003%
78	11.289	3168	3172	3176	rBV4	1029	1234	0.03%	0.004%
79	11.392	3198	3204	3206	rBV4	1142	1398	0.03%	0.005%
80	11.415	3209	3211	3217	rVB7	1709	1548	0.04%	0.005%
81	11.479	3217	3231	3259	rBV	1519032	2490734	62.03%	8.231%
82	11.717	3303	3305	3307	rBV3	1674	995	0.02%	0.003%
83	11.855	3336	3348	3371	rBV	1505889	2527034	62.93%	8.351%
84	12.382	3510	3512	3515	rBV	1122	762	0.02%	0.003%
85	12.456	3533	3535	3537	rVV2	1155	641	0.02%	0.002%
86	12.472	3537	3540	3546	rVV6	1966	1548	0.04%	0.005%
87	12.665	3597	3600	3605	rBV5	1073	960	0.02%	0.003%
88	12.688	3605	3607	3611	rVV5	1044	595	0.01%	0.002%
89	12.874	3661	3665	3666	rBV3	1206	829	0.02%	0.003%
90	13.131	3742	3745	3750	rBV3	1506	1226	0.03%	0.004%
91	13.173	3756	3758	3759	rBV2	1191	577	0.01%	0.002%
92	13.411	3824	3832	3834	rBV7	1498	1937	0.05%	0.006%
93	13.611	3891	3894	3896	rBV2	933	573	0.01%	0.002%
94	13.861	3969	3972	3974	rBV2	1527	1039	0.03%	0.003%
95	14.035	4021	4026	4028	rBV	1564	1475	0.04%	0.005%
96	14.402	4137	4140	4143	rVB2	1327	968	0.02%	0.003%
97	14.495	4166	4169	4175	rBV4	1334	1045	0.03%	0.003%
98	14.569	4189	4192	4198	rVB5	1519	1682	0.04%	0.006%
99	14.607	4198	4204	4207	rBV4	2234	2454	0.06%	0.008%
100	15.279	4409	4413	4415	rBV3	1774	1396	0.03%	0.005%


Sum of corrected areas: 30260282

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032036.D
Acq On : 15 May 2019 16:56
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

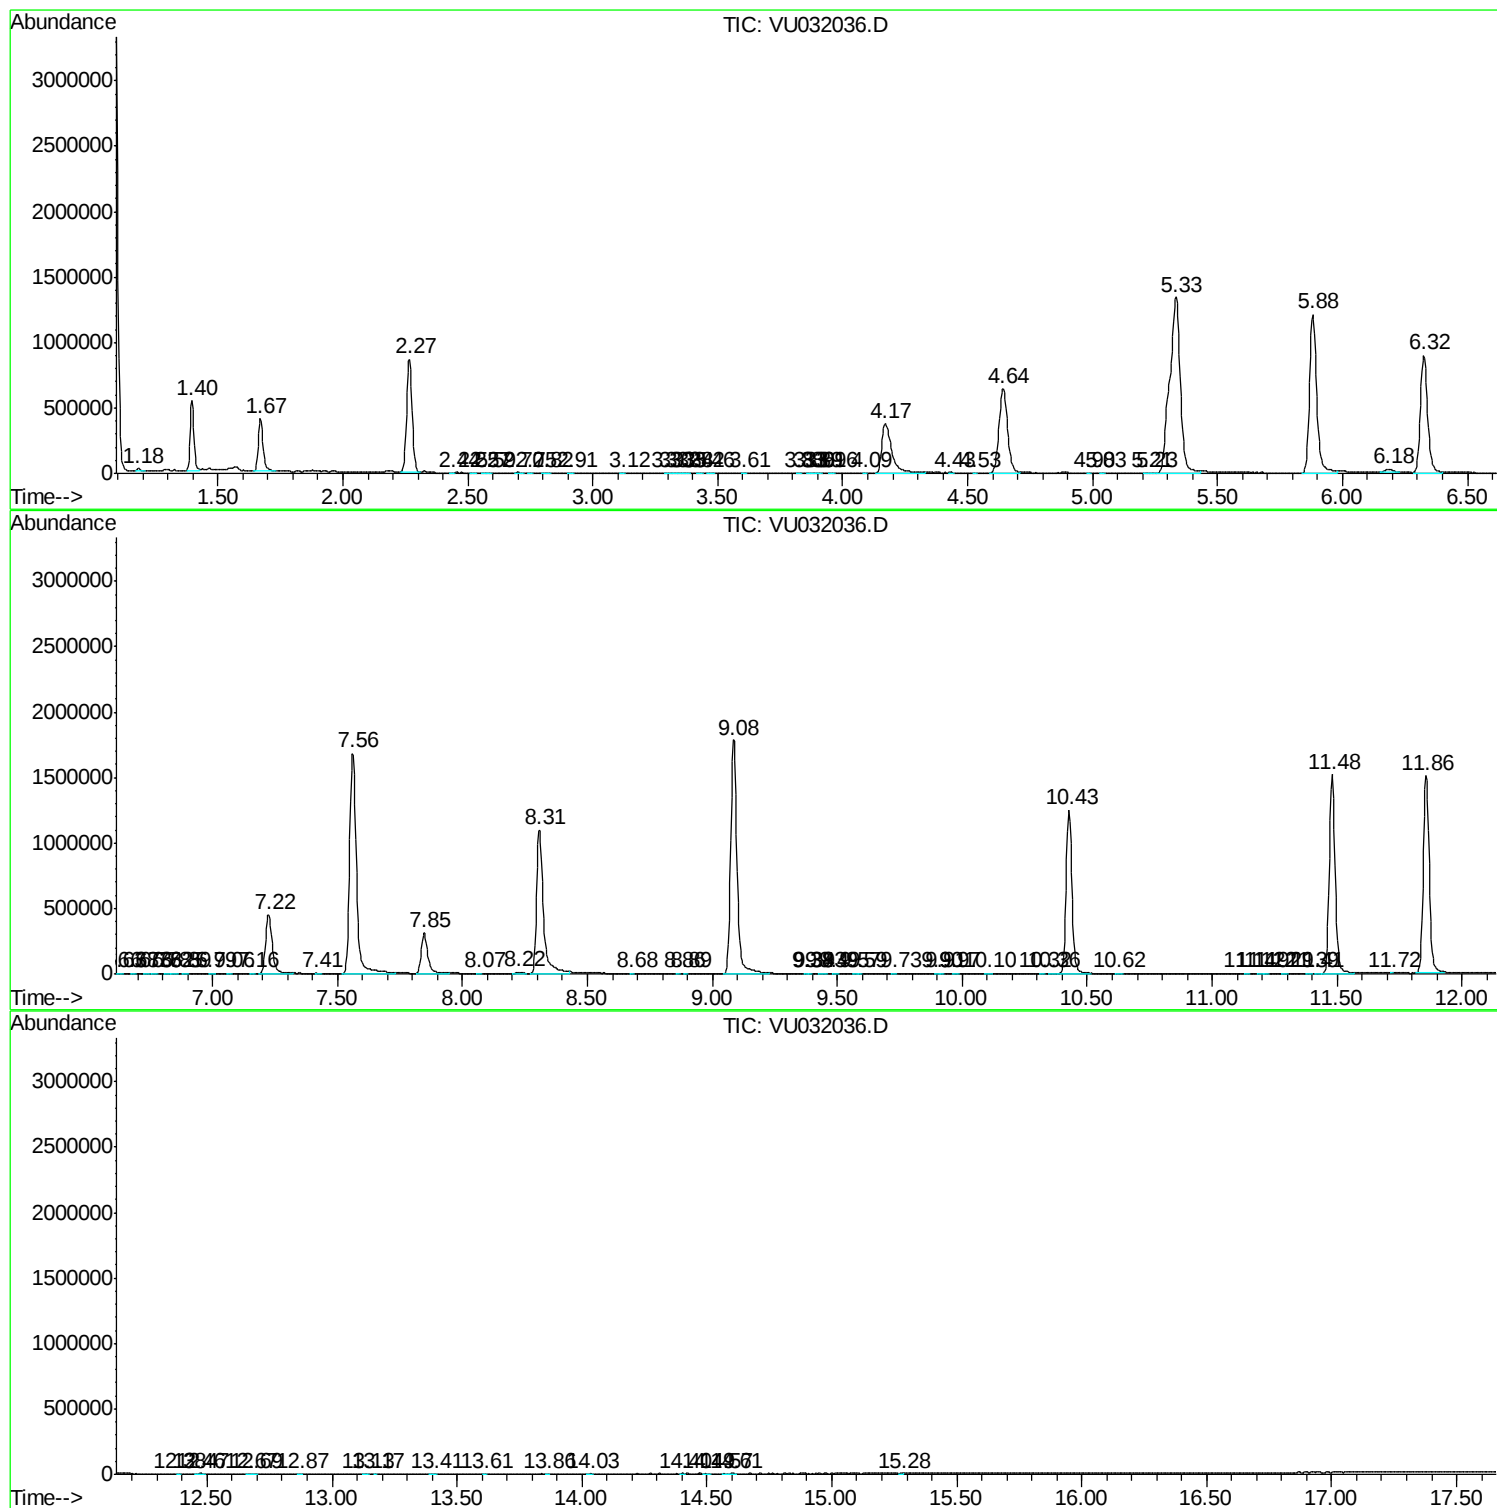

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032036.D
Acq On : 15 May 2019 16:56
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032036.D
Acq On : 15 May 2019 16:56
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc