

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032037.D
 Acq On : 15 May 2019 17:20
 Operator : JC/SP
 Sample : K2738-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB895

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	40	rVB3	22241	22474	0.14%	0.031%
2	1.399	88	96	113	rBV2	4362051	4704736	29.30%	6.538%
3	1.672	173	181	196	rVB	406290	525116	3.27%	0.730%
4	2.270	355	367	380	rBV2	1246422	2215365	13.80%	3.079%
5	2.447	411	422	437	rBV	28508	56672	0.35%	0.079%
6	2.691	492	498	506	rVB8	3083	3896	0.02%	0.005%
7	2.836	531	543	557	rVB4	7390	16463	0.10%	0.023%
8	2.977	570	587	613	rBV	7678614	13999018	87.19%	19.453%
9	3.858	858	861	864	rVV5	1148	832	0.01%	0.001%
10	3.923	879	881	884	rVB	990	526	0.00%	0.001%
11	3.952	884	890	893	rVB5	815	964	0.01%	0.001%
12	4.029	909	914	917	rBV3	864	685	0.00%	0.001%
13	4.096	931	935	938	rVB4	680	619	0.00%	0.001%
14	4.116	938	941	944	rBV	956	648	0.00%	0.001%
15	4.218	947	973	1015	rBV	6227075	16055572	100.00%	22.311%
16	4.643	1090	1105	1129	rVB	621559	1485866	9.25%	2.065%
17	5.090	1240	1244	1248	rBV5	1204	1186	0.01%	0.002%
18	5.151	1261	1263	1268	rVB4	972	672	0.00%	0.001%
19	5.334	1290	1320	1356	rBV2	1338634	3983046	24.81%	5.535%
20	5.742	1444	1447	1450	rBV4	1715	1156	0.01%	0.002%
21	5.759	1450	1452	1456	rVB4	1403	955	0.01%	0.001%
22	5.881	1474	1490	1524	rBV	1213201	2494163	15.53%	3.466%
23	6.180	1568	1583	1616	rBV	4099642	8014682	49.92%	11.137%
24	6.324	1617	1628	1652	rVB	882164	1799262	11.21%	2.500%
25	6.630	1718	1723	1725	rBV5	1988	1995	0.01%	0.003%
26	6.733	1748	1755	1757	rBV5	1309	1218	0.01%	0.002%
27	6.746	1757	1759	1764	rVB3	1529	844	0.01%	0.001%
28	6.797	1772	1775	1779	rBV3	862	782	0.00%	0.001%
29	6.894	1799	1805	1806	rBV4	1081	951	0.01%	0.001%
30	6.945	1819	1821	1826	rVB4	1245	881	0.01%	0.001%
31	7.067	1855	1859	1861	rBV3	1045	798	0.00%	0.001%
32	7.096	1866	1868	1872	rBV4	773	591	0.00%	0.001%
33	7.138	1877	1881	1886	rBV5	1025	970	0.01%	0.001%
34	7.225	1895	1908	1938	rVV	453577	842675	5.25%	1.171%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032037.D
 Acq On : 15 May 2019 17:20
 Operator : JC/SP
 Sample : K2738-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB895

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	7.559	1999	2012	2033	rBV	1671898	3017283	18.79%	4.193%
36	7.845	2090	2101	2126	rBV	305508	551341	3.43%	0.766%
37	8.225	2209	2219	2231	rBV2	38661	68861	0.43%	0.096%
38	8.308	2234	2245	2285	rBV	1010542	1945634	12.12%	2.704%
39	8.842	2409	2411	2415	rVB3	1076	691	0.00%	0.001%
40	8.916	2430	2434	2437	rVB3	1694	1378	0.01%	0.002%
41	8.951	2442	2445	2449	rVB3	1350	1021	0.01%	0.001%
42	8.971	2449	2451	2453	rBV2	1013	609	0.00%	0.001%
43	9.029	2467	2469	2471	rBV2	1487	716	0.00%	0.001%
44	9.086	2473	2487	2535	rVV	1778668	3122398	19.45%	4.339%
45	9.357	2569	2571	2573	rVB2	1376	574	0.00%	0.001%
46	9.479	2607	2609	2613	rVV3	837	621	0.00%	0.001%
47	9.498	2613	2615	2619	rVB3	1169	634	0.00%	0.001%
48	9.524	2619	2623	2625	rBV3	1013	554	0.00%	0.001%
49	9.662	2661	2666	2667	rBV3	694	580	0.00%	0.001%
50	9.691	2672	2675	2677	rVB2	850	511	0.00%	0.001%
51	9.713	2677	2682	2686	rBV5	2125	2006	0.01%	0.003%
52	9.742	2688	2691	2695	rBV5	1079	621	0.00%	0.001%
53	9.855	2724	2726	2729	rVB2	1075	644	0.00%	0.001%
54	9.932	2748	2750	2752	rBV	1112	593	0.00%	0.001%
55	9.945	2752	2754	2758	rVB3	1411	833	0.01%	0.001%
56	9.983	2763	2766	2771	rVB6	885	604	0.00%	0.001%
57	10.019	2771	2777	2778	rBV5	695	513	0.00%	0.001%
58	10.083	2792	2797	2800	rBV3	1375	989	0.01%	0.001%
59	10.164	2819	2822	2825	rBV2	793	612	0.00%	0.001%
60	10.189	2829	2830	2835	rVB3	1018	610	0.00%	0.001%
61	10.215	2835	2838	2839	rBV2	1237	757	0.00%	0.001%
62	10.257	2847	2851	2855	rBV4	1657	1639	0.01%	0.002%
63	10.344	2874	2878	2881	rBV3	717	717	0.00%	0.001%
64	10.379	2885	2889	2890	rBV	1063	780	0.00%	0.001%
65	10.427	2891	2904	2929	rVV	1226009	1976120	12.31%	2.746%
66	10.562	2943	2946	2950	rVV5	1027	585	0.00%	0.001%
67	10.585	2951	2953	2955	rVV2	1149	755	0.00%	0.001%
68	10.604	2955	2959	2968	rVB9	4095	5864	0.04%	0.008%
69	10.646	2968	2972	2974	rBV2	1370	983	0.01%	0.001%
70	10.701	2986	2989	2992	rBV5	785	531	0.00%	0.001%
71	10.729	2995	2998	3001	rBV3	703	667	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032037.D
 Acq On : 15 May 2019 17:20
 Operator : JC/SP
 Sample : K2738-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB895

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	10.836	3029	3031	3034	rVB2	947	528	0.00%	0.001%
73	10.893	3046	3049	3053	rVB2	982	763	0.00%	0.001%
74	10.967	3070	3072	3075	rVB2	1363	819	0.01%	0.001%
75	10.996	3075	3081	3086	rBV4	1155	1728	0.01%	0.002%
76	11.070	3101	3104	3105	rBV2	1408	778	0.00%	0.001%
77	11.189	3136	3141	3143	rBV	918	729	0.00%	0.001%
78	11.260	3159	3163	3167	rBV3	1330	1446	0.01%	0.002%
79	11.376	3196	3199	3201	rBV2	1177	887	0.01%	0.001%
80	11.424	3212	3214	3219	rVB2	1078	802	0.00%	0.001%
81	11.479	3219	3231	3260	rBV	1512509	2467962	15.37%	3.430%
82	11.855	3336	3348	3380	rBV	1508249	2520415	15.70%	3.502%
83	12.205	3455	3457	3463	rVB2	1644	1081	0.01%	0.002%
84	12.405	3516	3519	3522	rBV3	1086	589	0.00%	0.001%
85	12.755	3626	3628	3632	rVB5	1210	819	0.01%	0.001%
86	12.781	3633	3636	3637	rBV	1315	675	0.00%	0.001%
87	12.951	3686	3689	3692	rBV4	1083	629	0.00%	0.001%
88	13.032	3709	3714	3715	rBV3	1217	889	0.01%	0.001%
89	13.099	3733	3735	3738	rBV3	995	810	0.01%	0.001%
90	13.183	3757	3761	3763	rBV2	1361	1256	0.01%	0.002%
91	13.408	3829	3831	3833	rBV2	1371	812	0.01%	0.001%
92	13.524	3865	3867	3870	rVB3	1345	672	0.00%	0.001%
93	13.633	3898	3901	3904	rBV3	1465	810	0.01%	0.001%
94	13.864	3971	3973	3976	rVB2	1222	585	0.00%	0.001%
95	13.887	3977	3980	3984	rBV3	1306	1257	0.01%	0.002%
96	14.012	4014	4019	4022	rBV3	1680	1896	0.01%	0.003%
97	14.099	4042	4046	4050	rBV4	1653	1559	0.01%	0.002%
98	14.363	4125	4128	4132	rBV4	1248	1021	0.01%	0.001%
99	14.607	4199	4204	4208	rBV6	1750	1852	0.01%	0.003%
100	14.768	4252	4254	4258	rBV3	1251	714	0.00%	0.001%


Sum of corrected areas: 71961891

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032037.D
Acq On : 15 May 2019 17:20
Operator : JC/SP
Sample : K2738-10
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
DB895

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

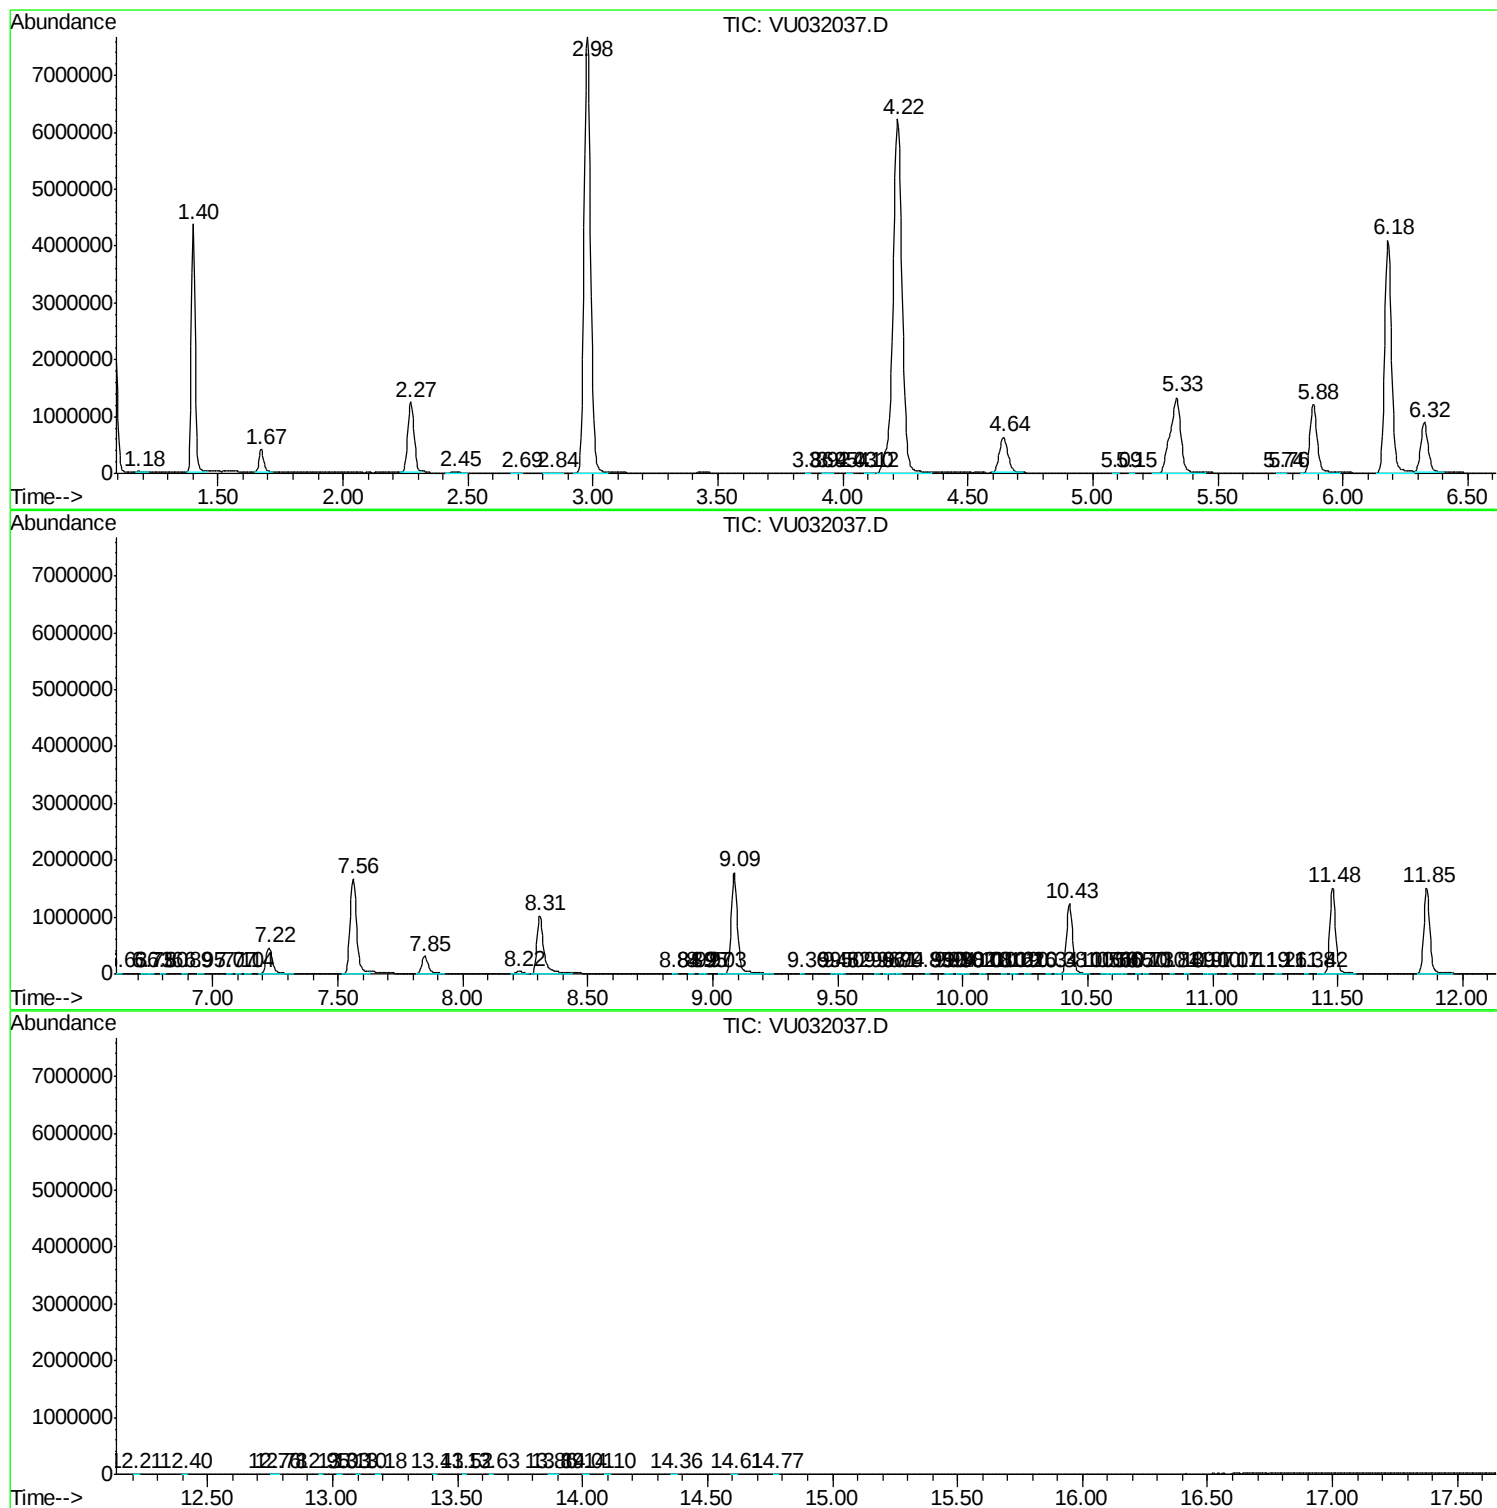

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032037.D
Acq On : 15 May 2019 17:20
Operator : JC/SP
Sample : K2738-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB895

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032037.D
Acq On : 15 May 2019 17:20
Operator : JC/SP
Sample : K2738-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB895

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc