

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032038.D
 Acq On : 15 May 2019 17:44
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	33	rVB2	17043	12872	0.31%	0.041%
2	1.396	88	95	106	rBV	602677	629799	15.16%	2.011%
3	1.669	172	180	197	rVB	435128	574103	13.82%	1.833%
4	2.267	355	366	379	rVB	923334	1400697	33.72%	4.472%
5	2.421	411	414	416	rBV3	934	626	0.02%	0.002%
6	2.511	439	442	445	rBV2	1519	1117	0.03%	0.004%
7	2.559	453	457	464	rBV6	1437	1836	0.04%	0.006%
8	2.624	471	477	480	rBV4	1038	1311	0.03%	0.004%
9	2.653	484	486	489	rVB4	920	551	0.01%	0.002%
10	2.868	547	553	559	rBV5	1056	1486	0.04%	0.005%
11	2.904	559	564	569	rVB4	1172	1452	0.03%	0.005%
12	2.929	569	572	575	rBV2	817	633	0.02%	0.002%
13	2.981	575	588	602	rBV2	24469	47011	1.13%	0.150%
14	3.164	639	645	648	rBV3	1338	1395	0.03%	0.004%
15	3.257	667	674	676	rBV6	1228	1167	0.03%	0.004%
16	3.322	690	694	697	rVB2	775	558	0.01%	0.002%
17	3.367	703	708	709	rBV2	651	593	0.01%	0.002%
18	3.431	723	728	731	rBV2	1030	742	0.02%	0.002%
19	3.743	823	825	830	rVB3	851	570	0.01%	0.002%
20	3.772	832	834	839	rVB4	831	533	0.01%	0.002%
21	3.881	865	868	870	rBV3	882	628	0.02%	0.002%
22	3.961	888	893	895	rBV2	1076	789	0.02%	0.003%
23	4.174	946	959	994	rBV	394006	1083451	26.09%	3.459%
24	4.569	1079	1082	1084	rBV3	1050	886	0.02%	0.003%
25	4.640	1088	1104	1135	rVV	669067	1597026	38.45%	5.098%
26	4.884	1176	1180	1183	rBV5	2398	2050	0.05%	0.007%
27	4.945	1196	1199	1203	rVB5	1306	1084	0.03%	0.003%
28	4.981	1208	1210	1214	rVV3	1095	779	0.02%	0.002%
29	5.039	1225	1228	1230	rBV2	873	517	0.01%	0.002%
30	5.071	1236	1238	1241	rBV3	798	523	0.01%	0.002%
31	5.129	1250	1256	1261	rBV6	1702	2313	0.06%	0.007%
32	5.151	1261	1263	1267	rVB3	1271	779	0.02%	0.002%
33	5.212	1278	1282	1287	rBV5	715	815	0.02%	0.003%
34	5.334	1295	1320	1355	rBV2	1381720	4153350	100.00%	13.259%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032038.D
 Acq On : 15 May 2019 17:44
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

35	5.881	1476	1490	1512	rBV	1225261	2493508	60.04%	7.960%
36	6.186	1574	1585	1600	rBV8	22641	52278	1.26%	0.167%
37	6.325	1614	1628	1660	rBV	928679	1881529	45.30%	6.007%
38	6.836	1783	1787	1792	rBV4	1187	989	0.02%	0.003%
39	6.894	1803	1805	1808	rBV2	849	621	0.01%	0.002%
40	6.939	1815	1819	1823	rBV3	727	769	0.02%	0.002%
41	7.029	1844	1847	1851	rVB3	1158	709	0.02%	0.002%
42	7.119	1869	1875	1880	rVB3	1130	1095	0.03%	0.003%
43	7.148	1880	1884	1886	rBV2	771	595	0.01%	0.002%
44	7.167	1886	1890	1894	rBV6	598	674	0.02%	0.002%
45	7.225	1895	1908	1947	rBV	471804	881867	21.23%	2.815%
46	7.559	1998	2012	2035	rBV	1721324	3157999	76.03%	10.082%
47	7.845	2090	2101	2123	rBV	326830	577431	13.90%	1.843%
48	8.138	2189	2192	2196	rVB4	1731	1114	0.03%	0.004%
49	8.161	2196	2199	2200	rBV3	846	594	0.01%	0.002%
50	8.177	2200	2204	2212	rVB7	2059	2297	0.06%	0.007%
51	8.225	2212	2219	2230	rBV10	4563	6760	0.16%	0.022%
52	8.308	2234	2245	2288	rBV	1110995	2162921	52.08%	6.905%
53	8.833	2405	2408	2410	rBV3	1306	821	0.02%	0.003%
54	8.926	2433	2437	2440	rBV3	1439	1190	0.03%	0.004%
55	8.993	2454	2458	2459	rBV3	1017	673	0.02%	0.002%
56	9.087	2473	2487	2532	rBV	1844654	3217431	77.47%	10.271%
57	9.328	2560	2562	2565	rVB3	1420	685	0.02%	0.002%
58	9.466	2603	2605	2610	rVB4	841	627	0.02%	0.002%
59	9.488	2610	2612	2616	rVB4	1210	847	0.02%	0.003%
60	9.511	2616	2619	2622	rBV3	787	529	0.01%	0.002%
61	9.527	2622	2624	2629	rVB3	1692	1319	0.03%	0.004%
62	9.550	2629	2631	2634	rBV3	882	654	0.02%	0.002%
63	9.624	2652	2654	2659	rVB2	1020	751	0.02%	0.002%
64	9.649	2659	2662	2665	rVB5	996	710	0.02%	0.002%
65	9.800	2705	2709	2711	rBV5	1568	1110	0.03%	0.004%
66	9.855	2722	2726	2728	rBV	967	600	0.01%	0.002%
67	9.871	2728	2731	2734	rBV4	1287	936	0.02%	0.003%
68	10.003	2769	2772	2776	rVB2	1144	916	0.02%	0.003%
69	10.074	2790	2794	2797	rBV3	736	762	0.02%	0.002%
70	10.106	2800	2804	2808	rBV3	913	747	0.02%	0.002%
71	10.193	2828	2831	2837	rVB3	1222	1133	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051519\
 Data File : VU032038.D
 Acq On : 15 May 2019 17:44
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis

72	10.225	2837	2841	2843	rBV3	668	498	0.01%	0.002%
73	10.238	2843	2845	2851	rVB5	772	763	0.02%	0.002%
74	10.360	2877	2883	2885	rBV4	656	642	0.02%	0.002%
75	10.373	2885	2887	2891	rVV3	911	669	0.02%	0.002%
76	10.427	2891	2904	2942	rVV	1275542	2117891	50.99%	6.761%
77	10.640	2968	2970	2975	rVV4	889	560	0.01%	0.002%
78	10.678	2979	2982	2984	rVB3	912	589	0.01%	0.002%
79	10.730	2994	2998	3001	rBV3	1019	701	0.02%	0.002%
80	10.807	3019	3022	3027	rBV4	860	853	0.02%	0.003%
81	10.865	3037	3040	3048	rVB5	1024	1073	0.03%	0.003%
82	10.923	3052	3058	3059	rBV4	1346	1176	0.03%	0.004%
83	10.974	3072	3074	3077	rVB	1132	542	0.01%	0.002%
84	11.006	3082	3084	3087	rVV3	1151	753	0.02%	0.002%
85	11.083	3103	3108	3114	rVB5	1936	1934	0.05%	0.006%
86	11.154	3127	3130	3132	rBV	893	663	0.02%	0.002%
87	11.212	3145	3148	3151	rBV3	722	545	0.01%	0.002%
88	11.479	3217	3231	3257	rBV	1546314	2551287	61.43%	8.145%
89	11.855	3336	3348	3378	rBV	1595439	2651166	63.83%	8.464%
90	12.395	3513	3516	3521	rBV5	1539	1638	0.04%	0.005%
91	12.569	3567	3570	3576	rBV6	1253	1399	0.03%	0.004%
92	12.791	3633	3639	3642	rBV3	1721	1897	0.05%	0.006%
93	12.913	3674	3677	3679	rBV2	1139	776	0.02%	0.002%
94	12.951	3688	3689	3693	rBV3	807	514	0.01%	0.002%
95	13.453	3843	3845	3848	rBV2	1280	773	0.02%	0.002%
96	13.488	3853	3856	3857	rBV2	965	568	0.01%	0.002%
97	13.562	3874	3879	3884	rBV4	1434	1811	0.04%	0.006%
98	13.659	3907	3909	3912	rBV	815	655	0.02%	0.002%
99	14.077	4037	4039	4042	rBV	1000	698	0.02%	0.002%
100	14.482	4161	4165	4168	rBV2	1524	1292	0.03%	0.004%


Sum of corrected areas: 31324559

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051519\
Data File : VU032038.D
Acq On : 15 May 2019 17:44
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

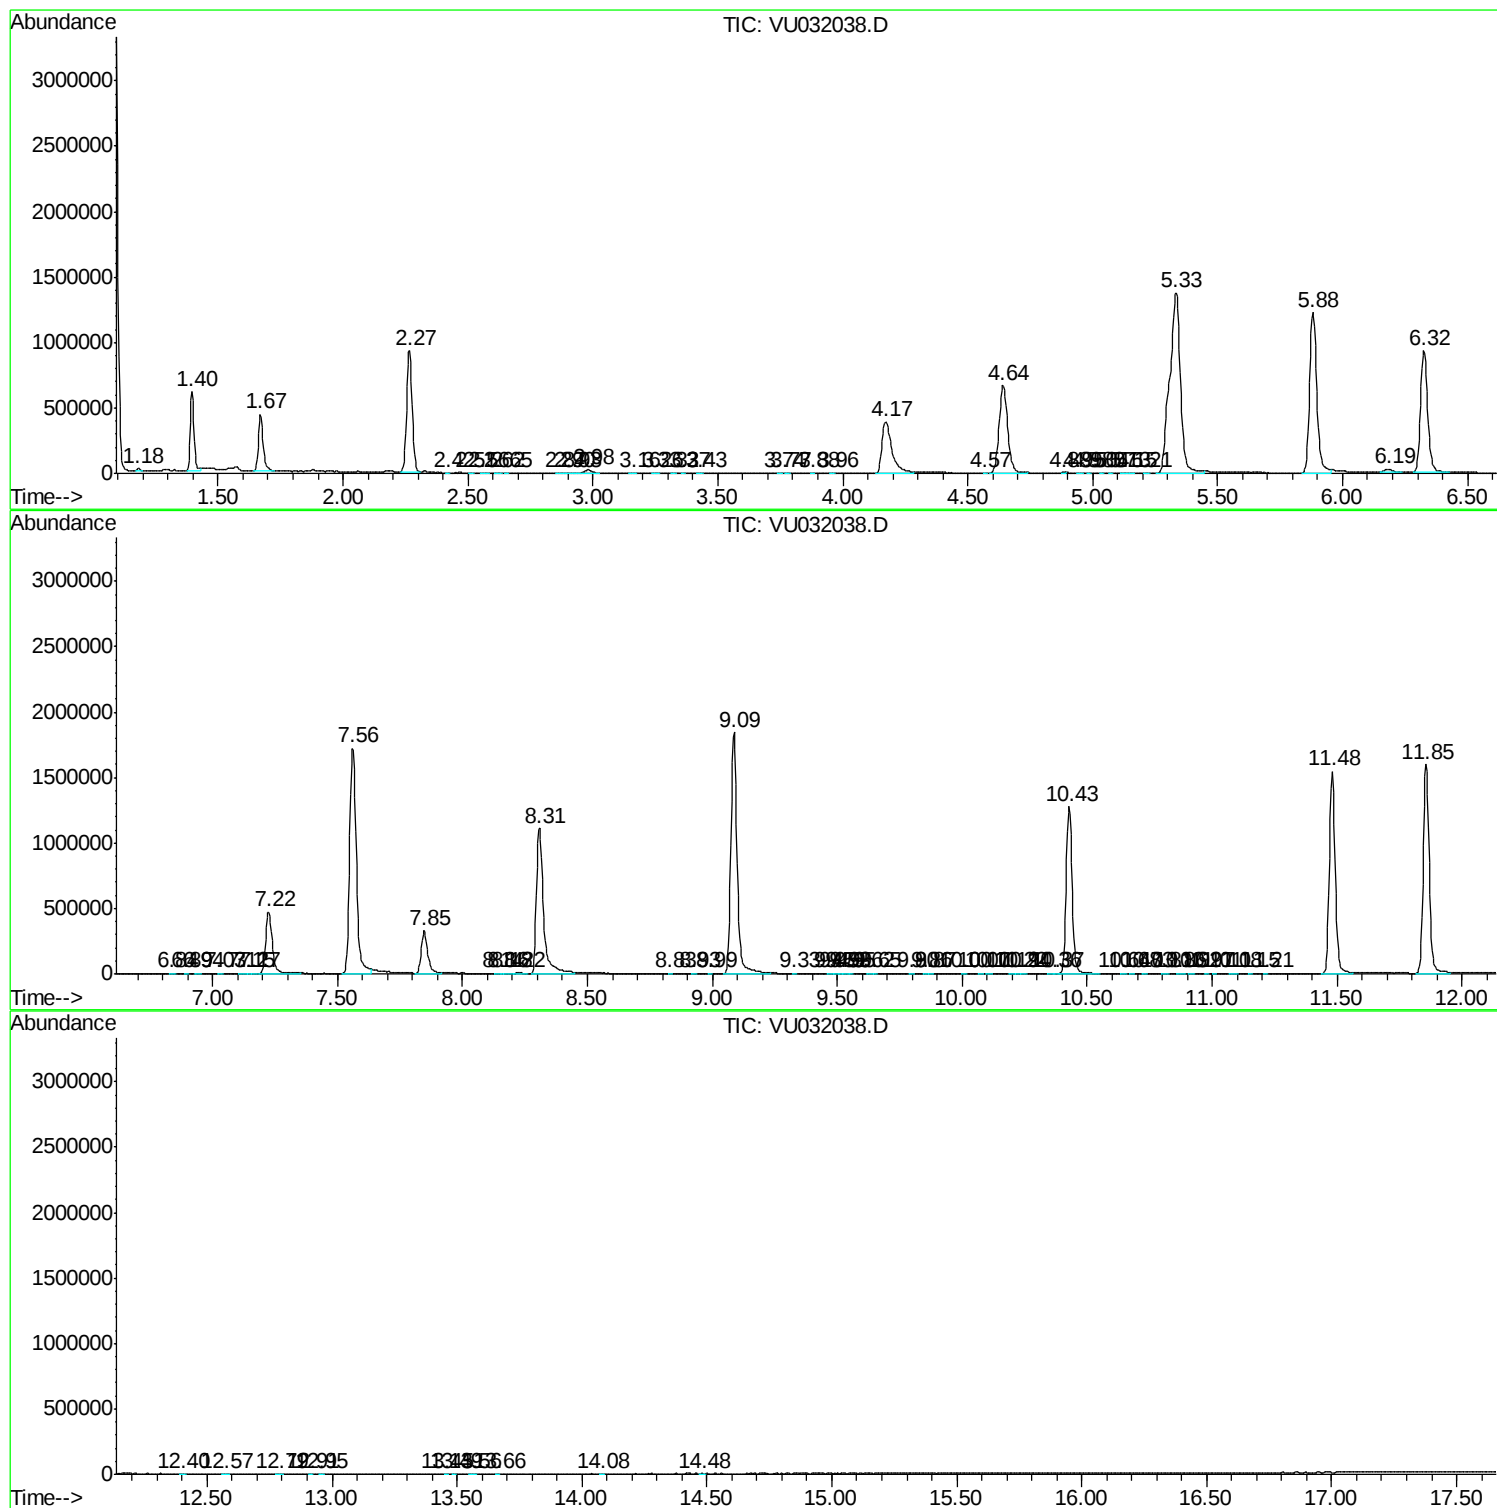

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032038.D
Acq On : 15 May 2019 17:44
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU051519\
Data File : VU032038.D
Acq On : 15 May 2019 17:44
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc